

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024803.D
 Acq On : 07 Apr 2023 09:39
 Operator : CG/JU
 Sample : PB151914BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 07 22:38:31 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	8845	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.758	136	27890	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.593	164	16466	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.338	188	34834	0.400	ng/ul	0.00
17) Chrysene-d12	21.537	240	29035	0.400	ng/ul	0.00
23) Perylene-d12	23.981	264	31404	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	62879	6.926	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.347	152	12819	0.372	ng/ul	0.00
18) Fluoranthene-d10	19.367	212	28996	0.408	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.588	166	4579	0.079	ng/ul#	11
20) Pyrene	19.734	202	4460	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.826	252	10109	0.099	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024803.D
Acq On : 07 Apr 2023 09:39
Operator : CG/JU
Sample : PB151914BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Apr 07 22:38:31 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration

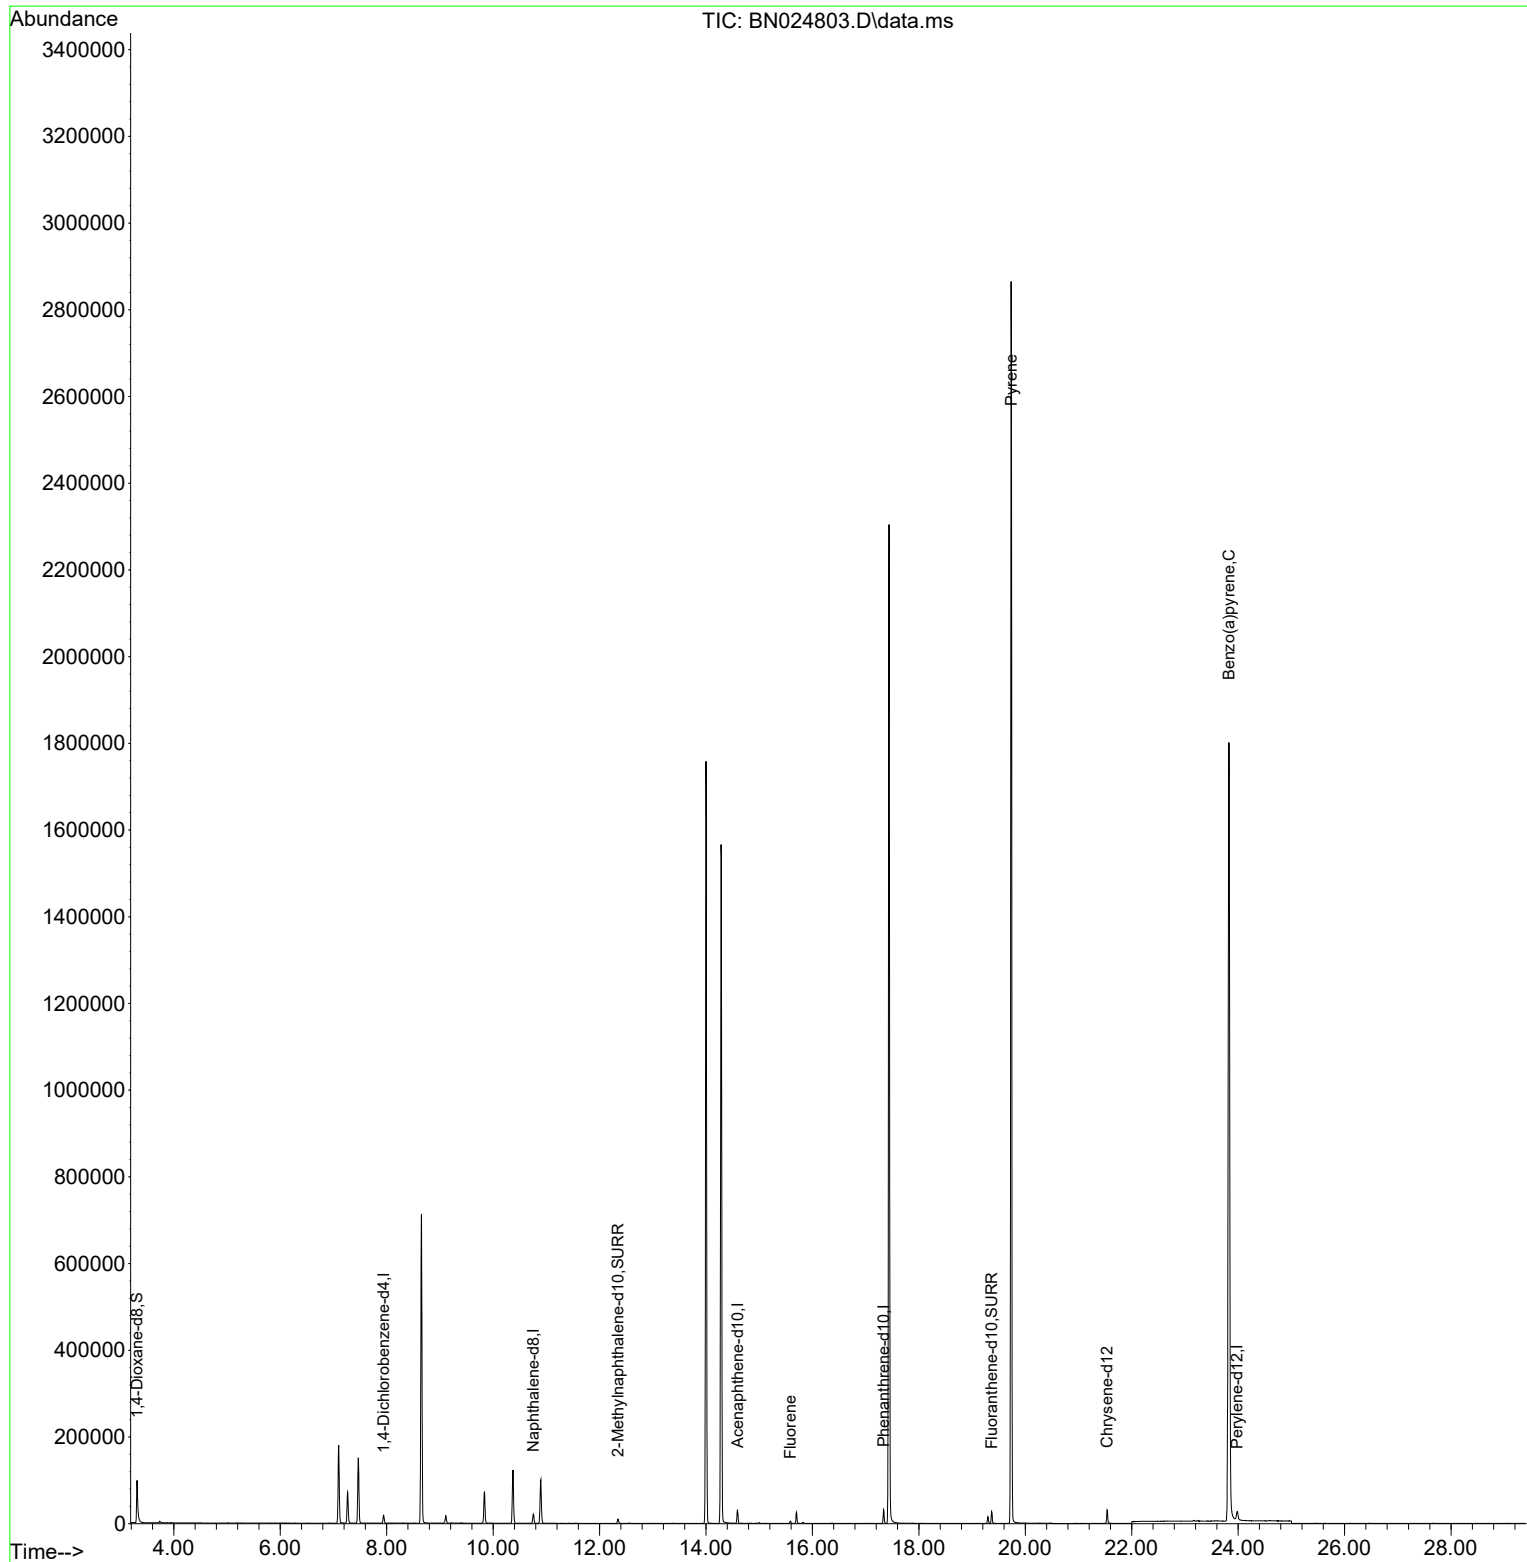



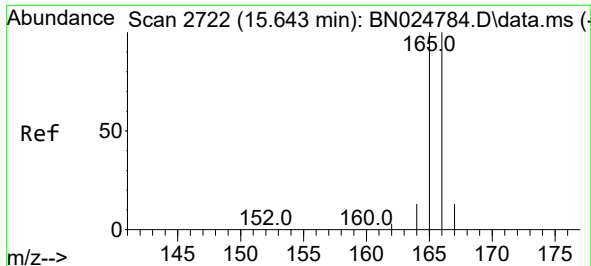


#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.588 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN024803.D
Acq: 07 Apr 2023 09:39

Instrument :
BNA_N
ClientSampleId :



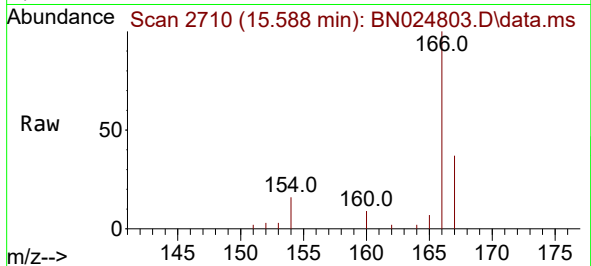



Tgt Ion:166 Resp: 4579
Ion Ratio Lower Upper
166 100
165 7.2 80.0 120.0#
167 37.1 10.8 16.2#

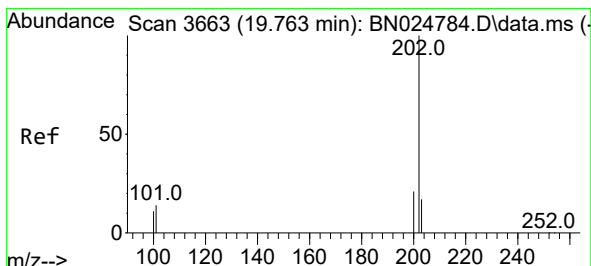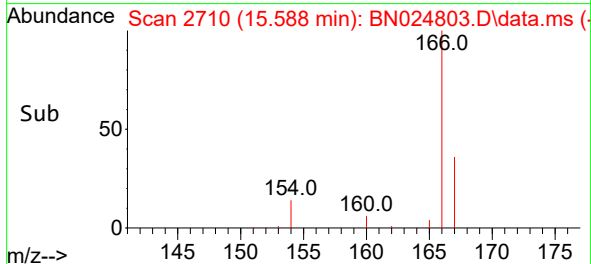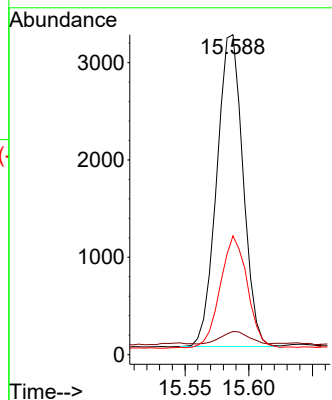

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.734 min Scan# 3657
Delta R.T. -0.029 min
Lab File: BN024803.D
Acq: 07 Apr 2023 09:39

Tgt Ion:202 Resp: 4460
Ion Ratio Lower Upper
202 100
101 180.6 10.9 16.3#
100 1344.8 8.7 13.1#

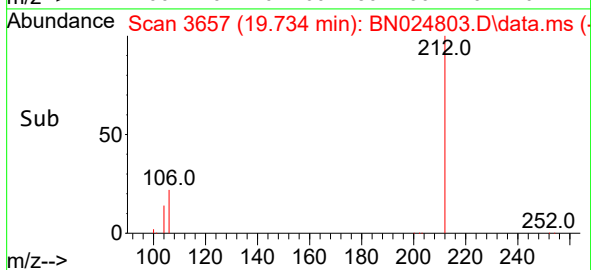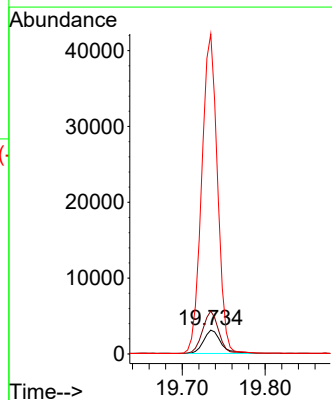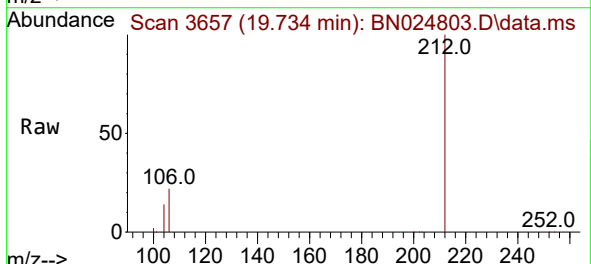

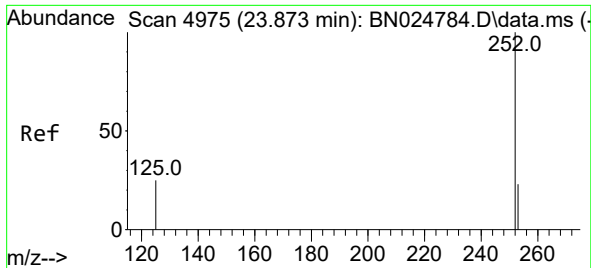

#26

Benzo(a)pyrene

Concen: 0.099 ng/ul

RT: 23.826 min Scan# 49

Delta R.T. -0.048 min


Lab File: BN024803.D

Acq: 07 Apr 2023 09:39

Instrument :

BNA_N

ClientSampleId :

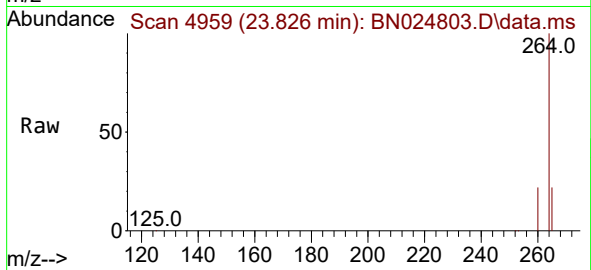

Tgt Ion:252 Resp: 10109

Ion Ratio Lower Upper

252 100

253 43.7 21.8 32.8#

125 38.1 15.4 23.0#

