


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040623\  
Data File : BN024774.D  
Acq On : 06 Apr 2023 10:40  
Operator : CG/JU  
Sample : SSTDC00.4  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SSTD0.4259

Quant Time: Apr 06 22:21:37 2023  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN033023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 06 22:19:46 2023  
Response via : Initial Calibration

Manual Integrations  
APPROVED

Reviewed By : Christian Giraldo 04/07/2023  
Supervised By : mohammad ahmed 04/07/2023

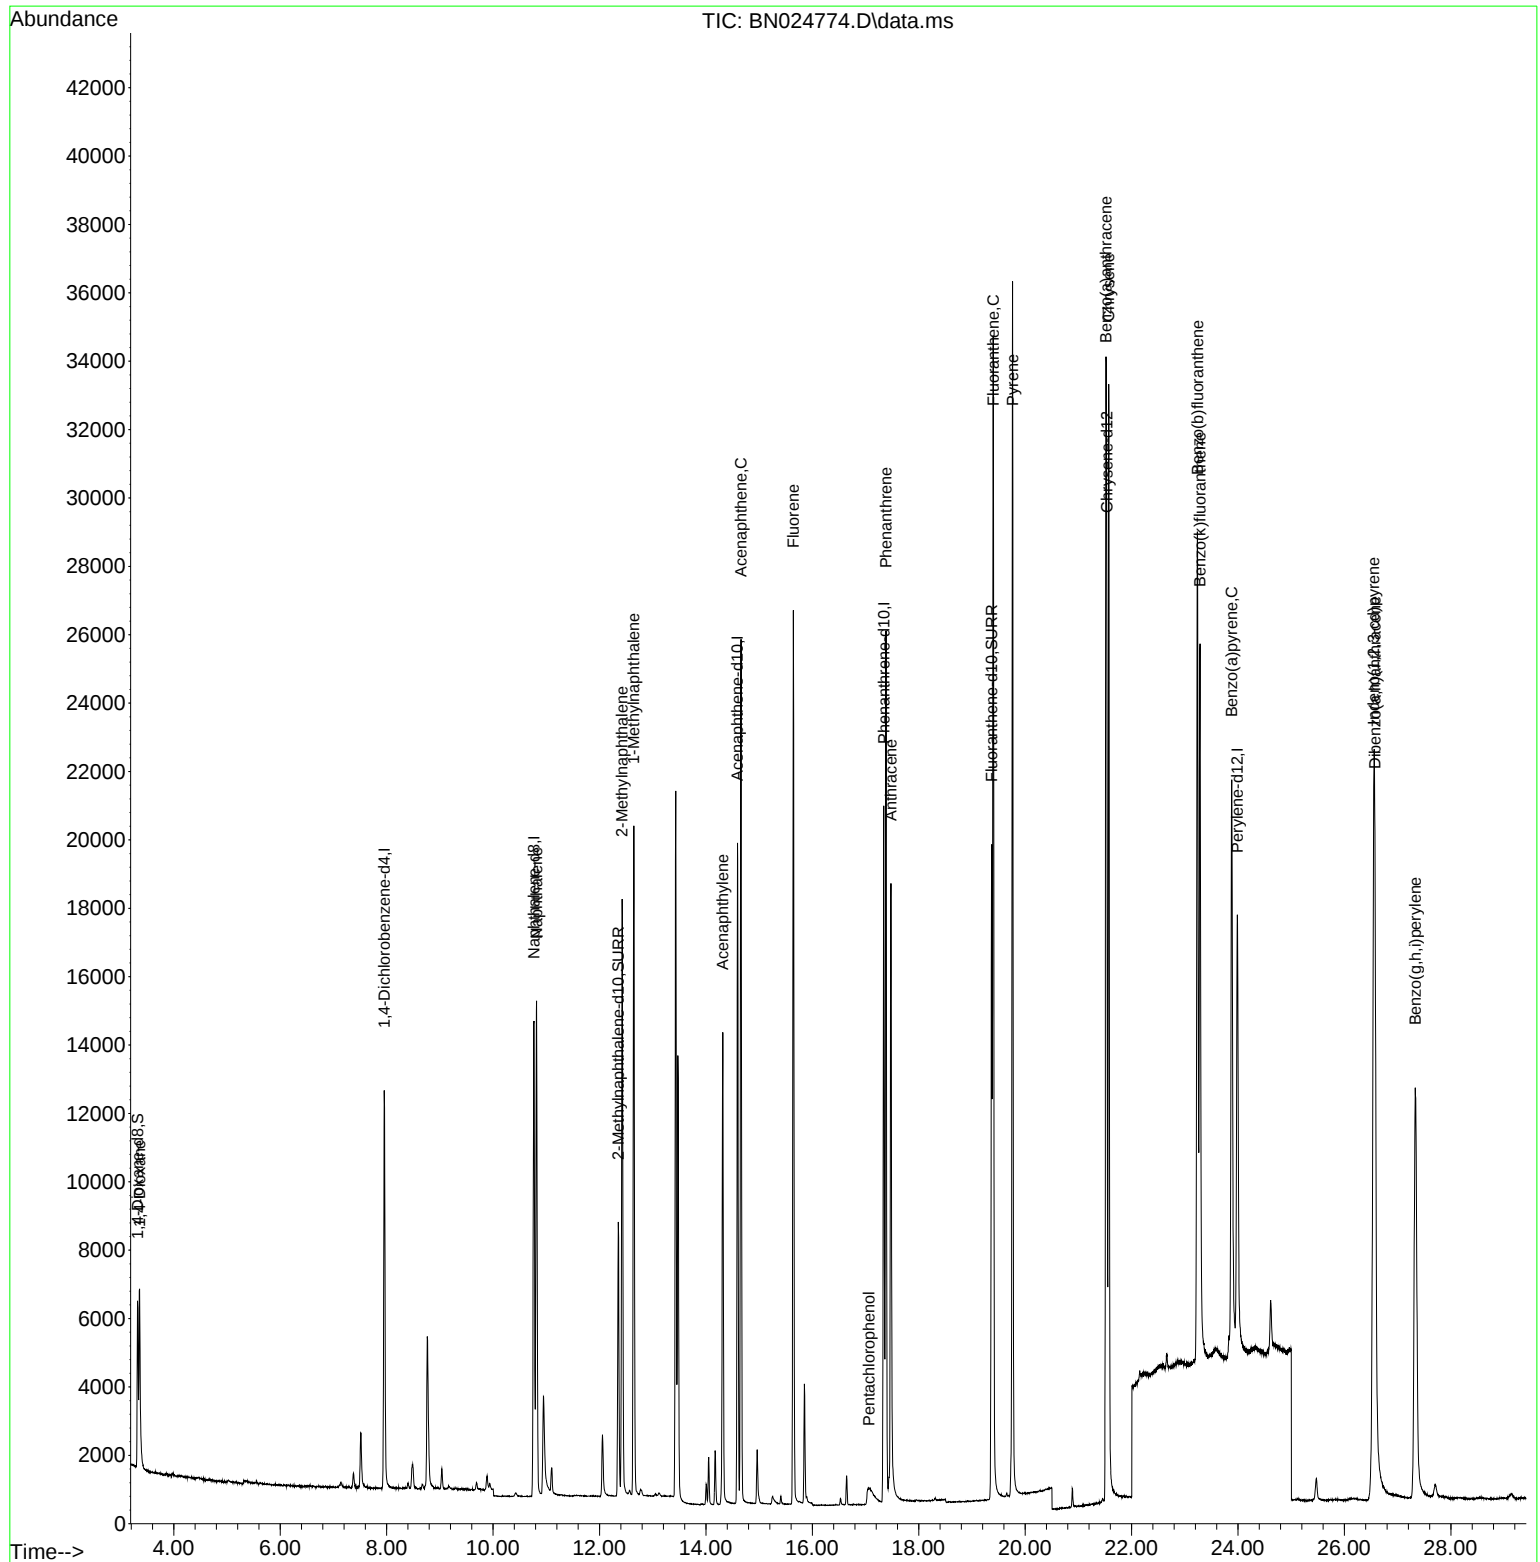

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040623\  
 Data File : BN024774.D  
 Acq On : 06 Apr 2023 10:40  
 Operator : CG/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD0.4259

Manual Integrations  
 APPROVED

Reviewed By : Christian Giraldo 04/07/2023  
 Supervised By : mohammad ahmed 04/07/2023

Quant Time: Apr 06 22:21:37 2023  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN033023.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Apr 06 22:19:46 2023  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.955  | 152  | 6459     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.769 | 136  | 18803    | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.593 | 164  | 10449    | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.342 | 188  | 23011    | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.534 | 240  | 19701    | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.986 | 264  | 18556    | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.318  | 96   | 3052     | 0.460 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.353 | 152  | 10365    | 0.447 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.367 | 212  | 21209    | 0.440 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 2) 1,4-Dioxane              | 3.356  | 88   | 3388     | 0.486 | ng/ul  | 97       |
| 5) Naphthalene              | 10.818 | 128  | 20531    | 0.445 | ng/ul  | 100      |
| 7) 2-Methylnaphthalene      | 12.424 | 142  | 12708    | 0.442 | ng/ul  | 100      |
| 8) 1-Methylnaphthalene      | 12.644 | 142  | 13380    | 0.445 | ng/ul  | 100      |
| 10) Acenaphthylene          | 14.315 | 152  | 16131    | 0.437 | ng/ul  | 100      |
| 11) Acenaphthene            | 14.658 | 153  | 14383    | 0.449 | ng/ul  | 99       |
| 12) Fluorene                | 15.643 | 166  | 16380    | 0.448 | ng/ul  | 99       |
| 14) Pentachlorophenol       | 17.068 | 266  | 1920m    | 0.386 | ng/ul  |          |
| 15) Phenanthrene            | 17.384 | 178  | 26989    | 0.428 | ng/ul  | 100      |
| 16) Anthracene              | 17.477 | 178  | 21941    | 0.416 | ng/ul  | 100      |
| 19) Fluoranthene            | 19.400 | 202  | 29419    | 0.424 | ng/ul  | 99       |
| 20) Pyrene                  | 19.762 | 202  | 29995    | 0.424 | ng/ul  | 98       |
| 21) Benzo(a)anthracene      | 21.516 | 228  | 26445    | 0.447 | ng/ul  | 99       |
| 22) Chrysene                | 21.569 | 228  | 29241    | 0.449 | ng/ul  | 100      |
| 24) Benzo(b)fluoranthene    | 23.238 | 252  | 31450    | 0.408 | ng/ul  | 99       |
| 25) Benzo(k)fluoranthene    | 23.282 | 252  | 30155    | 0.407 | ng/ul  | 98       |
| 26) Benzo(a)pyrene          | 23.881 | 252  | 26477    | 0.437 | ng/ul# | 94       |
| 27) Indeno(1,2,3-cd)pyrene  | 26.550 | 276  | 33889    | 0.469 | ng/ul# | 99       |
| 28) Dibenzo(a,h)anthracene  | 26.573 | 278  | 26188    | 0.453 | ng/ul  | 99       |
| 29) Benzo(g,h,i)perylene    | 27.331 | 276  | 28489    | 0.459 | ng/ul  | 100      |

(#) = qualifier out of range (m) = manual integration (+) = signals summed






Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040623\  
 Data File : BN024774.D  
 Acq On : 06 Apr 2023 10:40  
 Operator : CG/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD0.4259

Manual Integrations  
 APPROVED

Reviewed By : Christian Giraldo 04/07/2023  
 Supervised By : mohammad ahmed 04/07/2023

Quant Time: Apr 06 22:21:37 2023  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN033023.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Apr 06 22:19:46 2023  
 Response via : Initial Calibration

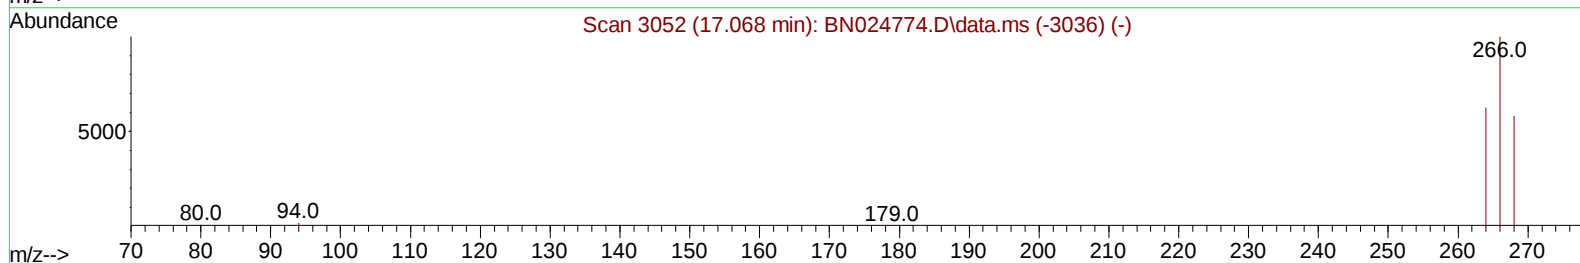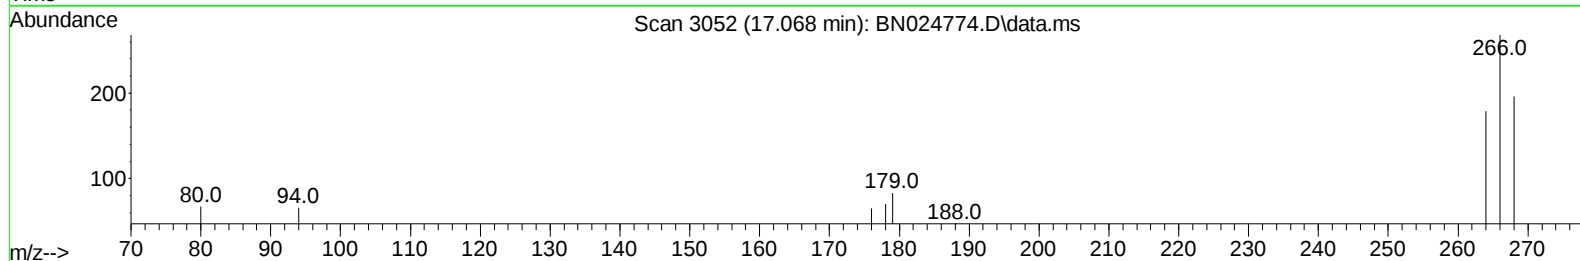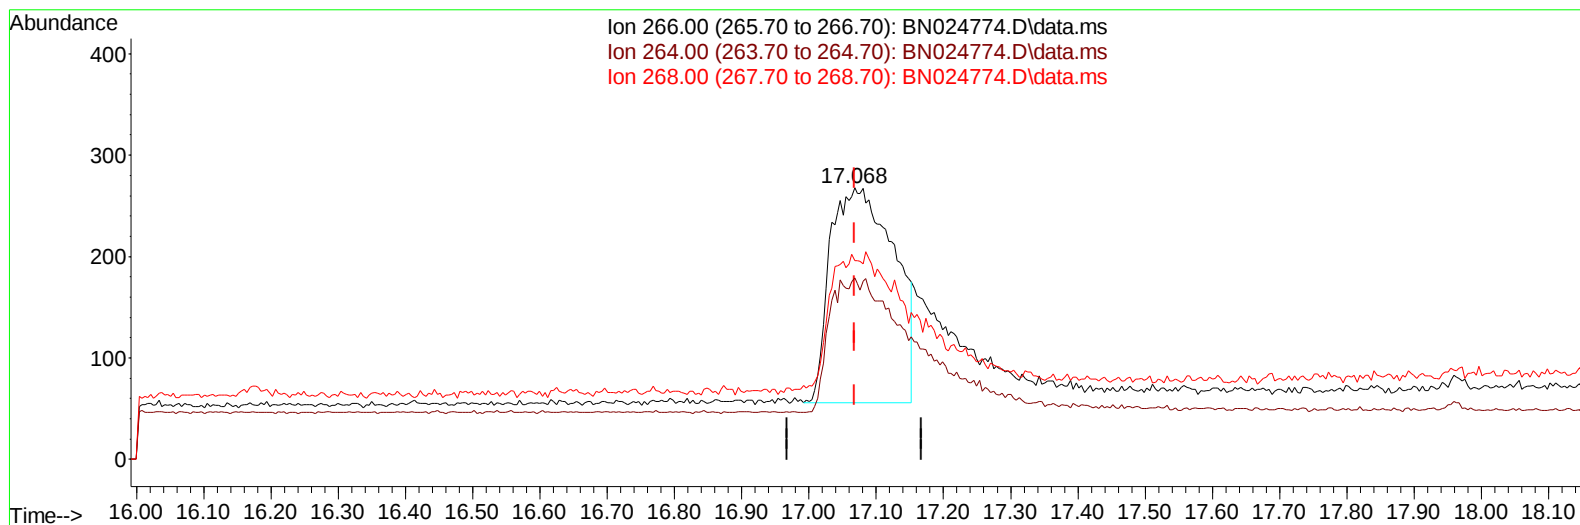

TIC: BN024774.D\data.ms

(14) Pentachloropheno1

17.068min ( 0.000) 0.28 ng/u1

response 1398

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 266.00 | 100.00 | 100.00 |
| 264.00 | 62.00  | 60.94  |
| 268.00 | 65.70  | 61.73  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040623\  
Data File : BN024774.D  
Acq On : 06 Apr 2023 10:40  
Operator : CG/JU  
Sample : SSTDCCC0.4  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
SSTD0.4259

Manual Integrations  
APPROVED

Reviewed By : Christian Giraldo 04/07/2023  
Supervised By : mohammad ahmed 04/07/2023

Quant Time: Apr 06 22:21:37 2023  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN033023.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Apr 06 22:19:46 2023  
Response via : Initial Calibration

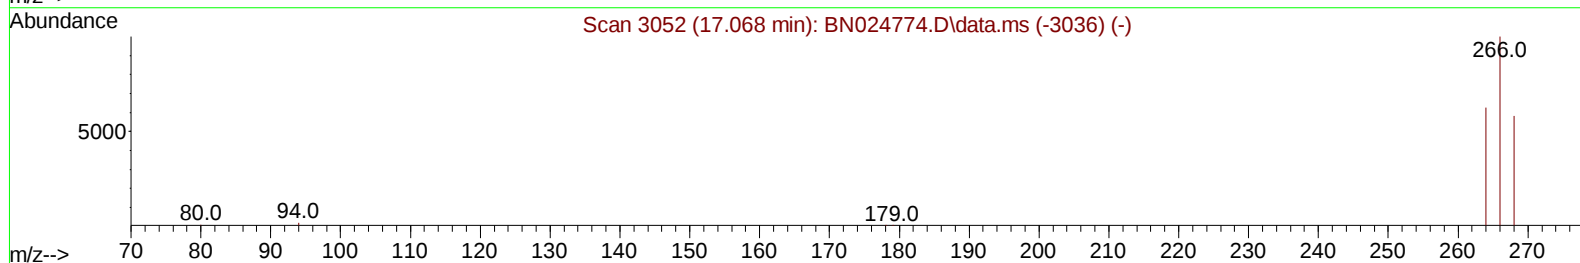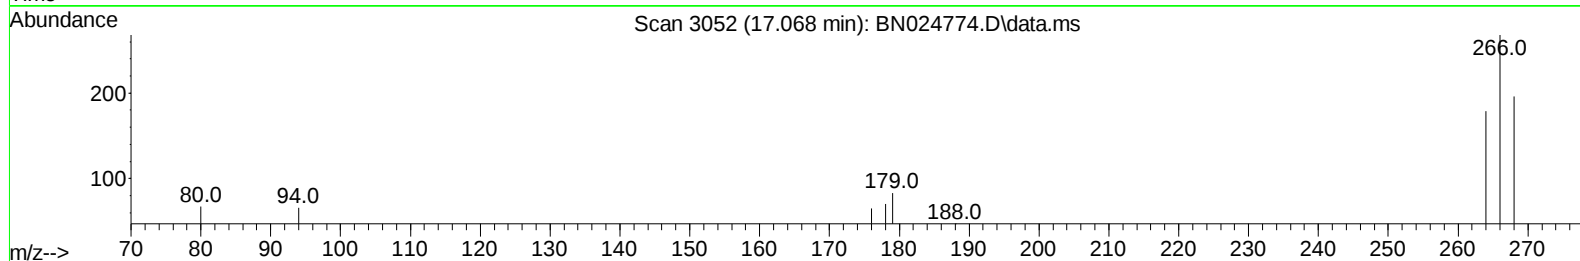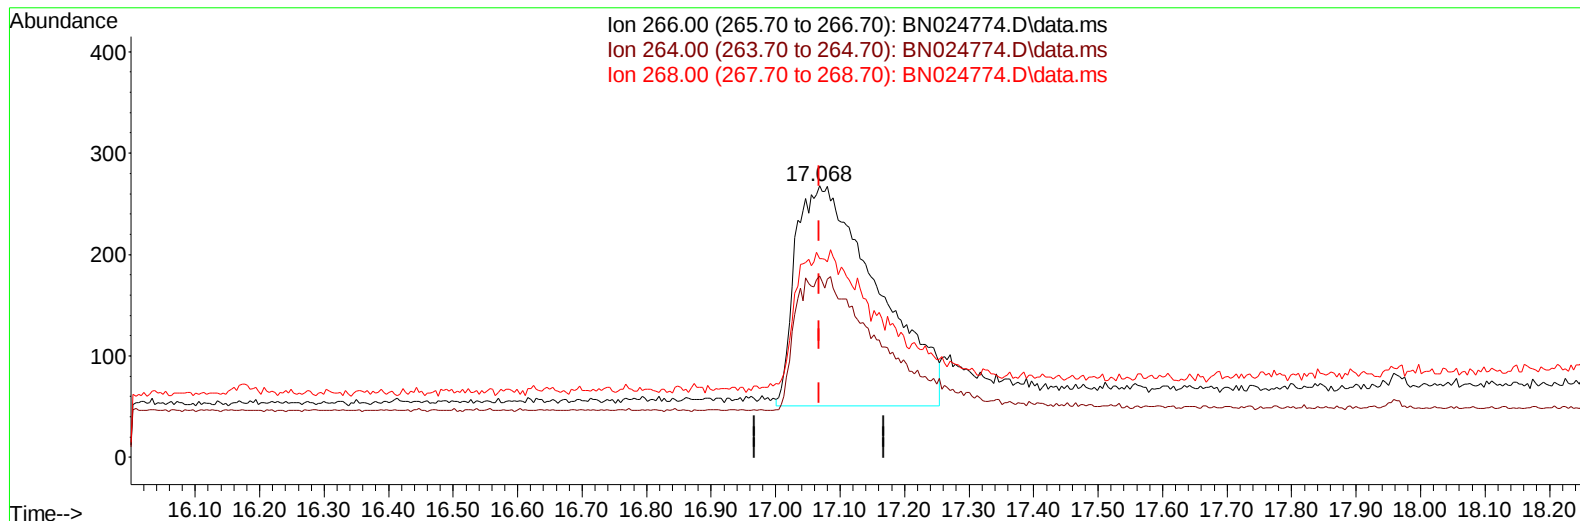

TIC: BN024774.D\data.ms

(14) Pentachloropheno1

17.068min ( 0.000) 0.39 ng/u1 m

response 1920

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 266.00 | 100.00 | 100.00 |
| 264.00 | 62.00  | 44.38# |
| 268.00 | 65.70  | 44.95# |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN040623\  
 Data File : BN024774.D  
 Acq On : 06 Apr 2023 10:40  
 Operator : CG/JU  
 Sample : SSTDCCC0.4  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 SSTD0.4259

Manual Integrations  
 APPROVED

Reviewed By : Christian Giraldo 04/07/2023  
 Supervised By : mohammad ahmed 04/07/2023

Quant Time: Apr 06 22:21:37 2023  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SFAM-EPA-SIM-BN033023.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Apr 06 22:19:46 2023  
 Response via : Initial Calibration

| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.955  | 152  | 6459     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.769 | 136  | 18803    | 0.400 | ng/ul  | 0.00     |
| 9) Acenaphthene-d10         | 14.593 | 164  | 10449    | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.342 | 188  | 23011    | 0.400 | ng/ul  | 0.00     |
| 17) Chrysene-d12            | 21.534 | 240  | 19701    | 0.400 | ng/ul  | 0.00     |
| 23) Perylene-d12            | 23.986 | 264  | 18556    | 0.400 | ng/ul  | 0.00     |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.318  | 96   | 3052     | 0.460 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.353 | 152  | 10365    | 0.447 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.367 | 212  | 21209    | 0.440 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       |        | Qvalue   |
| 2) 1,4-Dioxane              | 3.356  | 88   | 3388     | 0.486 | ng/ul  | 97       |
| 5) Naphthalene              | 10.818 | 128  | 20531    | 0.445 | ng/ul  | 100      |
| 7) 2-Methylnaphthalene      | 12.424 | 142  | 12708    | 0.442 | ng/ul  | 100      |
| 8) 1-Methylnaphthalene      | 12.644 | 142  | 13380    | 0.445 | ng/ul  | 100      |
| 10) Acenaphthylene          | 14.315 | 152  | 16131    | 0.437 | ng/ul  | 100      |
| 11) Acenaphthene            | 14.658 | 153  | 14383    | 0.449 | ng/ul  | 99       |
| 12) Fluorene                | 15.643 | 166  | 16380    | 0.448 | ng/ul  | 99       |
| 14) Pentachlorophenol       | 17.068 | 266  | 1920m    | 0.386 | ng/ul  |          |
| 15) Phenanthrene            | 17.384 | 178  | 26989    | 0.428 | ng/ul  | 100      |
| 16) Anthracene              | 17.477 | 178  | 21941    | 0.416 | ng/ul  | 100      |
| 19) Fluoranthene            | 19.400 | 202  | 29419    | 0.424 | ng/ul  | 99       |
| 20) Pyrene                  | 19.762 | 202  | 29995    | 0.424 | ng/ul  | 98       |
| 21) Benzo(a)anthracene      | 21.516 | 228  | 26445    | 0.447 | ng/ul  | 99       |
| 22) Chrysene                | 21.569 | 228  | 29241    | 0.449 | ng/ul  | 100      |
| 24) Benzo(b)fluoranthene    | 23.238 | 252  | 31450    | 0.408 | ng/ul  | 99       |
| 25) Benzo(k)fluoranthene    | 23.282 | 252  | 30155    | 0.407 | ng/ul  | 98       |
| 26) Benzo(a)pyrene          | 23.881 | 252  | 26477    | 0.437 | ng/ul# | 94       |
| 27) Indeno(1,2,3-cd)pyrene  | 26.550 | 276  | 33889    | 0.469 | ng/ul# | 99       |
| 28) Dibenzo(a,h)anthracene  | 26.573 | 278  | 26188    | 0.453 | ng/ul  | 99       |
| 29) Benzo(g,h,i)perylene    | 27.331 | 276  | 28489    | 0.459 | ng/ul  | 100      |
| -----                       |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed