

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024783.D
 Acq On : 06 Apr 2023 16:12
 Operator : CG/JU
 Sample : 02122-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB9B8

Quant Time: Apr 06 22:59:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	7708	0.400	ng/u1	0.00
4) Naphthalene-d8	10.765	136	24612	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.598	164	14852	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.343	188	31784	0.400	ng/u1	0.00
17) Chrysene-d12	21.529	240	25899	0.400	ng/u1	0.00
23) Perylene-d12	23.970	264	30277	0.400	ng/u1	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	43914	5.551	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.354	152	13530	0.445	ng/u1	0.00
18) Fluoranthene-d10	19.368	212	34468	0.544	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	16.992	266	4056	0.590	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024783.D
Acq On : 06 Apr 2023 16:12
Operator : CG/JU
Sample : 02122-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB9B8

Quant Time: Apr 06 22:59:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration

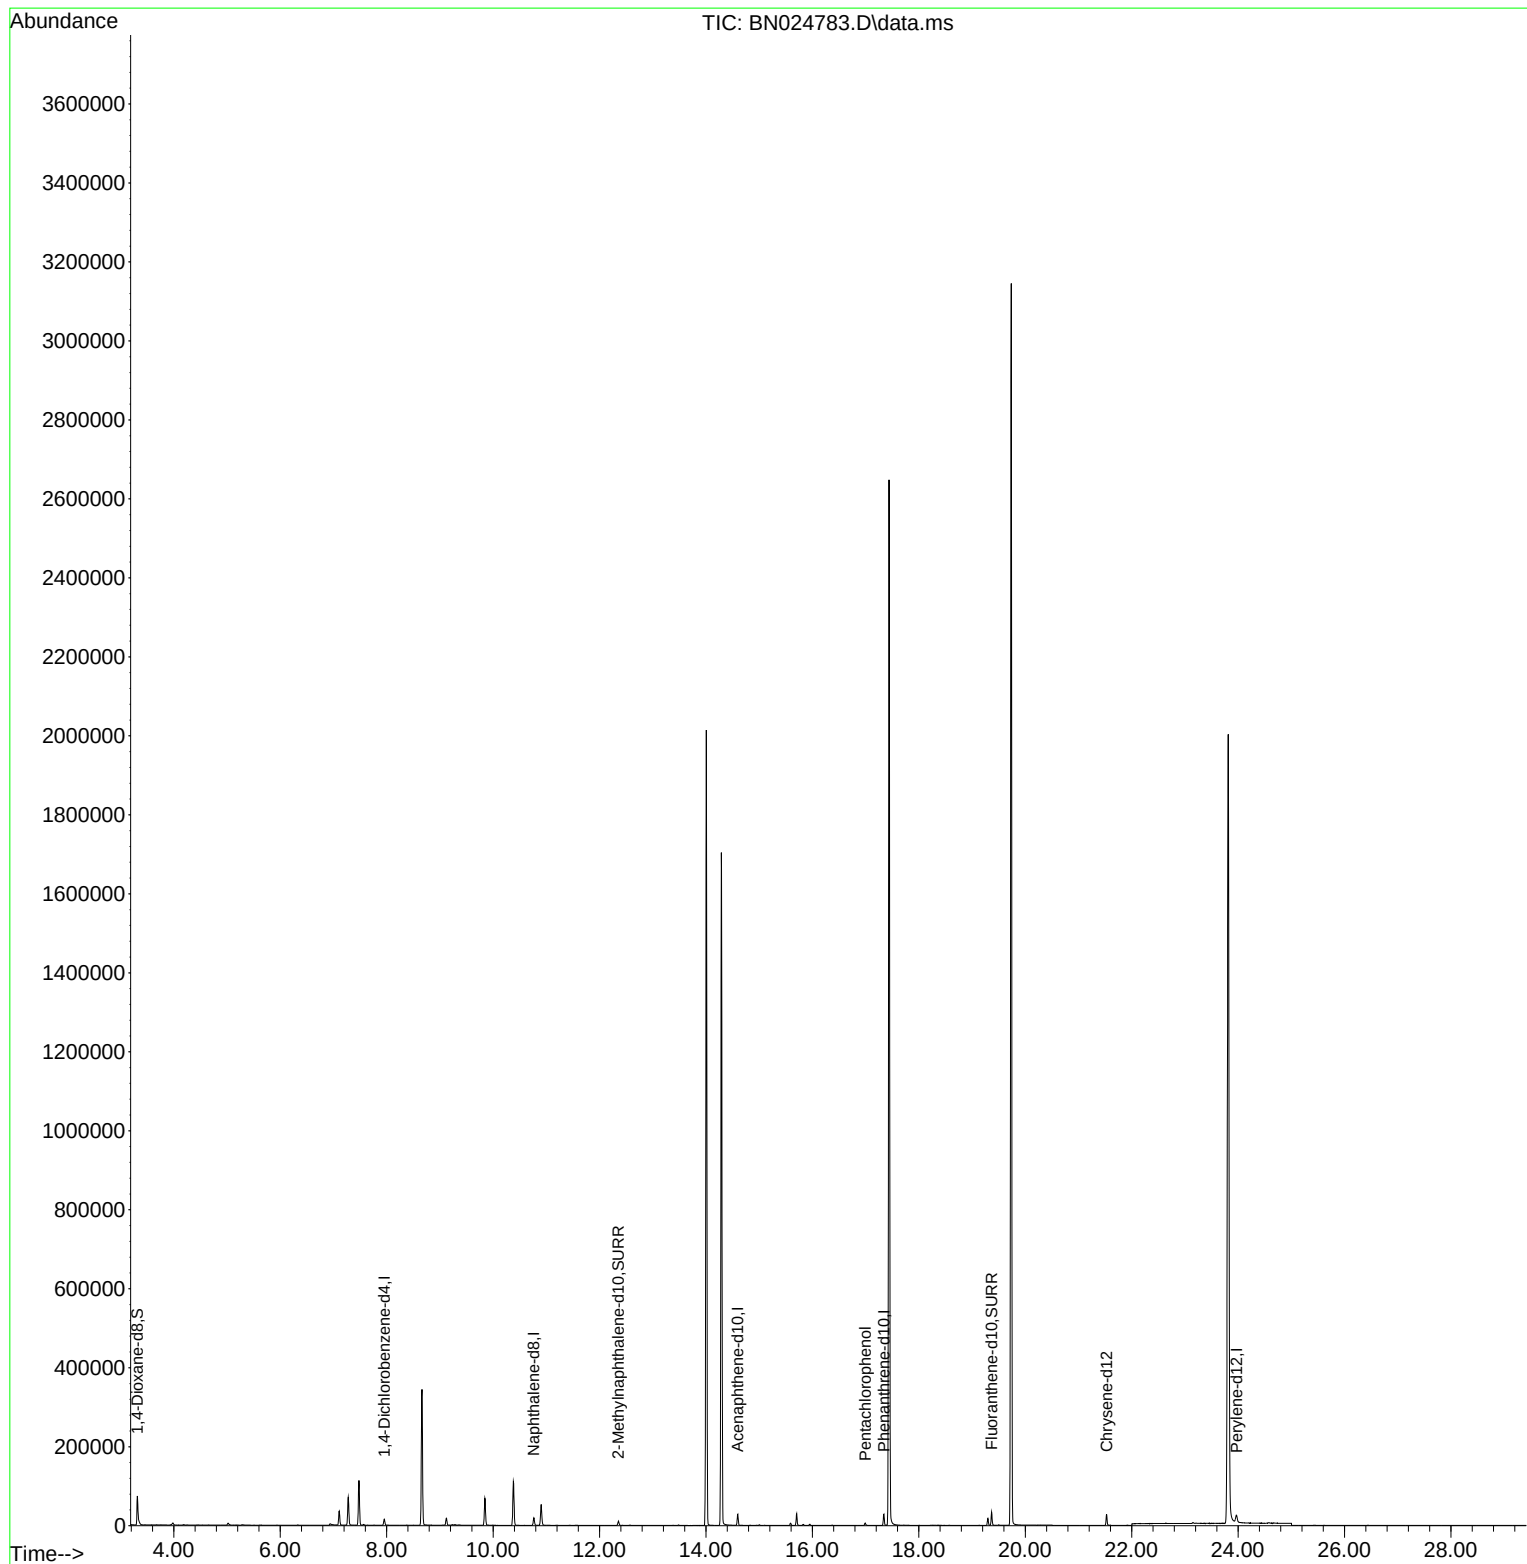

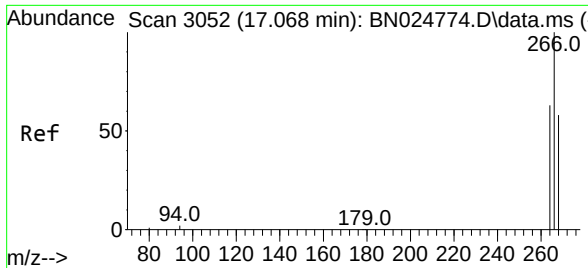

#14

Pentachlorophenol

Concen: 0.590 ng/ul

RT: 16.992 min Scan# 30

Delta R.T. -0.004 min

Lab File: BN024783.D


Acq: 06 Apr 2023 16:12

Instrument :

BNA_N

ClientSampleId :

CB9B8

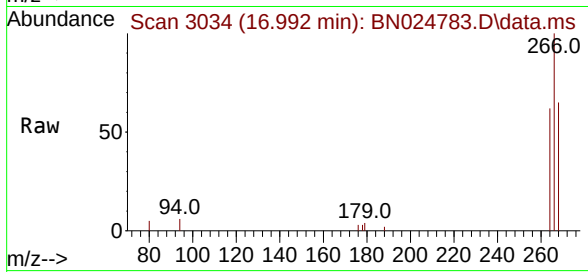

Tgt Ion:266 Resp: 4056

Ion Ratio Lower Upper

266 100

264 62.8 49.6 74.4

268 63.7 52.6 78.8

