

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024790.D
 Acq On : 06 Apr 2023 21:12
 Operator : CG/JU
 Sample : 02093-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB966

Quant Time: Apr 06 23:08:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	8317	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	26831	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.594	164	15831	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.343	188	35435	0.400	ng/ul	0.00
17) Chrysene-d12	21.527	240	30421	0.400	ng/ul	0.00
23) Perylene-d12	23.968	264	34213	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	45422	5.321	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	15337	0.463	ng/ul	0.00
18) Fluoranthene-d10	19.369	212	40535	0.544	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.356	88	966	0.108	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024790.D
Acq On : 06 Apr 2023 21:12
Operator : CG/JU
Sample : 02093-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB966


Quant Time: Apr 06 23:08:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration

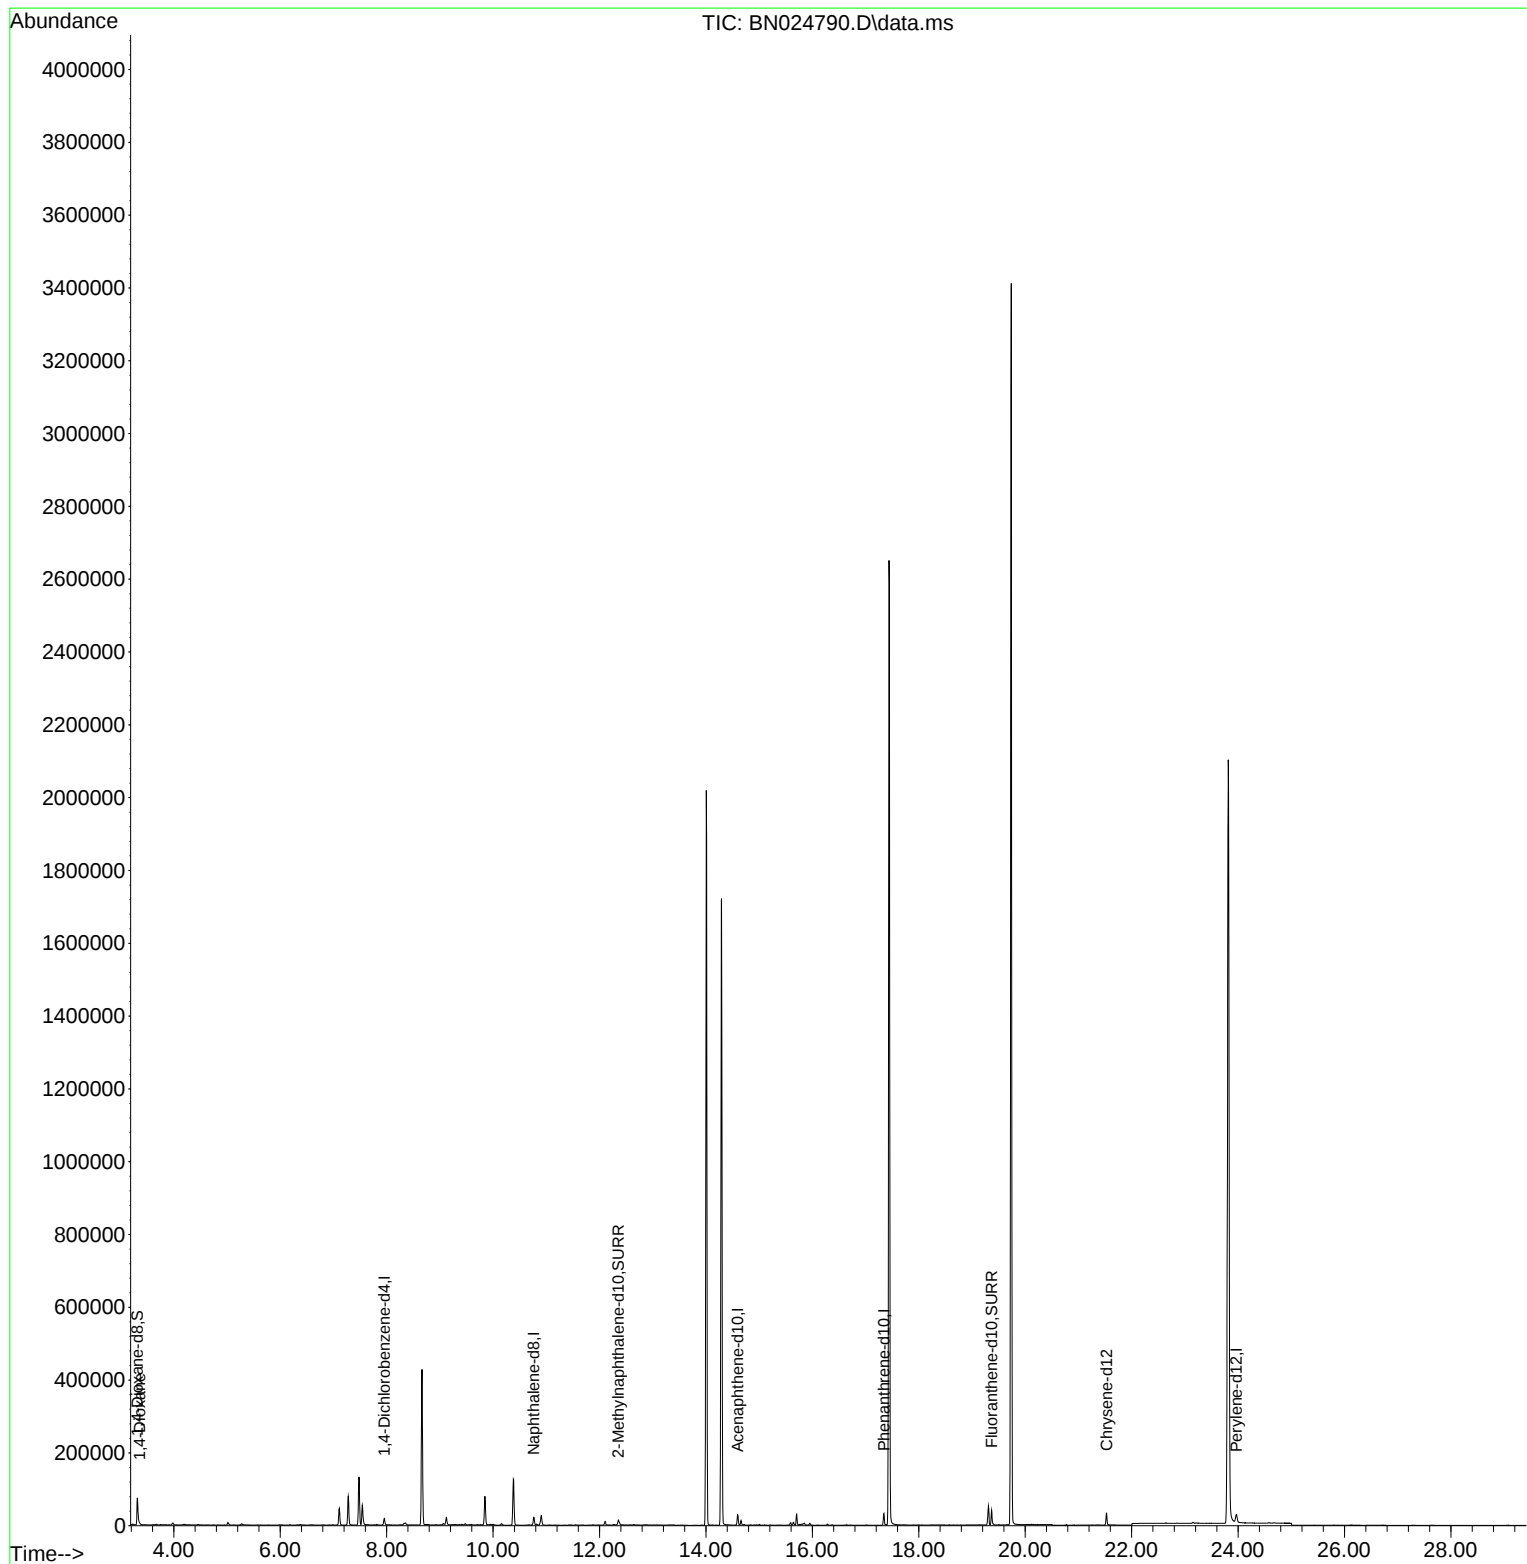

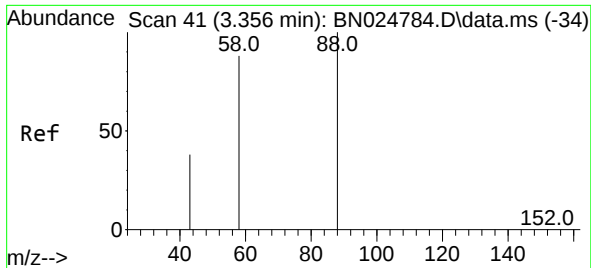

#2
 1,4-Dioxane
 Concen: 0.108 ng/ul
 RT: 3.356 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN024790.D
 Acq: 06 Apr 2023 21:12

Instrument :
 BNA_N
 ClientSampleId :
 CB966

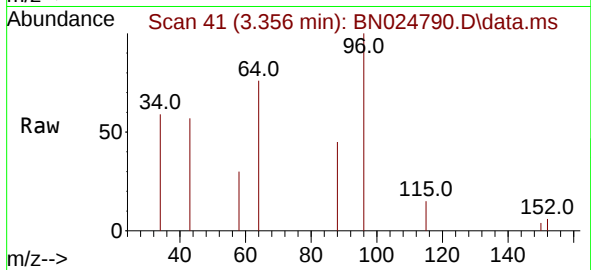

Tgt Ion:	88	Resp:	966
Ion	Ratio	Lower	Upper
88	100		
43	127.6	37.2	55.8#
58	67.8	61.5	92.3

