

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024798.D
 Acq On : 07 Apr 2023 02:08
 Operator : CG/JU
 Sample : 02194-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDW3

Quant Time: Apr 07 03:16:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.955	152	9085	0.400	ng/ul	0.00
4) Naphthalene-d8	10.765	136	28244	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.593	164	17184	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.343	188	38130	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	30622	0.400	ng/ul	0.00
23) Perylene-d12	23.970	264	33088	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	40707	4.365	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	11834	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	31652	0.422	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.356	88	2229	0.227	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024798.D
Acq On : 07 Apr 2023 02:08
Operator : CG/JU
Sample : 02194-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDW3


Quant Time: Apr 07 03:16:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration

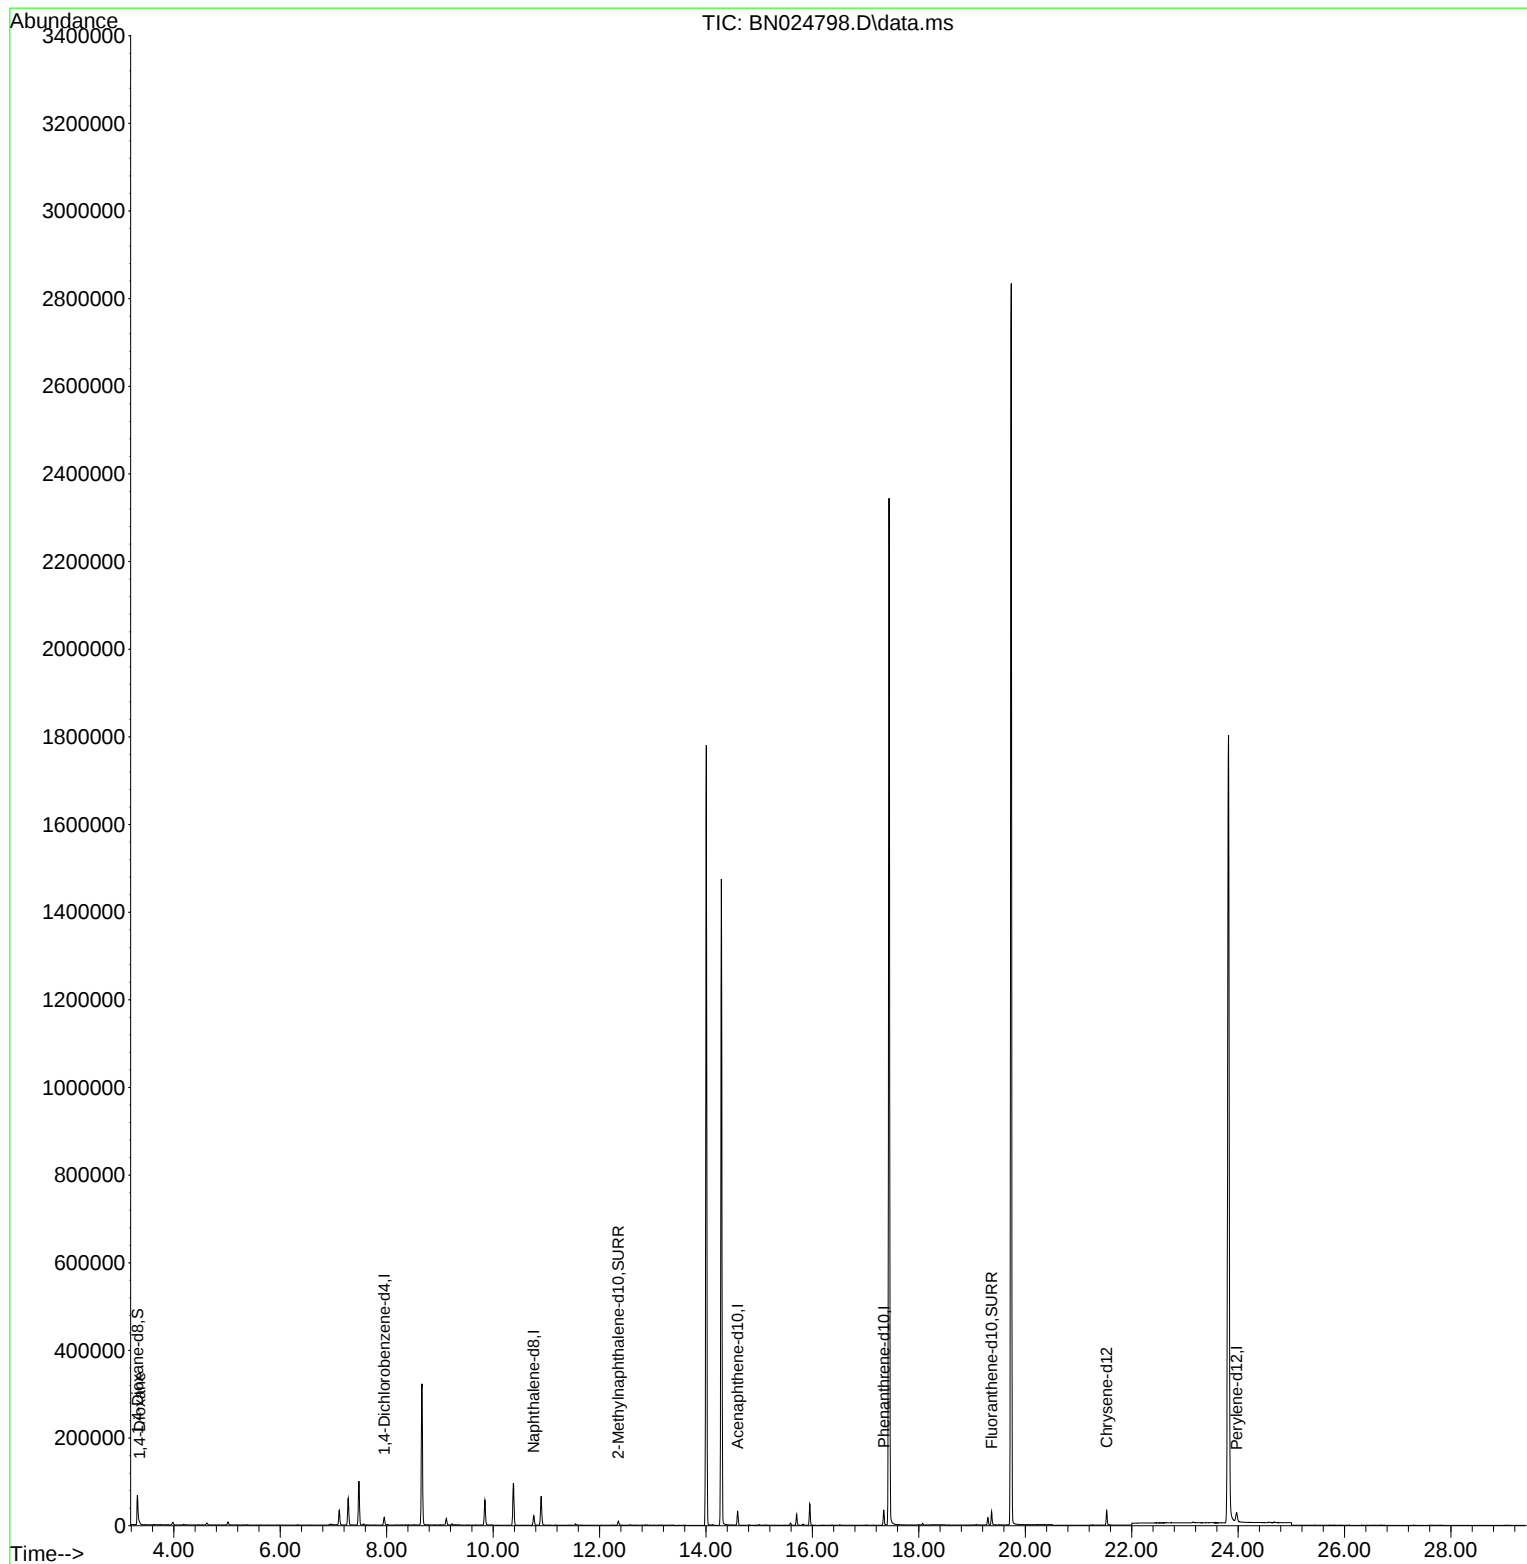

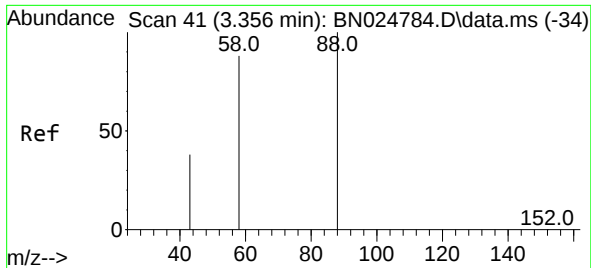

#2
 1,4-Dioxane
 Concen: 0.227 ng/ul
 RT: 3.356 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BN024798.D
 Acq: 07 Apr 2023 02:08

Instrument :
 BNA_N
 ClientSampleId :
 BHDW3

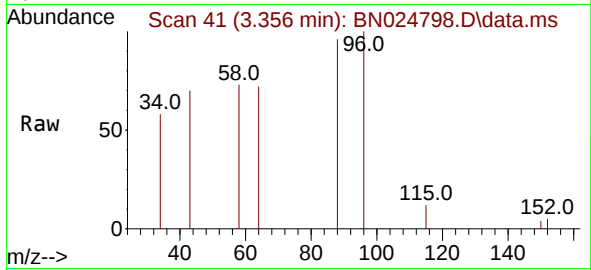

Tgt Ion:	88	Resp:	2229
Ion	Ratio	Lower	Upper
88	100		
43	72.9	37.2	55.8#
58	75.6	61.5	92.3

