

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024805.D
 Acq On : 07 Apr 2023 10:51
 Operator : CG/JU
 Sample : 02194-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDW6

Quant Time: Apr 07 22:38:51 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	10767	0.400	ng/ul	0.00
4) Naphthalene-d8	10.763	136	35651	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.592	164	20871	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.342	188	43570	0.400	ng/ul	0.00
17) Chrysene-d12	21.533	240	35453	0.400	ng/ul	0.00
23) Perylene-d12	23.989	264	38575	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	62016	5.612	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.347	152	18682	0.425	ng/ul	0.00
18) Fluoranthene-d10	19.367	212	44750	0.516	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.356	88	1361	0.117	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024805.D
Acq On : 07 Apr 2023 10:51
Operator : CG/JU
Sample : 02194-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDW6


Quant Time: Apr 07 22:38:51 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration

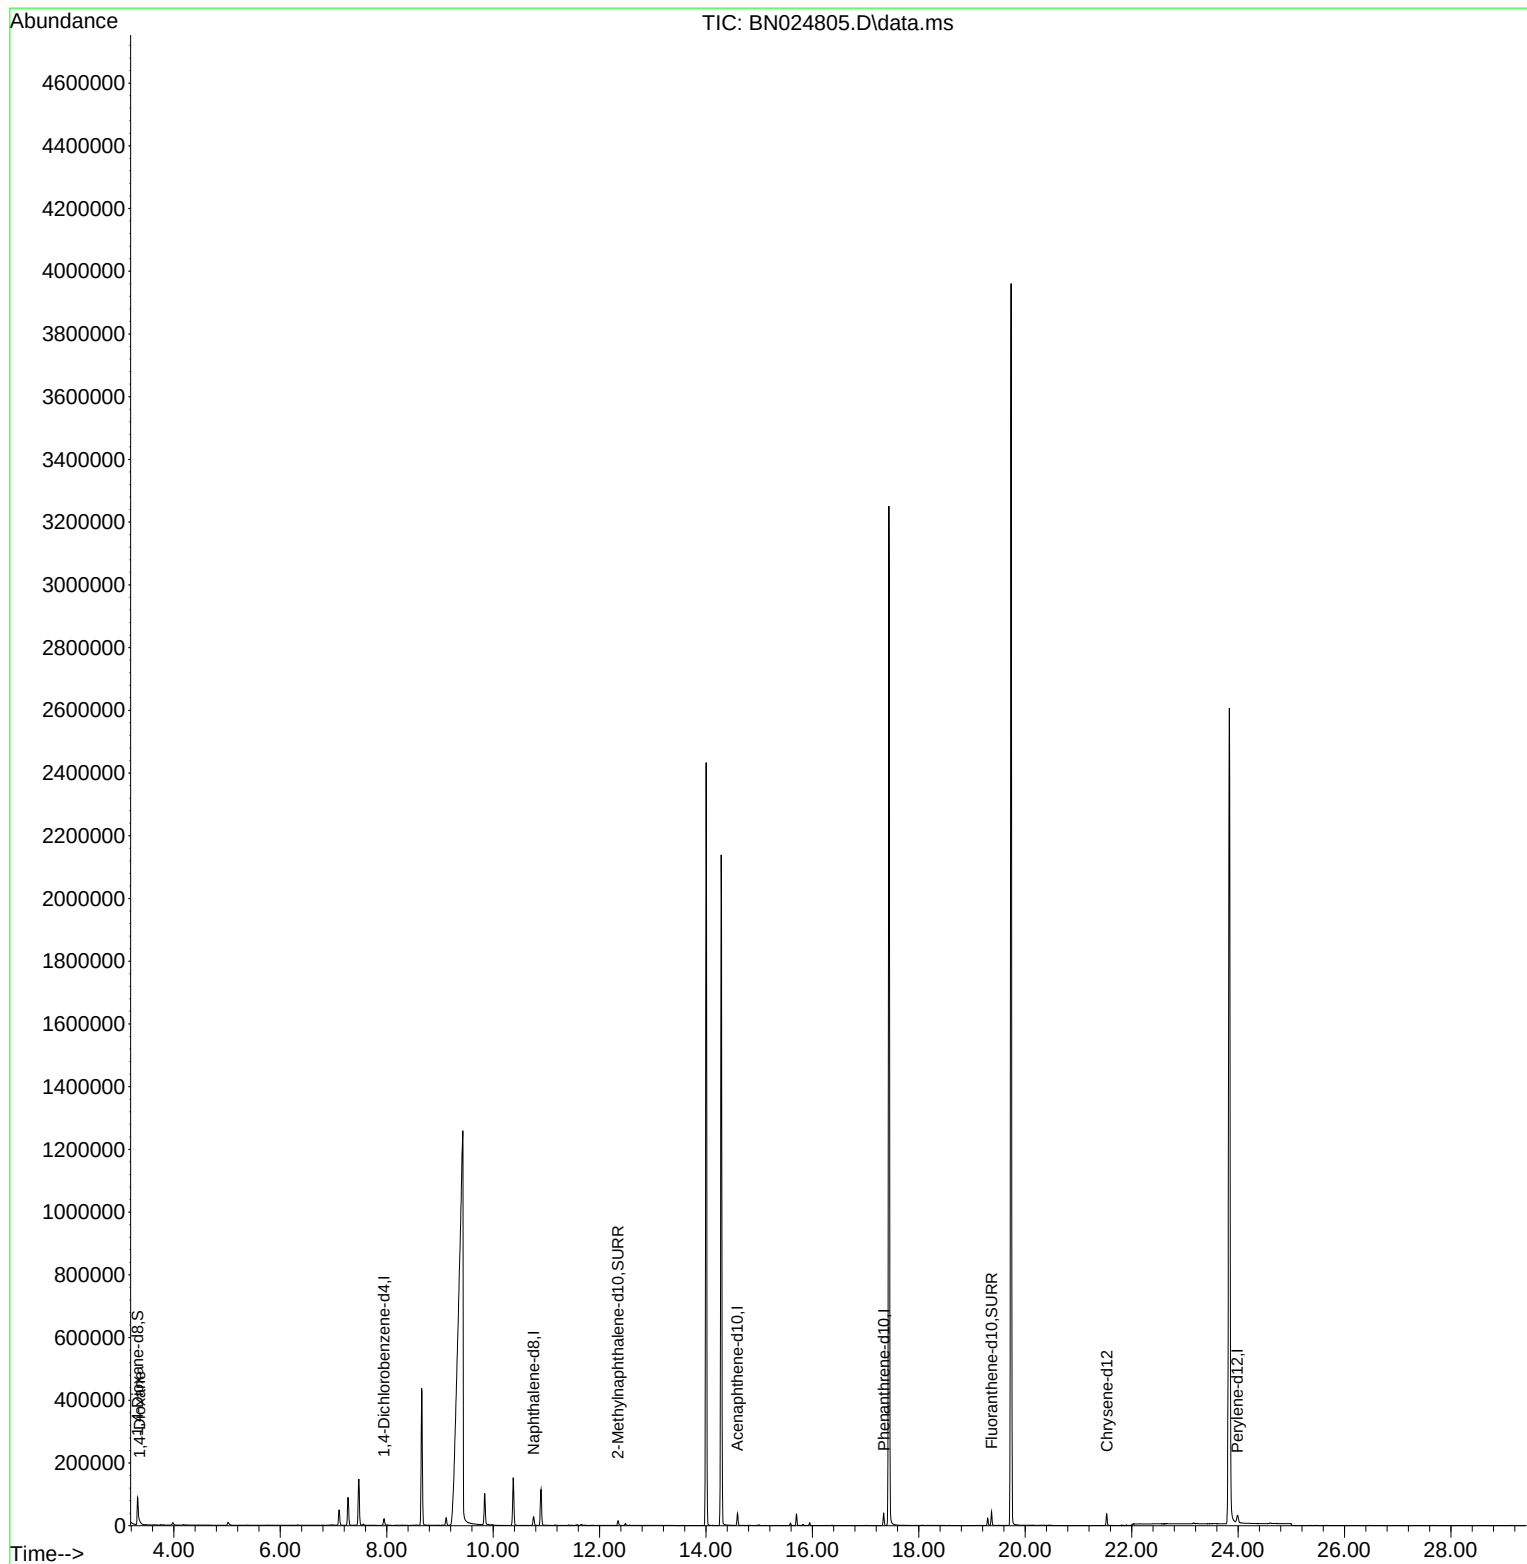

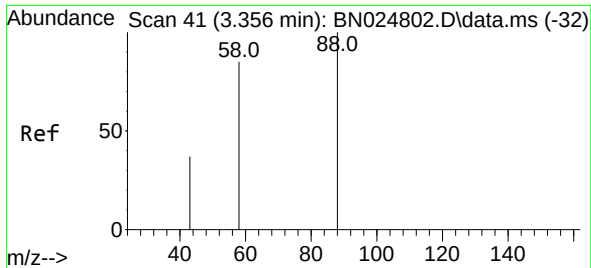

#2
 1,4-Dioxane
 Concen: 0.117 ng/ul
 RT: 3.356 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: BN024805.D
 Acq: 07 Apr 2023 10:51

Instrument :
 BNA_N
 ClientSampleId :
 BHDW6

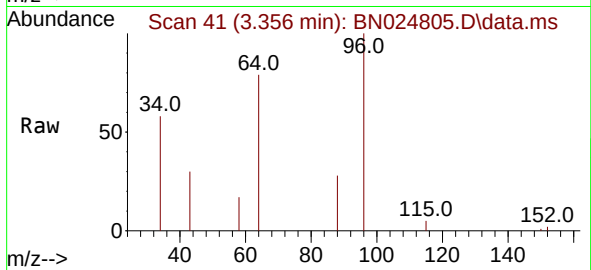

Tgt Ion: 88 Resp: 1361

Ion	Ratio	Lower	Upper
88	100		
43	107.3	37.2	55.8#
58	60.6	61.5	92.3#

