

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
 Data File : BN024806.D
 Acq On : 07 Apr 2023 11:27
 Operator : CG/JU
 Sample : 02194-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDW7

Quant Time: Apr 07 22:38:59 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 22:57:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7435	0.400	ng/u1	0.00
4) Naphthalene-d8	10.765	136	23181	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.593	164	14202	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.338	188	31425	0.400	ng/u1	0.00
17) Chrysene-d12	21.532	240	25054	0.400	ng/u1	0.00
23) Perylene-d12	23.984	264	26835	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	43179	5.658	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	12118	0.424	ng/u1	0.00
18) Fluoranthene-d10	19.368	212	33691	0.549	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	16819	2.095	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040623\
Data File : BN024806.D
Acq On : 07 Apr 2023 11:27
Operator : CG/JU
Sample : 02194-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDW7


Quant Time: Apr 07 22:38:59 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 22:57:45 2023
Response via : Initial Calibration

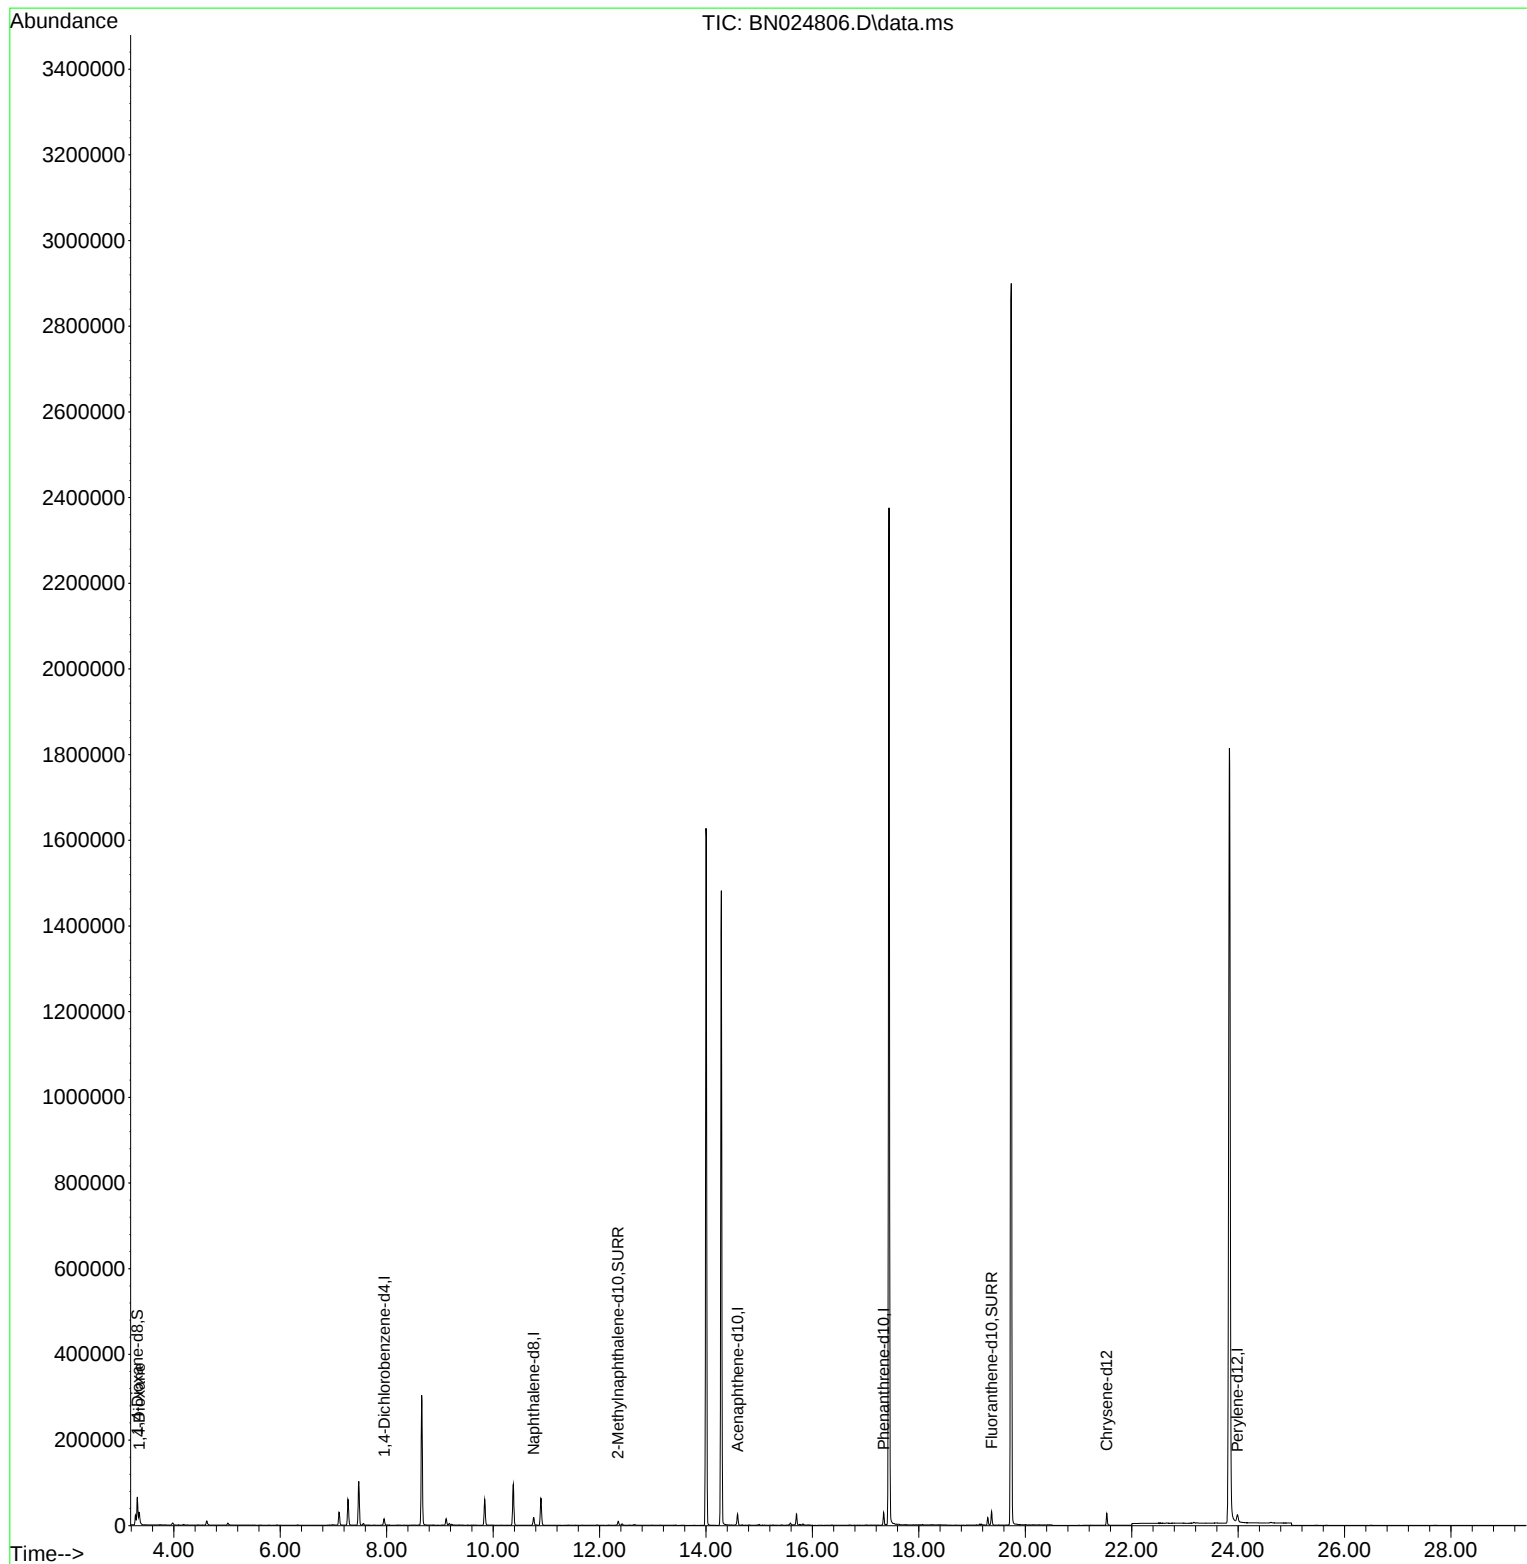

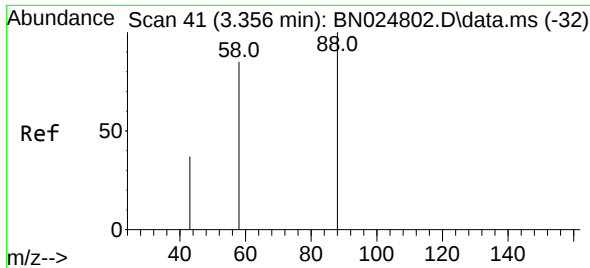

#2
 1,4-Dioxane
 Concen: 2.095 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN024806.D
 Acq: 07 Apr 2023 11:27

Instrument :
 BNA_N
 ClientSampleId :
 BHDW7

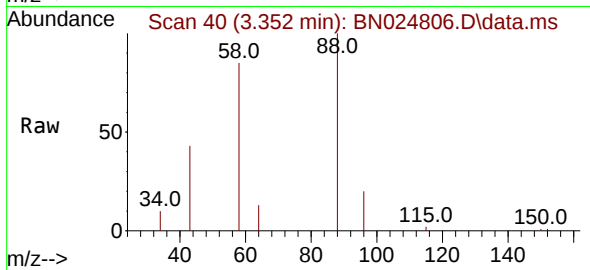

Tgt Ion:	88	Resp:	16819
Ion	Ratio	Lower	Upper
88	100		
43	43.2	37.2	55.8
58	85.1	61.5	92.3

