
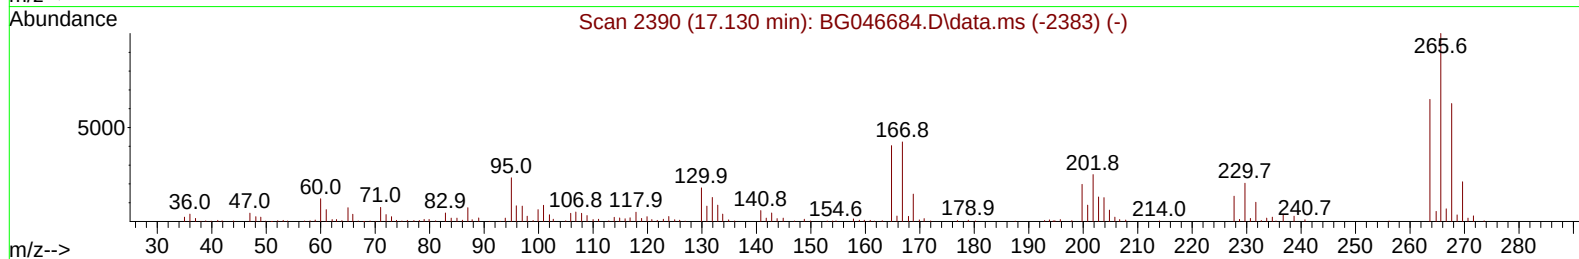
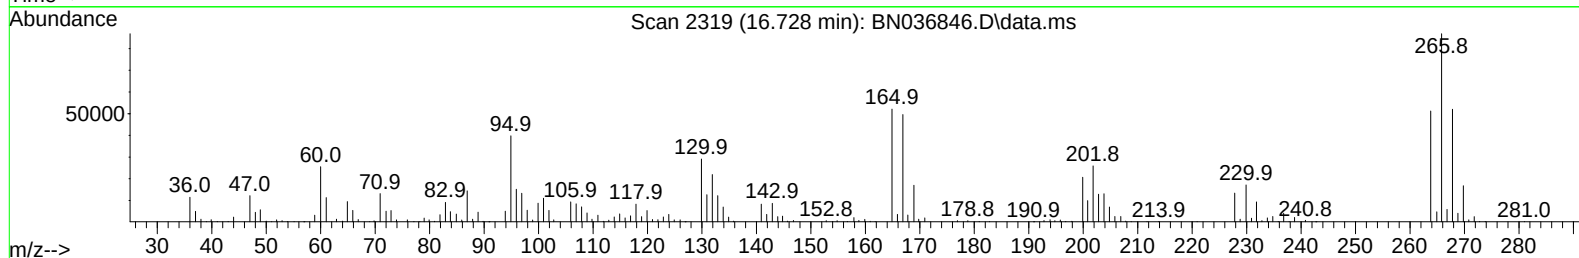


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040725\
Data File : BN036846.D
Acq On : 07 Apr 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 17:29:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

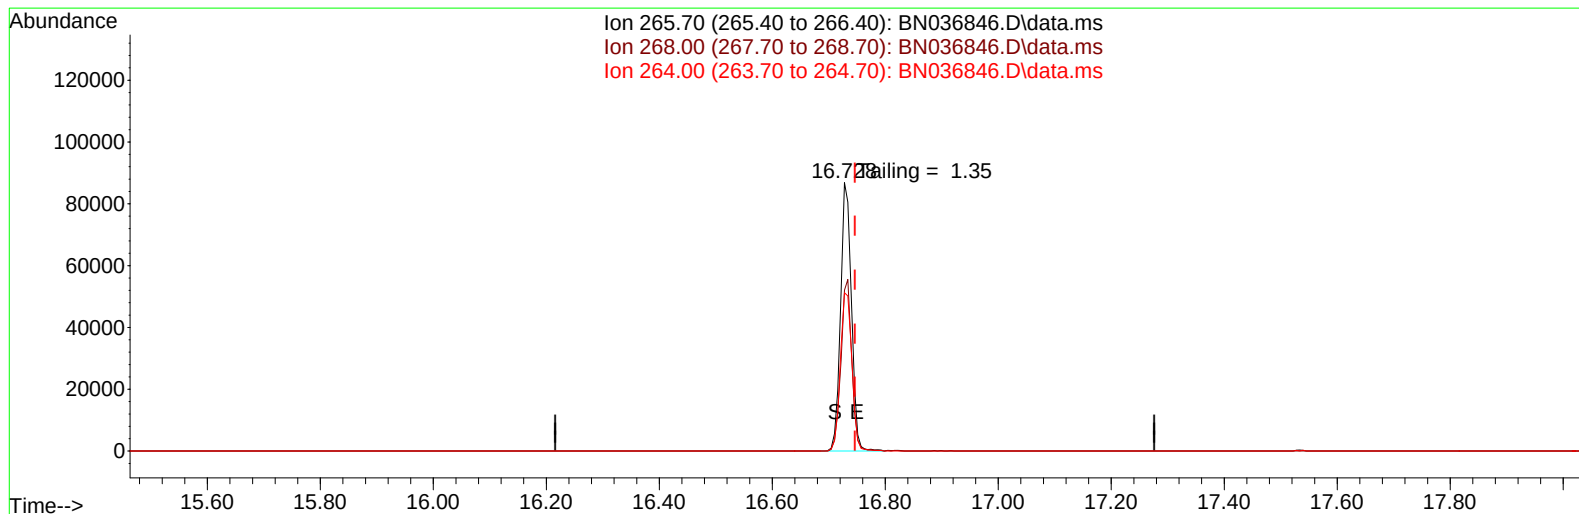

TIC: BN036846.D\data.ms

(70) Pentachlorophenol (C)




16.728min (-0.018) 17027.90 ng

response 115056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.94
264.00	61.60	58.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040725\
Data File : BN036846.D
Acq On : 07 Apr 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 17:29:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

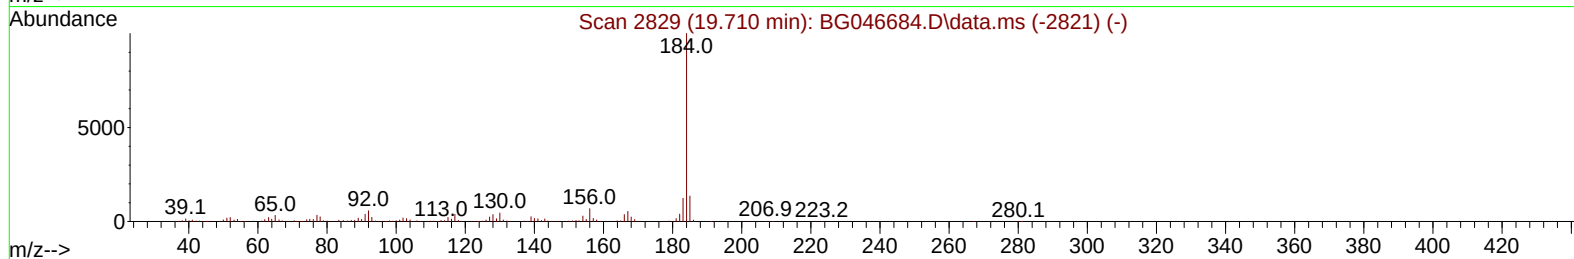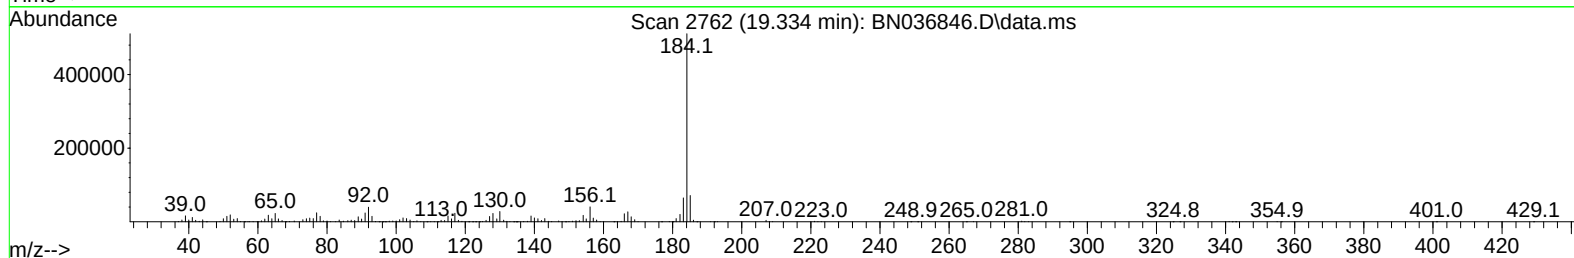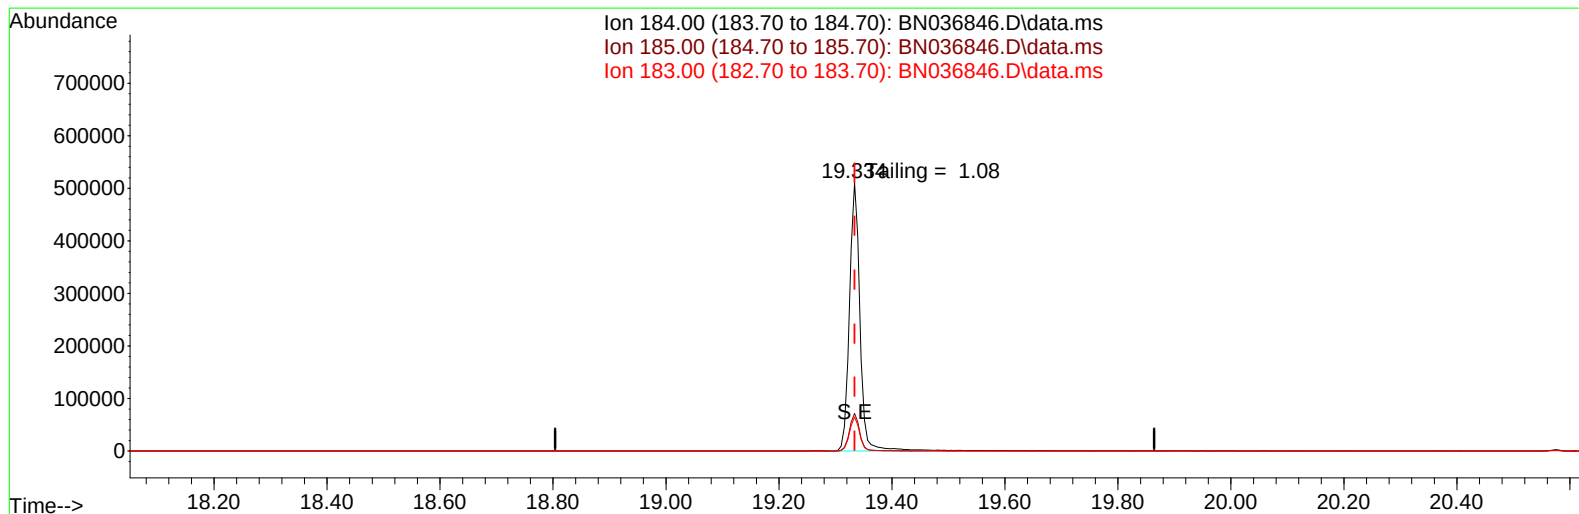

TIC: BN036846.D\data.ms

(77) Benzidine

19.334min (-0.001) 0.00 ng

response 661335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.73
0.00	0.00	0.00