


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040725\
Data File : BN036846.D
Acq On : 07 Apr 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 04 17:30:43 2025

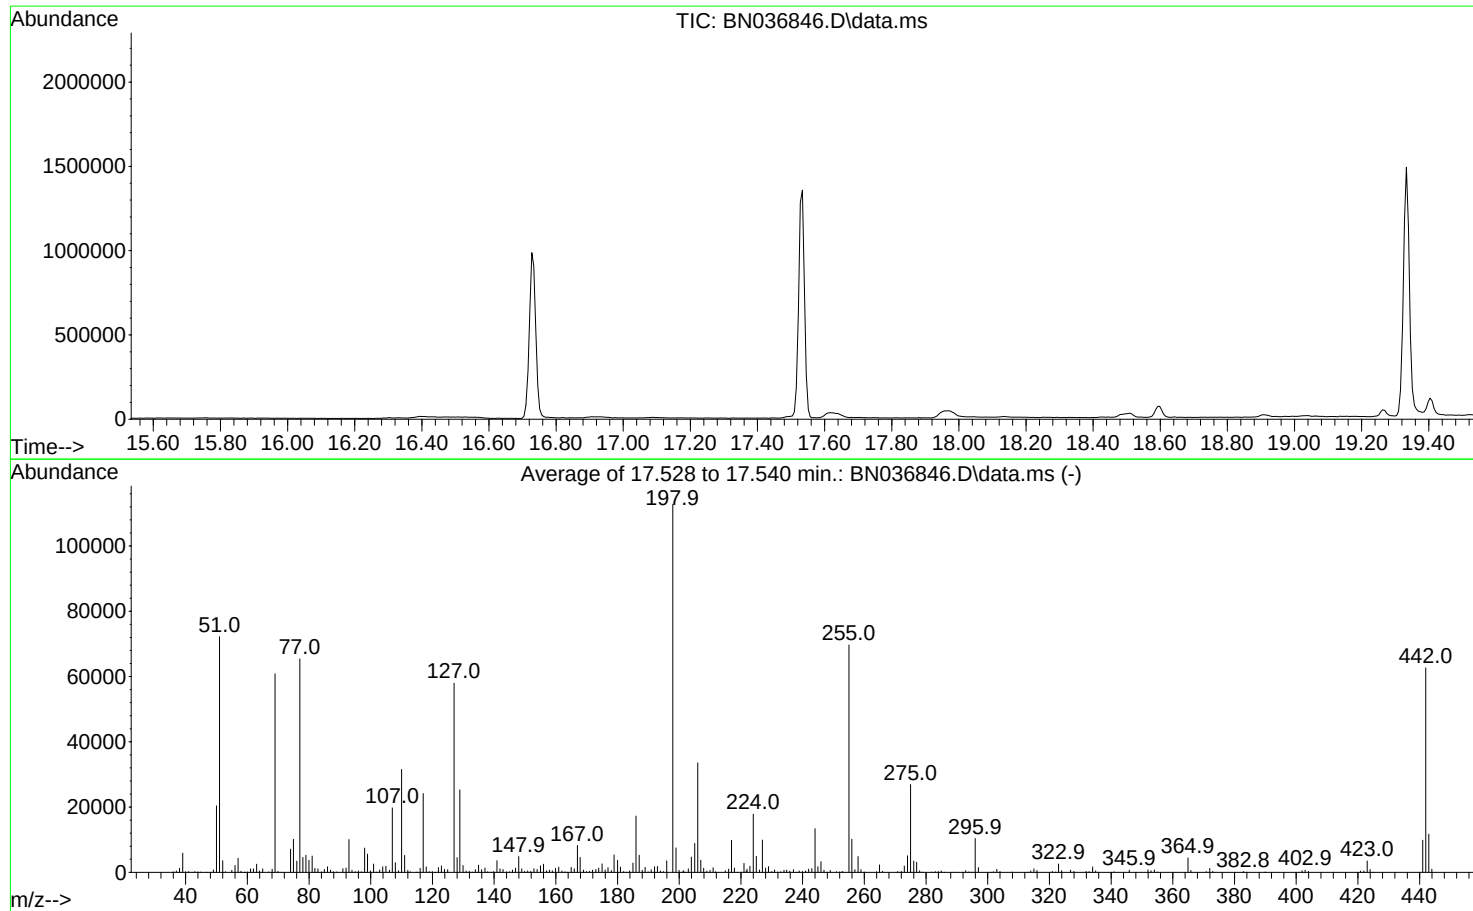




AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.1	72241	PASS
68	69	0.00	2	1.6	1000	PASS
69	198	0.00	100	54.0	60832	PASS
70	69	0.00	2	0.5	313	PASS
127	198	10	80	51.4	57968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112723	PASS
199	198	5	9	6.7	7515	PASS
275	198	10	60	23.9	26899	PASS
365	198	1	100	3.9	4404	PASS
441	198	0.01	100	8.8	9864	PASS
442	442	50	100	100.0	62661	PASS
443	442	15	24	18.7	11731	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040725\
Data File : BN036846.D
Acq On : 07 Apr 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 07 17:29:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

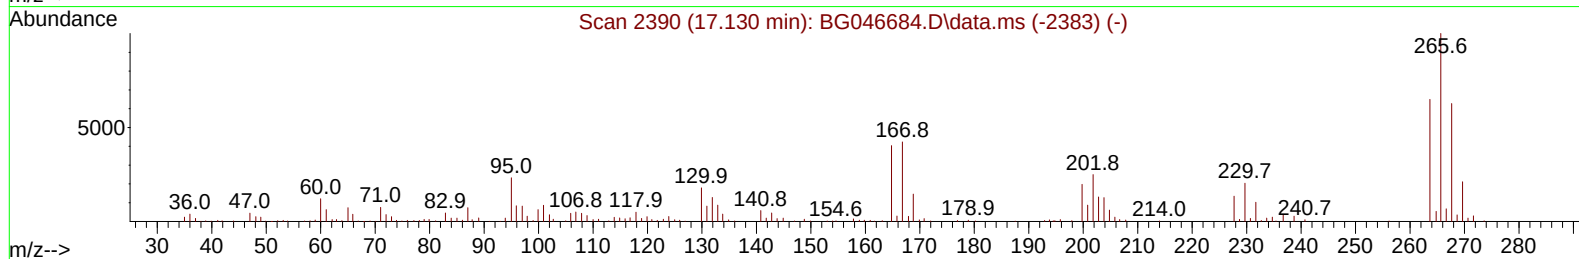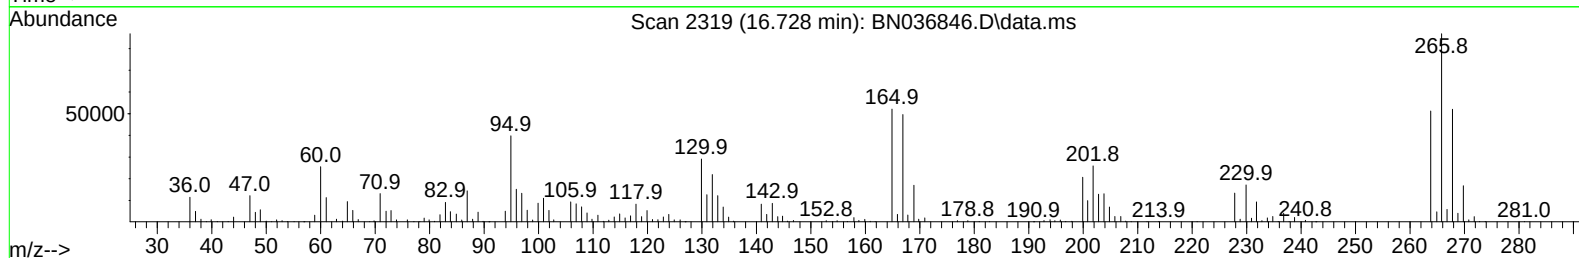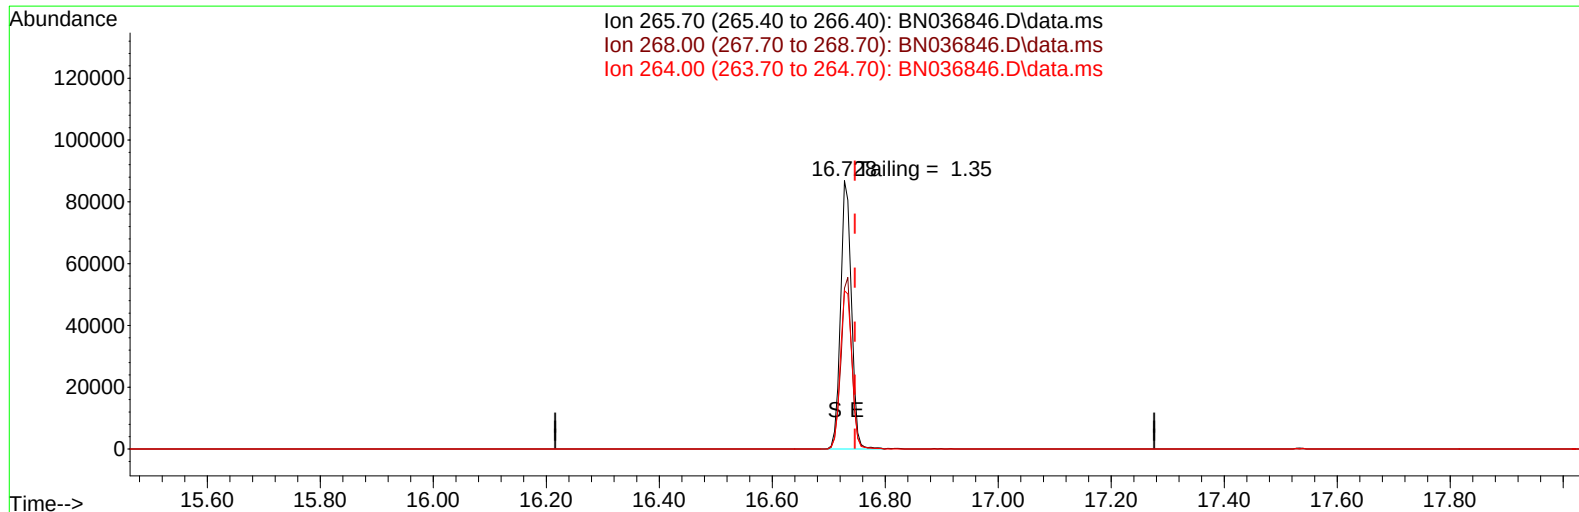

TIC: BN036846.D\data.ms

(70) Pentachlorophenol (C)

16.728min (-0.018) 17027.90 ng




response 115056

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.94
264.00	61.60	58.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040725\
Data File : BN036846.D
Acq On : 07 Apr 2025 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 07 17:29:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

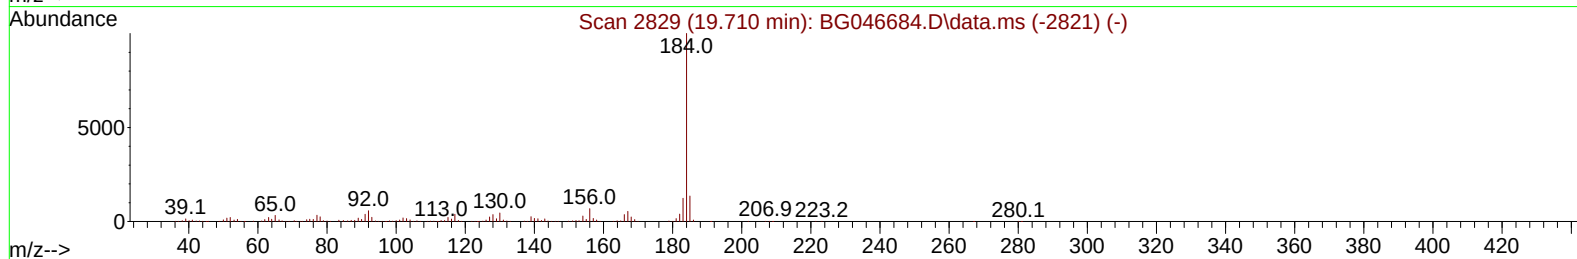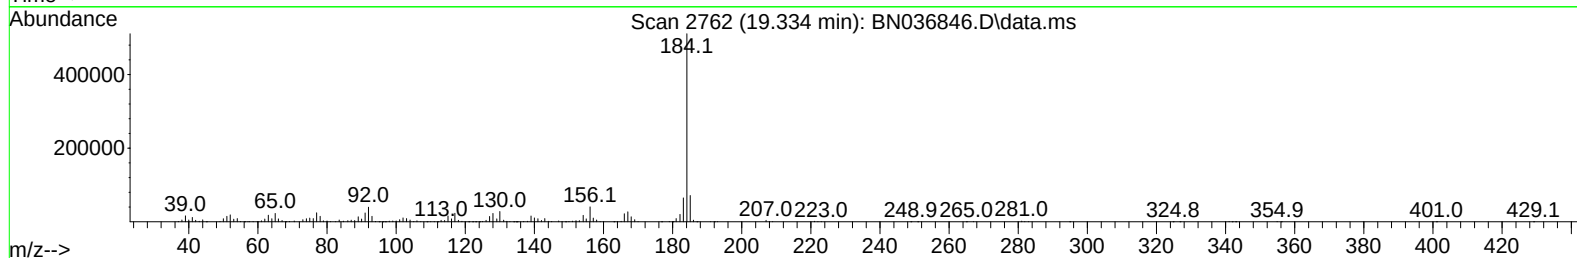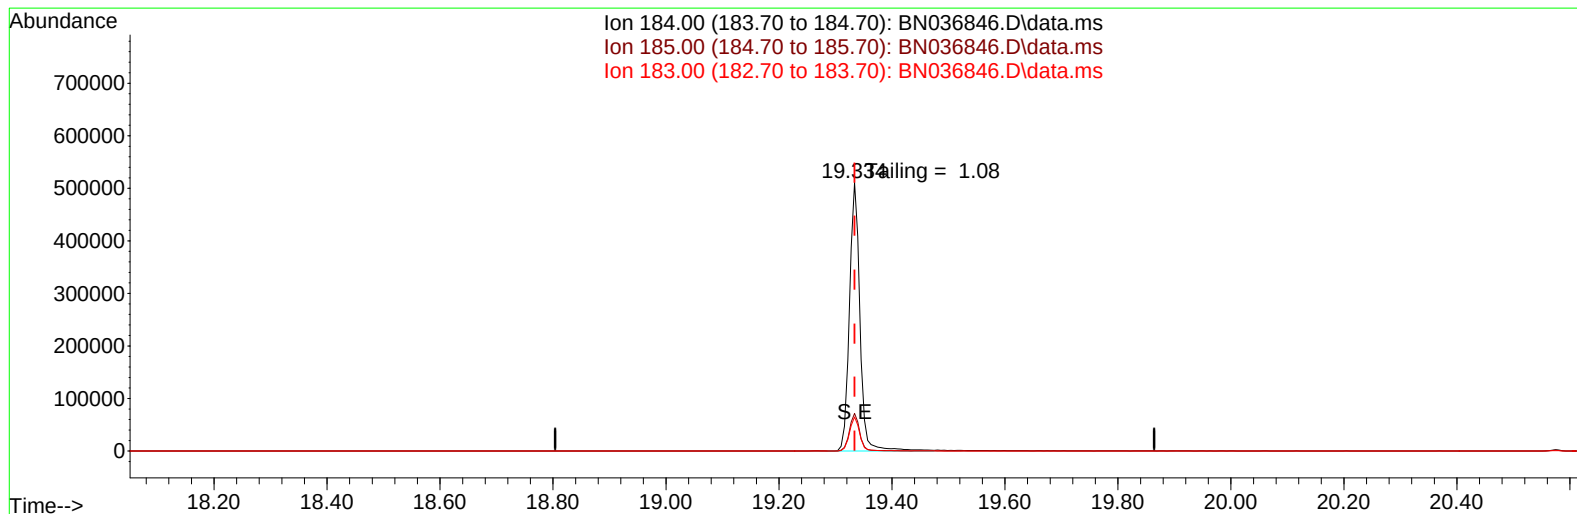

TIC: BN036846.D\data.ms

(77) Benzidine

19.334min (-0.001) 0.00 ng

response 661335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	12.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/7/2025	BNA_N	<u>BN036846.D</u>
Compound Name	Response	Retention Time
DDT	386395	20.575
DDD	7439	20.133
DDE	337	19.628
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7776	394171	1.97

Instrument :
BNA_N
ClientSampleId :
DFTPP