

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040820\
 Data File : BN010443.D
 Acq On : 09 Apr 2020 00:17
 Operator : CG/JU
 Sample : L2155-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFB3

Manual Integrations
 APPROVED

mohammad
 4/9/2020 11:38:44 AM

Quant Time: Apr 09 02:01:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 08 13:35:12 2020
 Response via : Initial Calibration

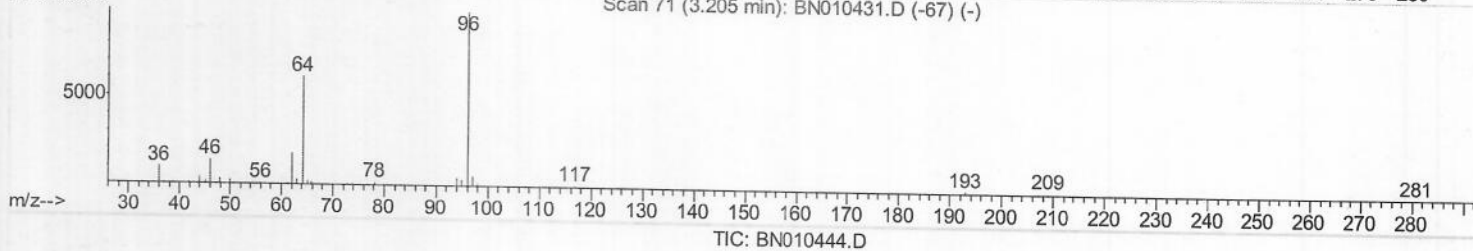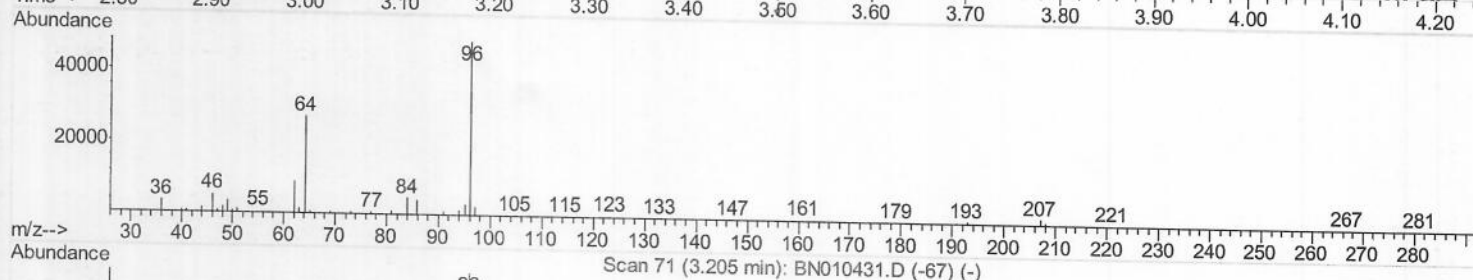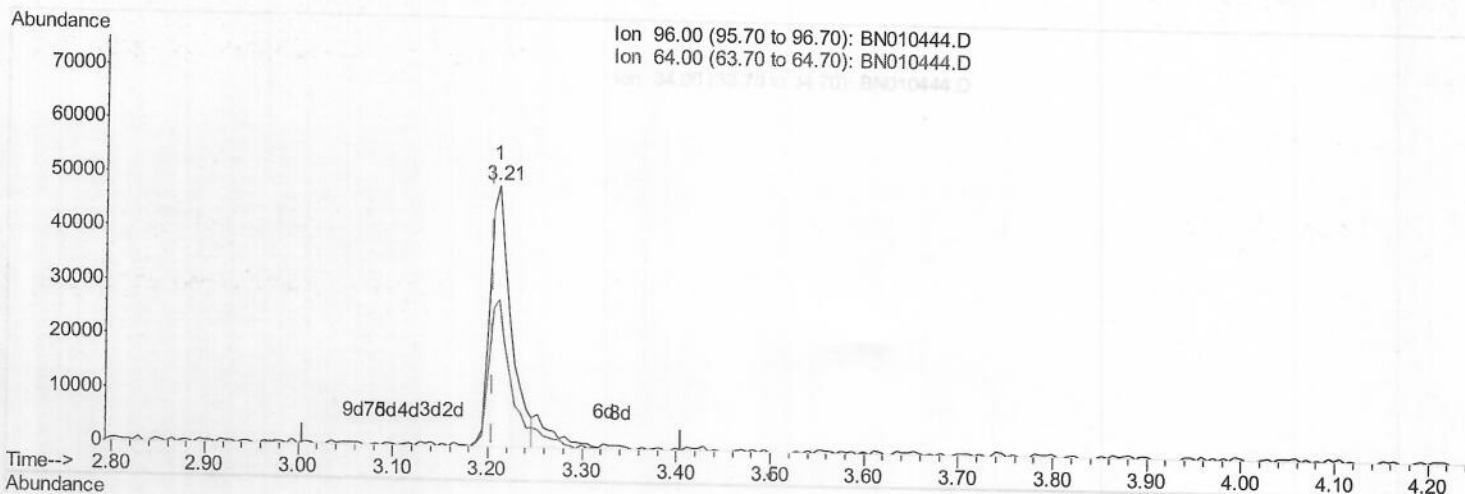

(3) 1,4-Dioxane-d8 (S)

3.211min (+0.006) 6.18ng/uL

response 75311

Ion	Exp%	Act%
96.00	100	100
64.00	59.90	56.30
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040820\
 Data File : BN010443.D
 Acq On : 09 Apr 2020 00:17
 Operator : CG/JU
 Sample : L2155-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFB3

Manual Integrations
 APPROVED

mohammad
 4/9/2020 11:38:44 AM

Quant Time: Apr 09 02:01:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 08 13:35:12 2020
 Response via : Initial Calibration

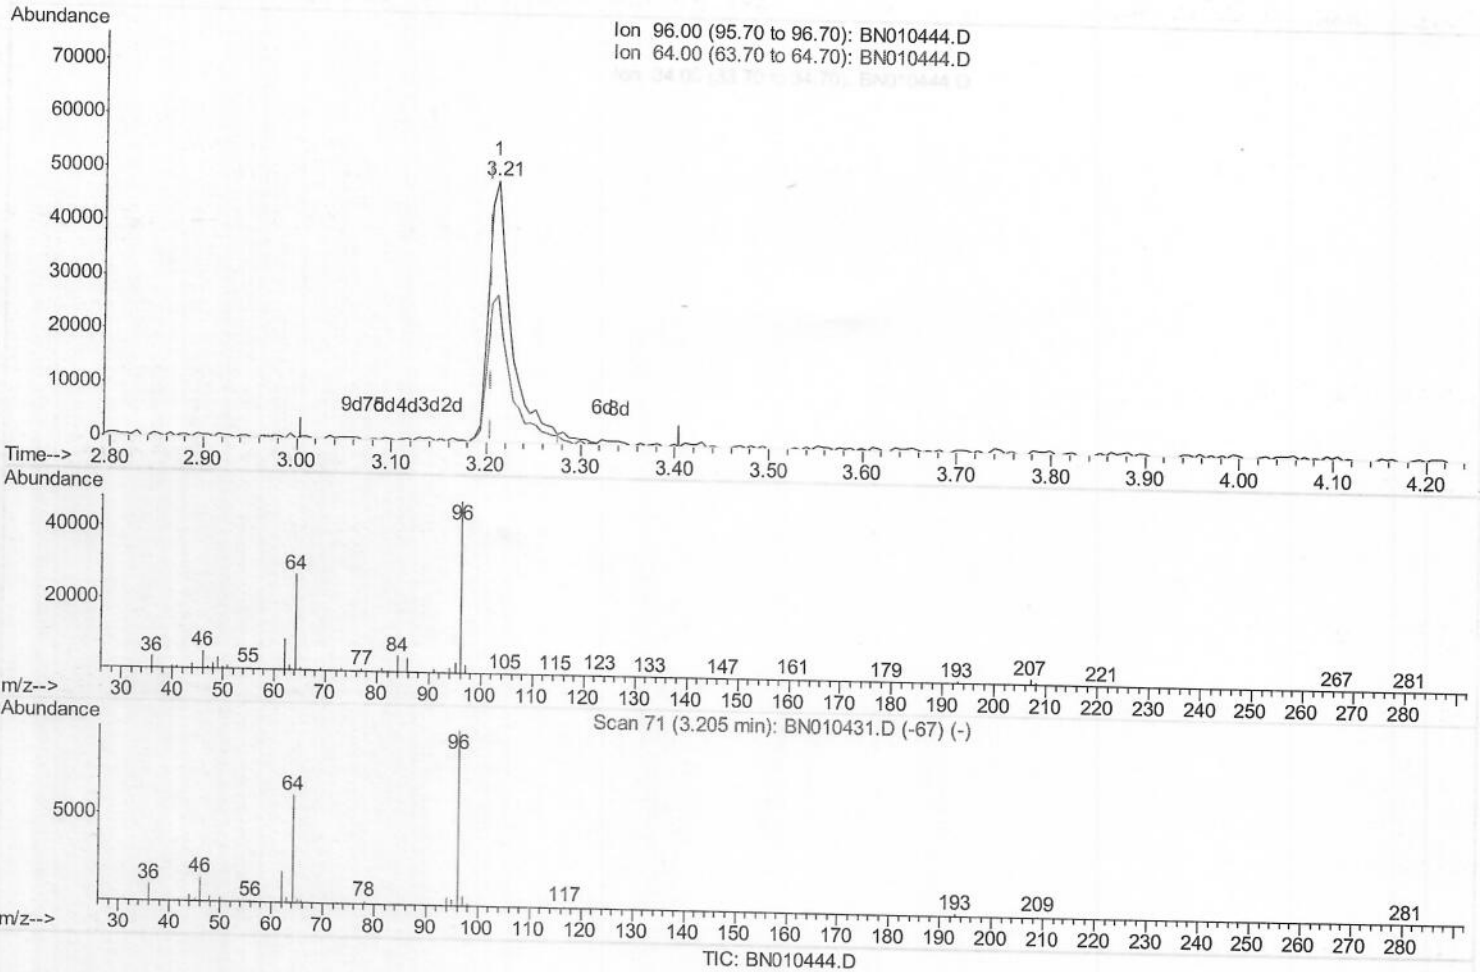

(3) 1,4-Dioxane-d8 (S)

3.211min (+0.006) 6.71ng/uL m

response 81738

Ion	Exp%	Act%
96.00	100	100
64.00	59.90	56.30
34.00	0.00	0.00
0.00	0.00	0.00

AP
 04/20/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040820\
 Data File : BN010443.D
 Acq On : 09 Apr 2020 00:17
 Operator : CG/JU
 Sample : L2155-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBFB3

Manual Integrations
 APPROVED

mohammad
 4/9/2020 11:38:44 AM

Quant Time: Apr 09 03:58:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 08 13:35:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	575921	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	2441511	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1572083	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	3536715	20.00	ng/ul	0.01
78) Chrysene-d12	21.19	240	3392047	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	2901587	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	81738m	6.71	ng/uL	0.00
5) Phenol-d5	6.80	99	1772669	36.90	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.95	67	957130	38.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	1567487	41.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	1384165	34.10	ng/ul	0.01
19) Nitrobenzene-d5	8.75	128	809909	44.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	916070	47.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	1655074	41.59	ng/ul	0.01
29) 4-Chloroaniline-d4	10.50	131	1634577	34.75	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	4951836	41.75	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	6229328	44.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.45	143	785534	35.26	ng/ul	0.01
58) Fluorene-d10	15.23	176	4545836	43.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.36	200	417942	20.64	ng/ul	0.00
71) Anthracene-d10	17.08	188	7070830	43.54	ng/ul	0.00
79) Pyrene-d10	19.39	212	7928658	45.36	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.23	264	6484585	44.92	ng/ul	0.00

AP
 04/10/2020

Target Compounds

45) Dimethylphthalate	13.70	163	1365123	11.145	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.13	149	324678	2.426	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040820\
 Data File : BN010443.D
 Acq On : 09 Apr 2020 00:17
 Operator : CG/JU
 Sample : L2155-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 DBFB3

Manual Integrations
 APPROVED

mohammad
 4/9/2020 11:38:44 AM

Quant Time: Apr 09 03:58:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 08 13:35:12 2020
 Response via : Initial Calibration

