

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040822\
 Data File : BN019397.D
 Acq On : 08 Apr 2022 20:24
 Operator : CG/JU
 Sample : N2333-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-9D

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/11/2022
 Supervised By : mohammad ahmed 04/11/2022

Quant Time: Apr 11 04:11:29 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 04 17:40:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.825	152	4353	0.400	ng	0.00
7) Naphthalene-d8	10.626	136	12974	0.400	ng	# 0.00
13) Acenaphthene-d10	14.463	164	8786	0.400	ng	0.00
19) Phenanthrene-d10	17.205	188	17874	0.400	ng	0.00
29) Chrysene-d12	21.386	240	15629	0.400	ng	# 0.00
35) Perylene-d12	23.741	264	13148	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.384	112	1915	0.164	ng	0.00
5) Phenol-d6	7.002	99	1305	0.093	ng	0.01
8) Nitrobenzene-d5	8.982	82	2957	0.251	ng	0.00
11) 2-Methylnaphthalene-d10	12.219	152	7069m	0.310	ng	0.00
14) 2,4,6-Tribromophenol	15.954	330	1846	0.346	ng	0.00
15) 2-Fluorobiphenyl	13.095	172	10148	0.278	ng	0.00
27) Fluoranthene-d10	19.236	212	22745	0.395	ng	0.00
31) Terphenyl-d14	19.830	244	13139	0.387	ng	0.00
Target Compounds						Qvalue
34) Bis(2-ethylhexyl)phtha...	21.306	149	3682	0.086	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040822\
Data File : BN019397.D
Acq On : 08 Apr 2022 20:24
Operator : CG/JU
Sample : N2333-05
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
MW-9D

Quant Time: Apr 11 04:11:29 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 04 17:40:00 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

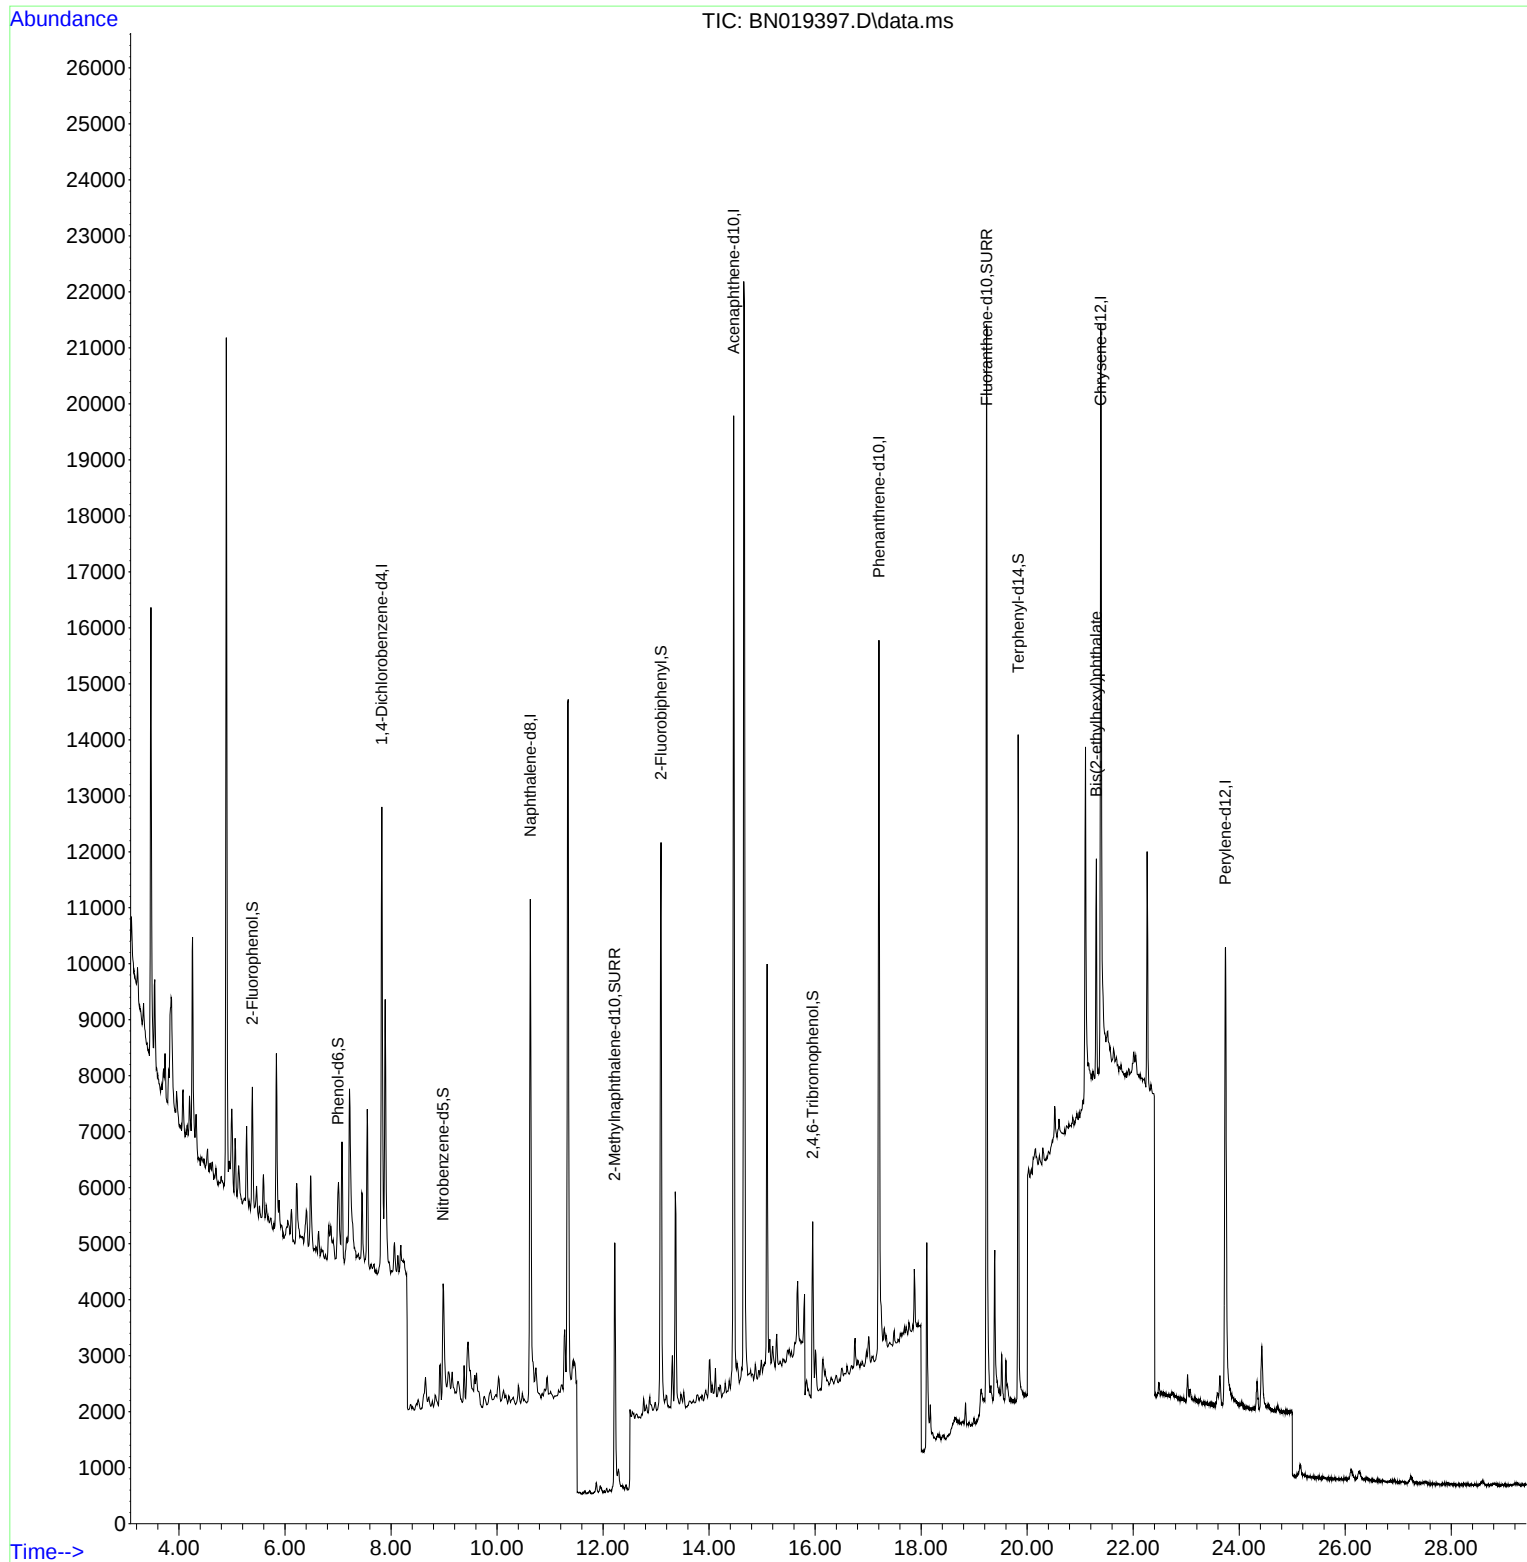

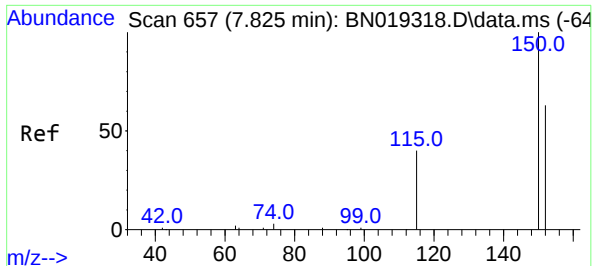

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.825 min Scan# 657
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24



Instrument :
BNA_N
ClientSampleId :
MW-9D

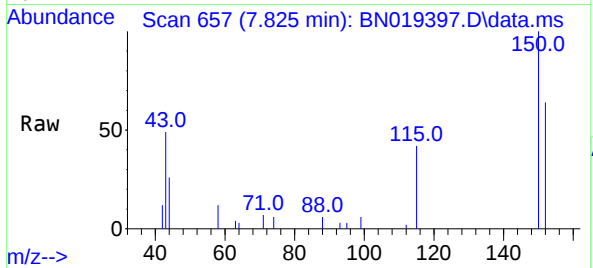


Tgt Ion:152 Resp: 435
Ion Ratio Lower Upper
152 100
150 156.0 123.9 185.9
115 65.2 48.2 72.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

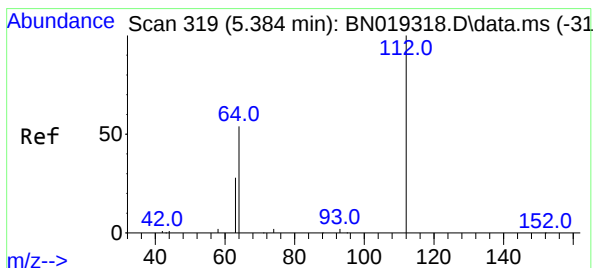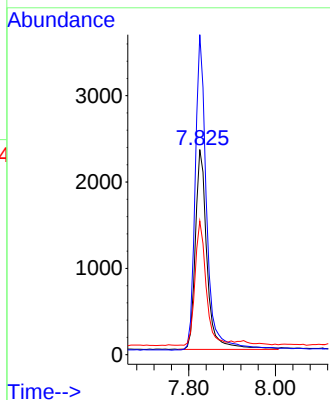

#4
2-Fluorophenol
Concen: 0.164 ng
RT: 5.384 min Scan# 319
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24

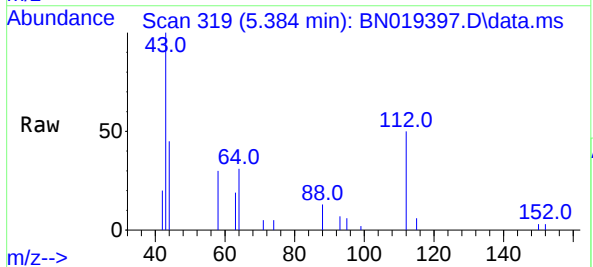

Tgt Ion:112 Resp: 1915
Ion Ratio Lower Upper
112 100
64 63.5 47.8 71.8
63 32.5 25.7 38.5

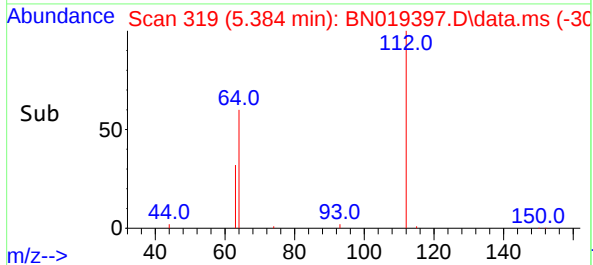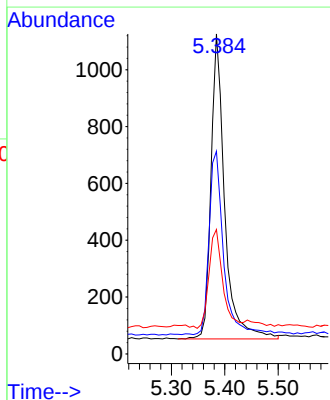







#5
Phenol-d6
Concen: 0.093 ng
RT: 7.002 min Scan# 541
Delta R.T. 0.014 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24

Instrument :
BNA_N
ClientSampleId :
MW-9D

Tgt Ion: 99 Resp: 1308
Ion Ratio Lower Upper
99 100
42 20.5 16.2 24.4
71 69.8 27.7 41.5




Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

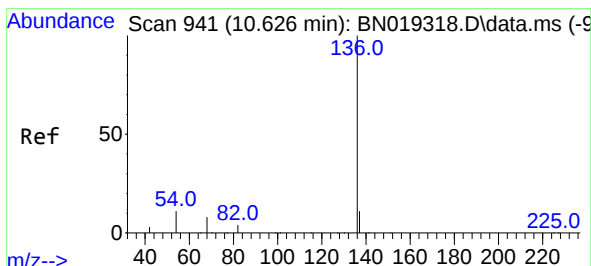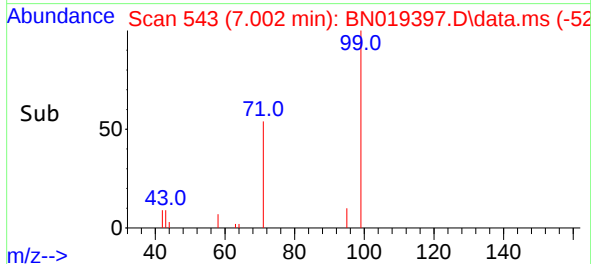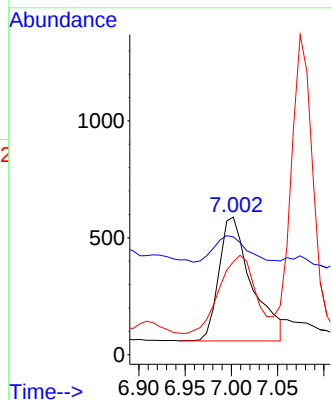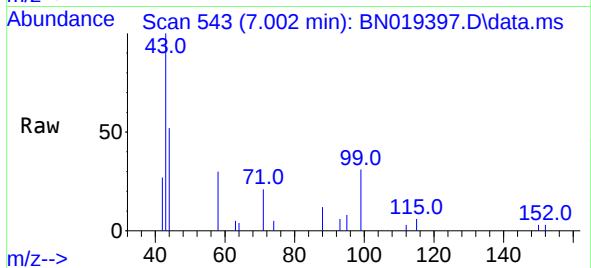

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.626 min Scan# 941
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24


Tgt Ion:136 Resp: 12974
Ion Ratio Lower Upper
136 100
137 11.7 9.0 13.4
54 12.0 5.8 8.6#
68 8.8 4.6 7.0#

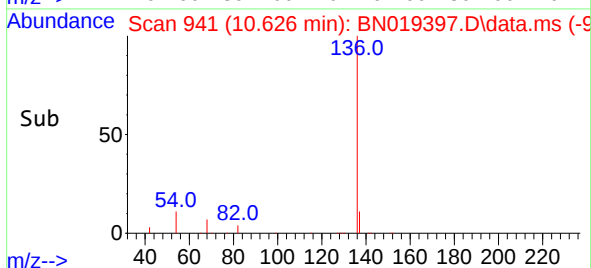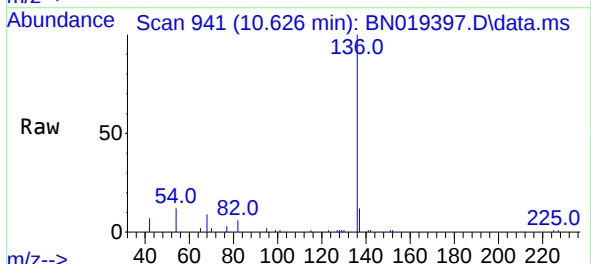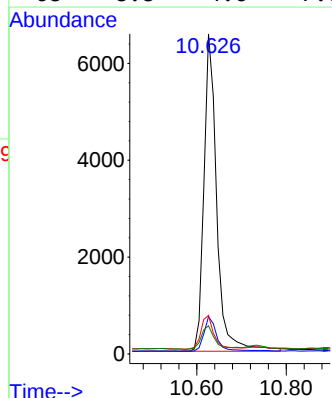



#8
Nitrobenzene-d5
Concen: 0.251 ng
RT: 8.982 min Scan# 787
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24




Instrument :
BNA_N
ClientSampleId :
MW-9D

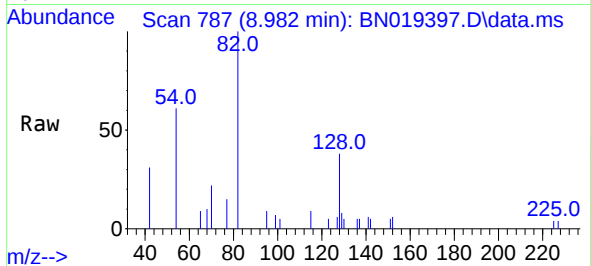

Tgt Ion: 82 Resp: 295
Ion Ratio Lower Upper
82 100
128 38.3 33.0 49.6
54 61.5 42.5 63.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

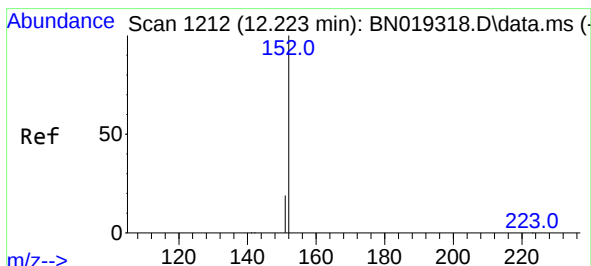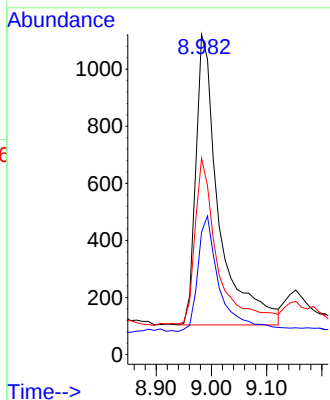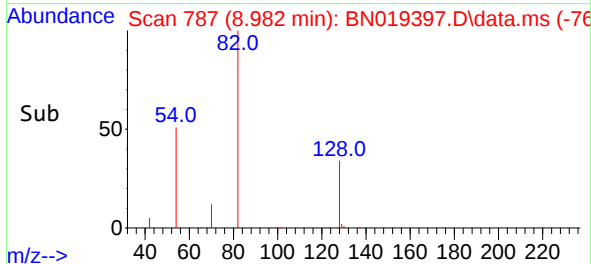

#11
2-Methylnaphthalene-d10
Concen: 0.310 ng m
RT: 12.219 min Scan# 1211
Delta R.T. -0.004 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24


Tgt Ion:152 Resp: 7069
Ion Ratio Lower Upper
152 100
151 20.4 16.5 24.7

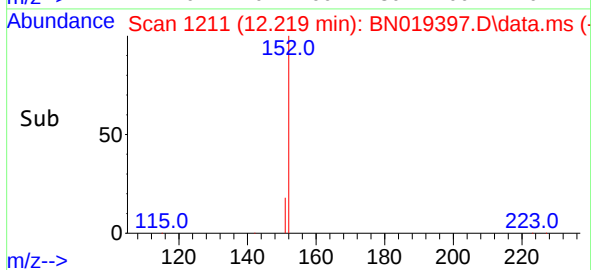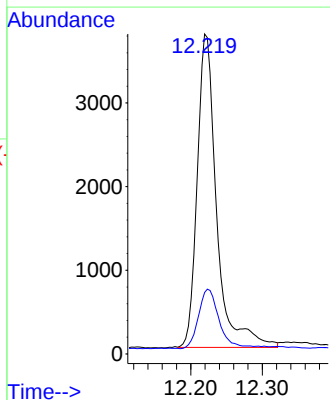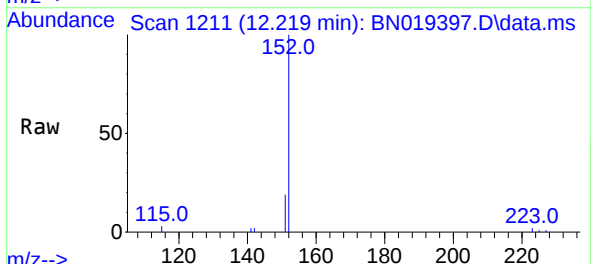

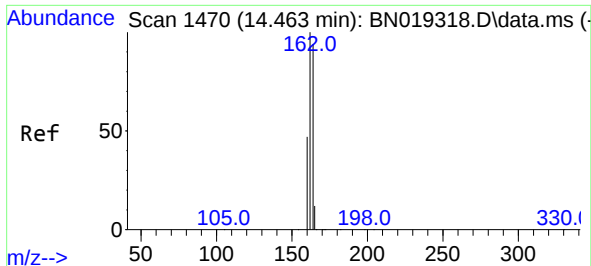

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.463 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24




Instrument :
BNA_N
ClientSampleId :
MW-9D

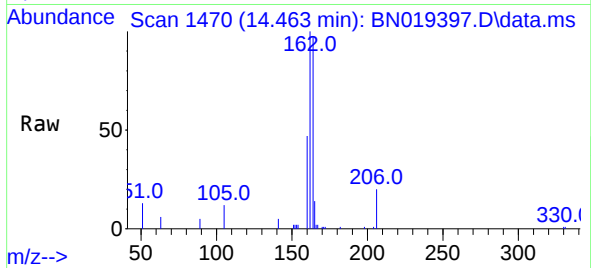


Tgt Ion:164 Resp: 8780
Ion Ratio Lower Upper
164 100
162 102.9 85.2 127.8
160 48.9 41.5 62.3

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

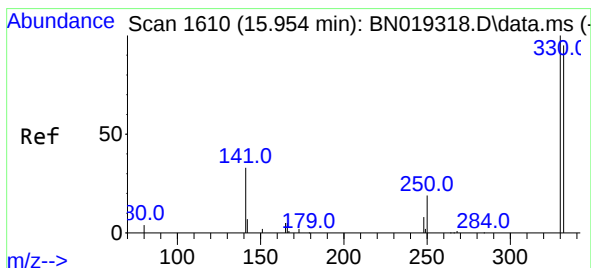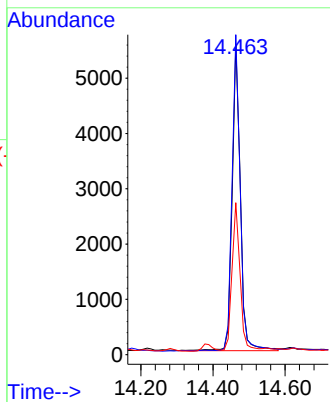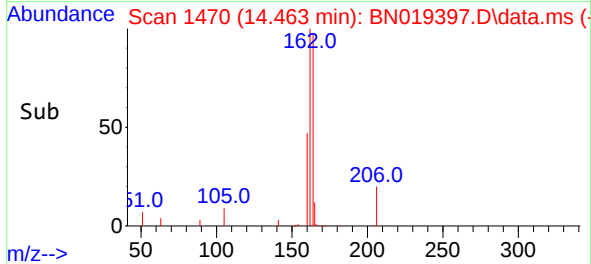


#14
2,4,6-Tribromophenol
Concen: 0.346 ng
RT: 15.954 min Scan# 1610
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24

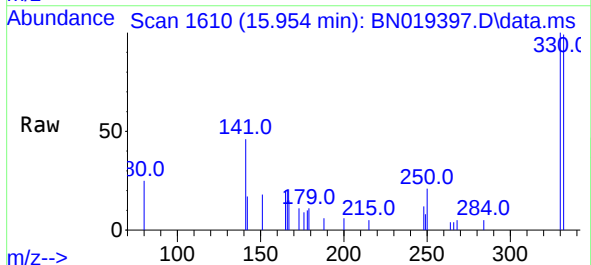


Tgt Ion:330 Resp: 1846
Ion Ratio Lower Upper
330 100
332 98.2 76.8 115.2
141 40.2 32.2 48.2

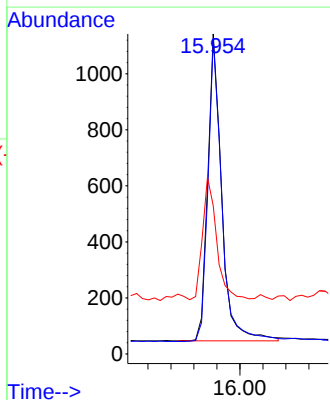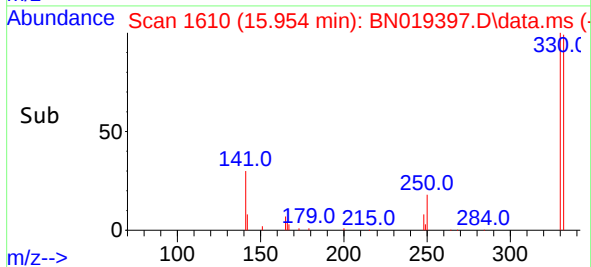

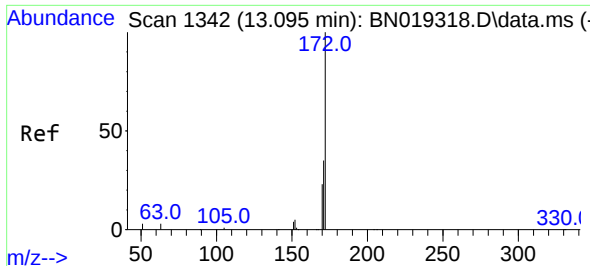

#15
2-Fluorobiphenyl
Concen: 0.278 ng
RT: 13.095 min Scan# 1342
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24




Instrument :
BNA_N
ClientSampleId :
MW-9D

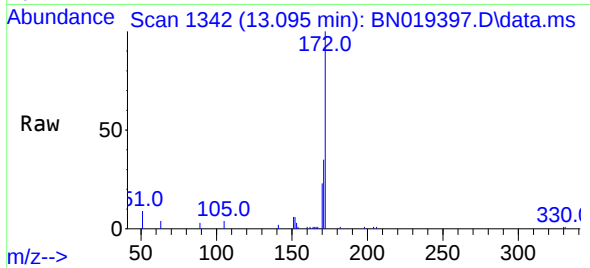


Tgt Ion:172 Resp: 10148
Ion Ratio Lower Upper
172 100
171 35.3 28.2 42.2
170 23.2 18.7 28.1

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

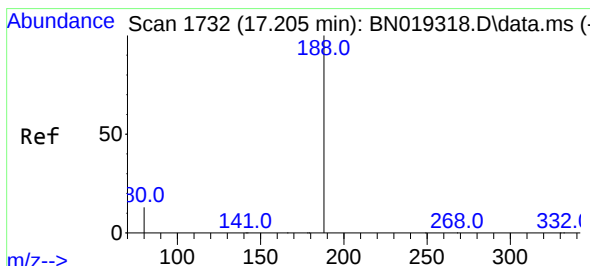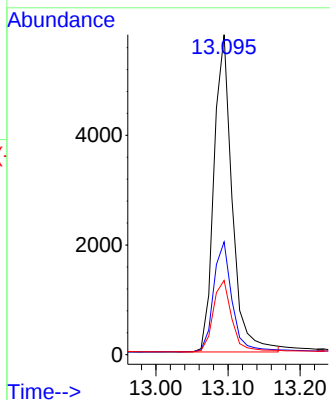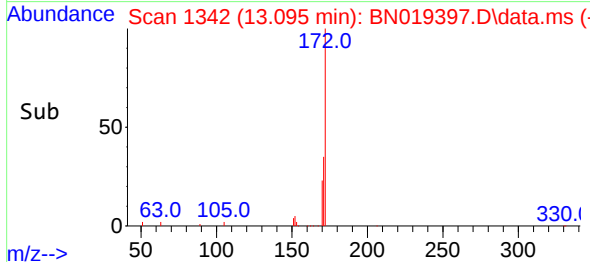


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.205 min Scan# 1732
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24

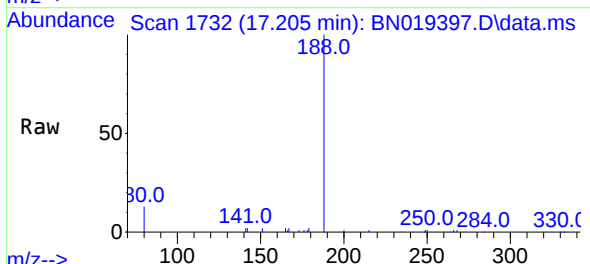


Tgt Ion:188 Resp: 17874
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.9 11.8 17.8

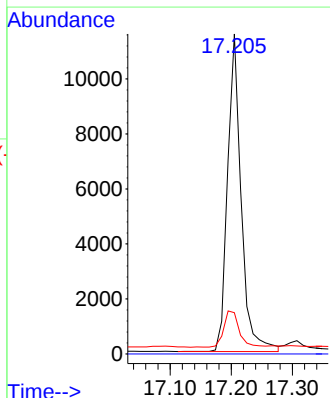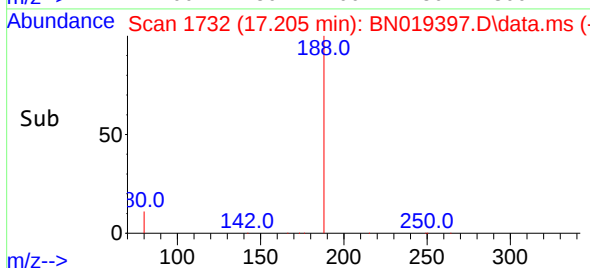

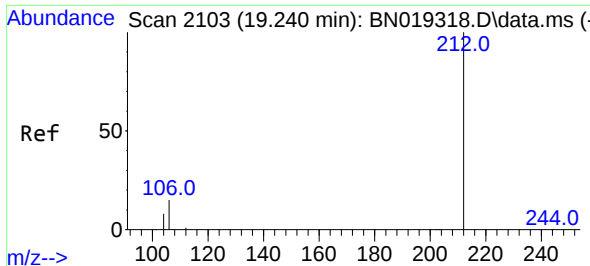

#27
Fluoranthene-d10
Concen: 0.395 ng
RT: 19.236 min Scan# 2102
Delta R.T. -0.004 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24




Instrument :
BNA_N
ClientSampleId :
MW-9D

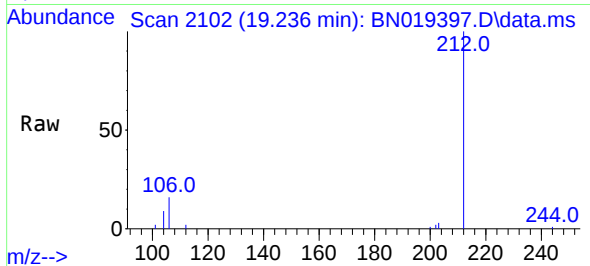

Tgt Ion:212 Resp: 22749
Ion Ratio Lower Upper
212 100
106 15.5 12.7 19.1
104 9.0 7.1 10.7




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

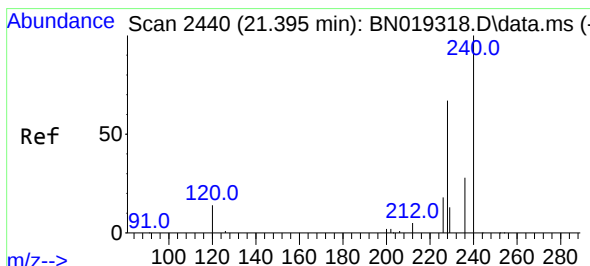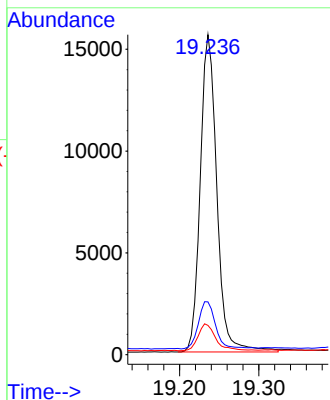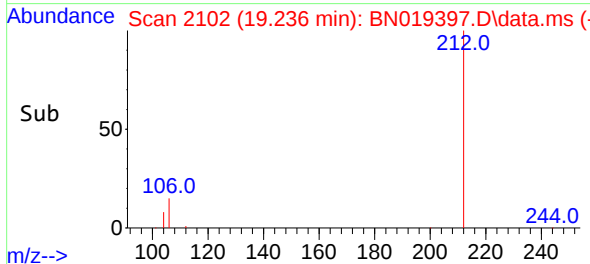

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.386 min Scan# 2439
Delta R.T. -0.009 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24


Tgt Ion:240 Resp: 15629
Ion Ratio Lower Upper
240 100
120 20.5 8.5 12.7#
236 29.8 22.4 33.6

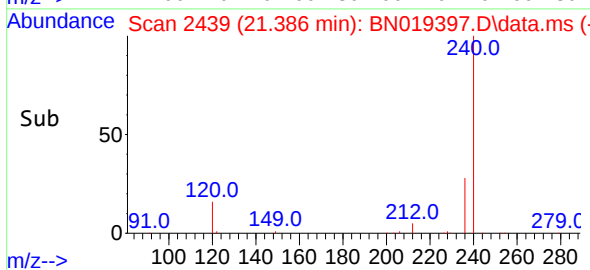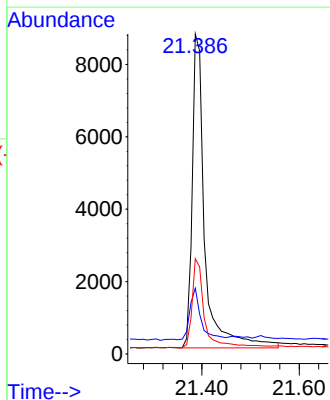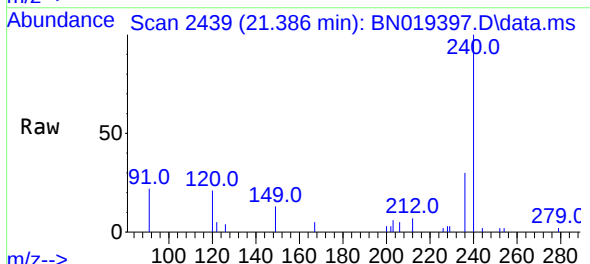

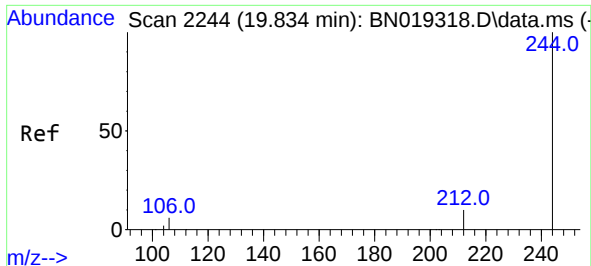

#31
Terphenyl-d14
Concen: 0.387 ng
RT: 19.830 min Scan# 2113
Delta R.T. -0.004 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24



Instrument :
BNA_N
ClientSampleId :
MW-9D

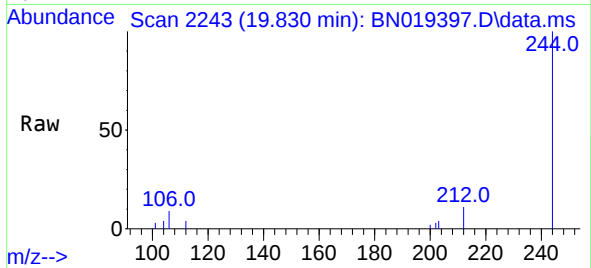

Tgt Ion:244 Resp: 13139
Ion Ratio Lower Upper
244 100
212 11.2 8.2 12.4
122 0.0 0.0 0.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 04/11/2022
Supervised By :mohammad ahmed 04/11/2022

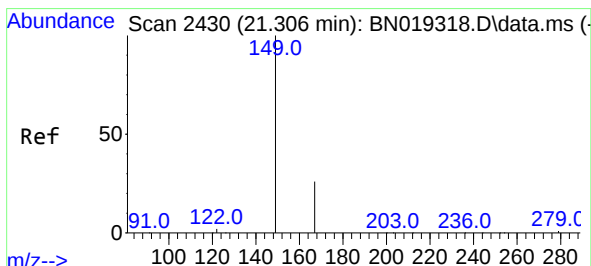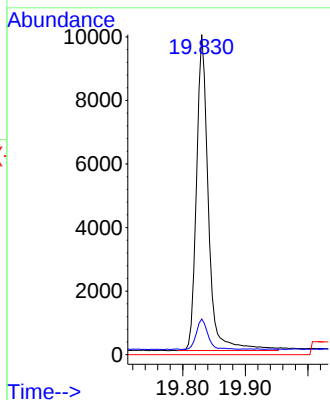

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.086 ng
RT: 21.306 min Scan# 2430
Delta R.T. 0.000 min
Lab File: BN019397.D
Acq: 08 Apr 2022 20:24


Tgt Ion:149 Resp: 3682
Ion Ratio Lower Upper
149 100
167 26.8 21.8 32.8
279 3.9 2.0 3.0#

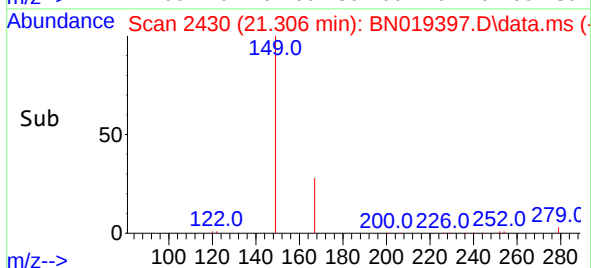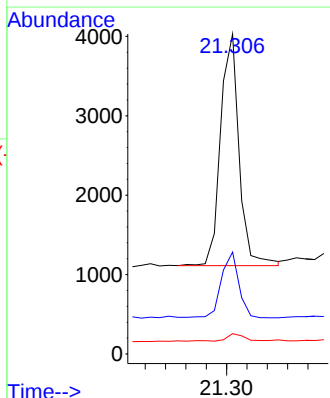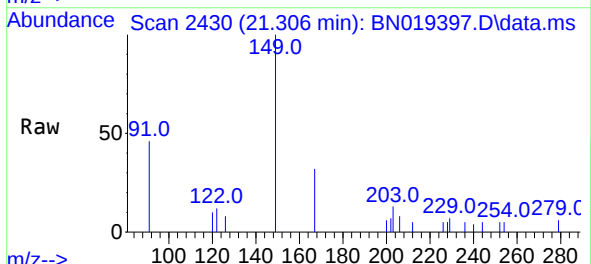

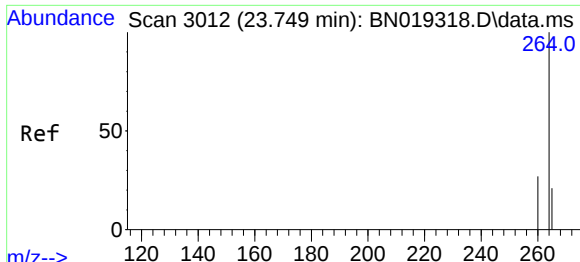

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.741 min Scan# 3012
 Delta R.T. -0.009 min
 Lab File: BN019397.D
 Acq: 08 Apr 2022 20:24

Instrument :
 BNA_N
 ClientSampleId :
 MW-9D

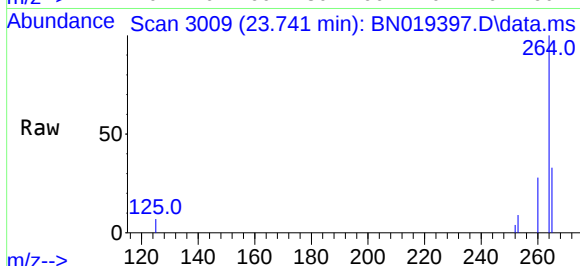

Tgt Ion: 264 Resp: 13148

Ion	Ratio	Lower	Upper
264	100		
260	28.1	22.4	33.6
265	33.1	25.3	37.9

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/11/2022
 Supervised By : mohammad ahmed 04/11/2022

