
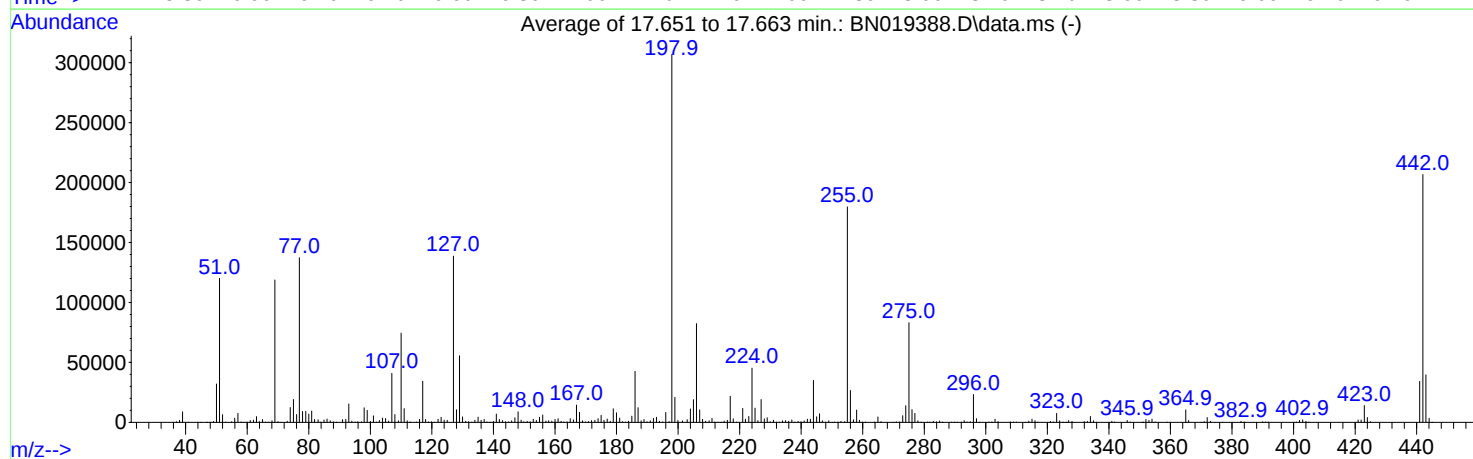


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040822\
 Data File : BN019388.D
 Acq On : 08 Apr 2022 12:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 04 17:40:00 2022

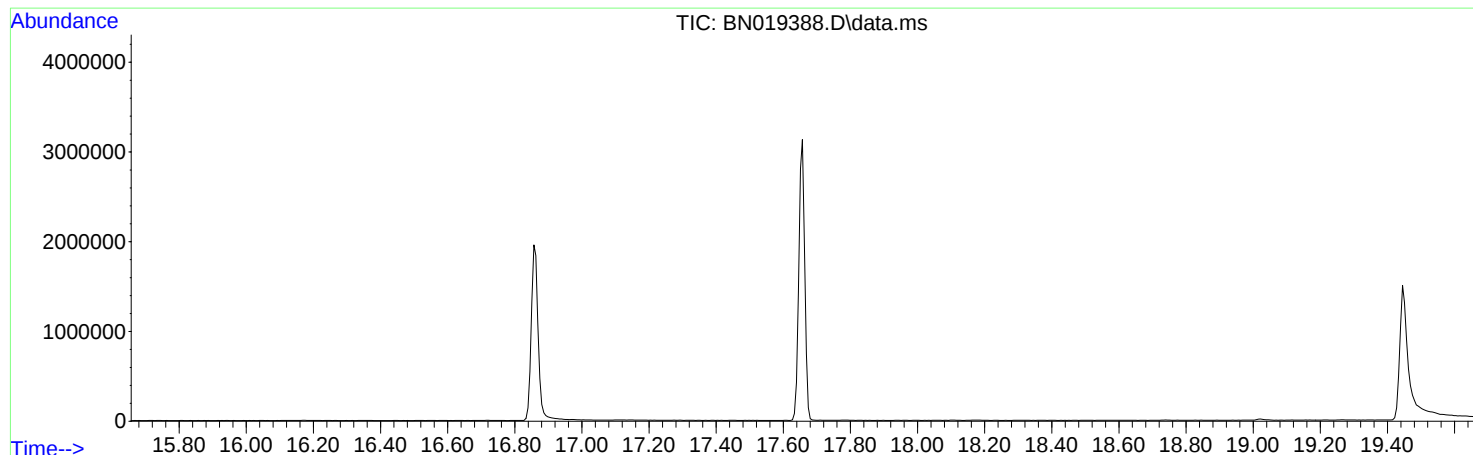




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	120101	PASS
68	69	0.00	2	1.1	1349	PASS
69	198	0.00	100	38.7	118745	PASS
70	69	0.00	2	0.6	710	PASS
127	198	10	80	45.2	138621	PASS
197	198	0.00	2	0.2	623	PASS
198	198	100	100	100.0	306837	PASS
199	198	5	9	6.8	20965	PASS
275	198	10	60	27.1	83216	PASS
365	198	1	100	3.4	10364	PASS
441	198	0.01	100	11.2	34237	PASS
442	442	50	100	100.0	206677	PASS
443	442	15	24	19.2	39688	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040822\
Data File : BN019388.D
Acq On : 08 Apr 2022 12:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 11 04:40:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

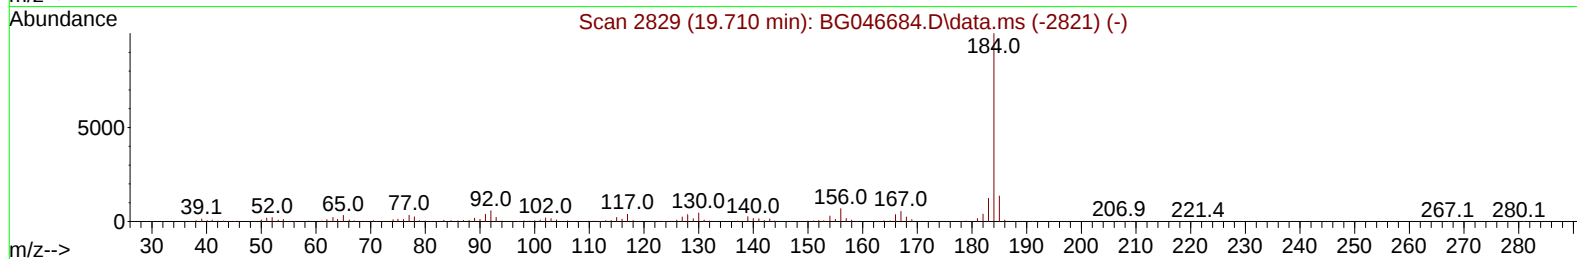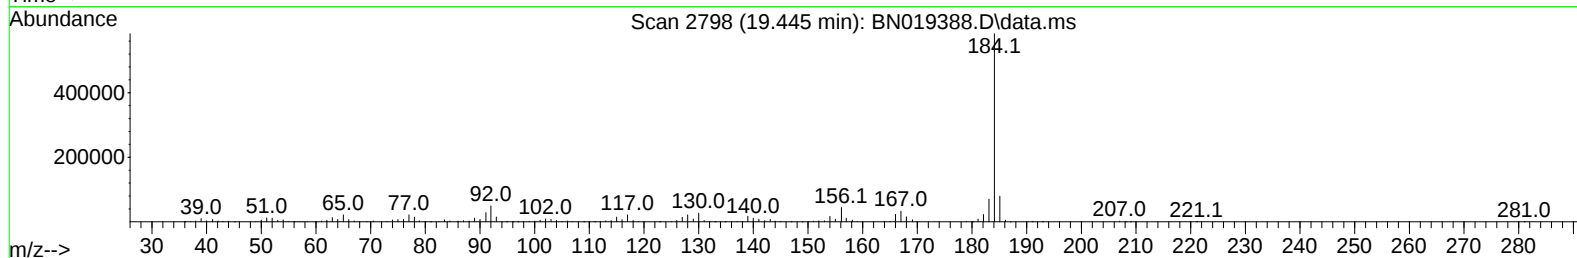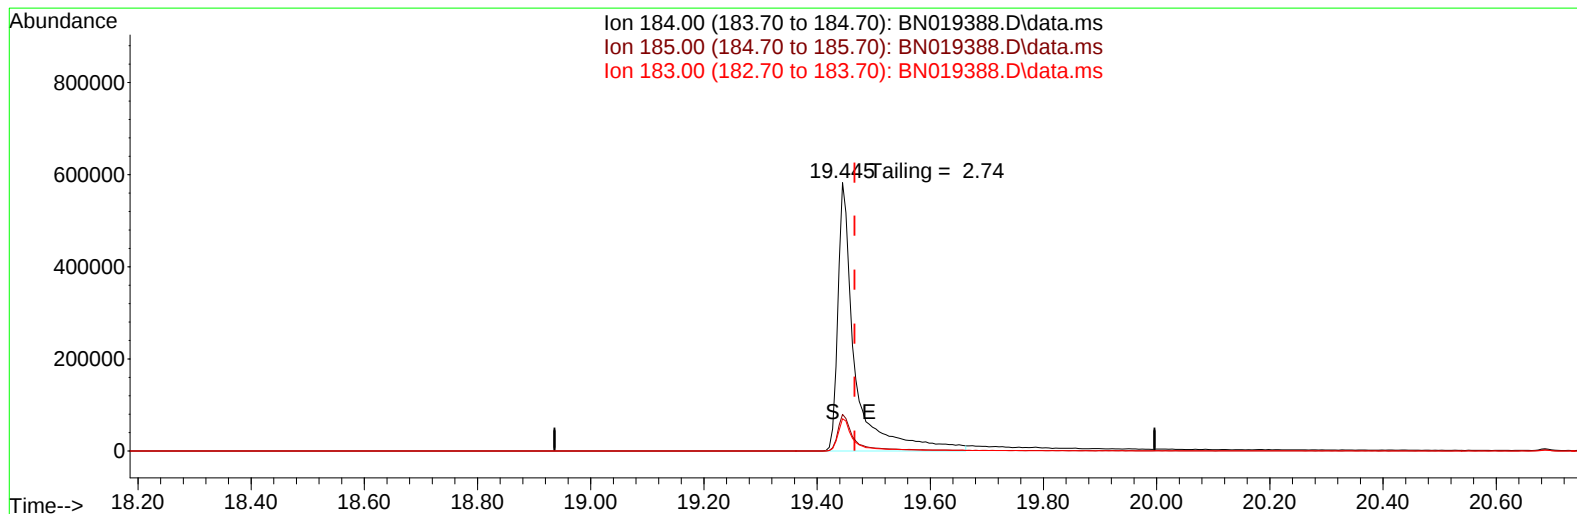

TIC: BN019388.D\data.ms

(77) Benzidine

19.445min (-0.021) 0.00 ng




response 1261015

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.68
183.00	13.20	12.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040822\
 Data File : BN019388.D
 Acq On : 08 Apr 2022 12:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 11 04:40:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

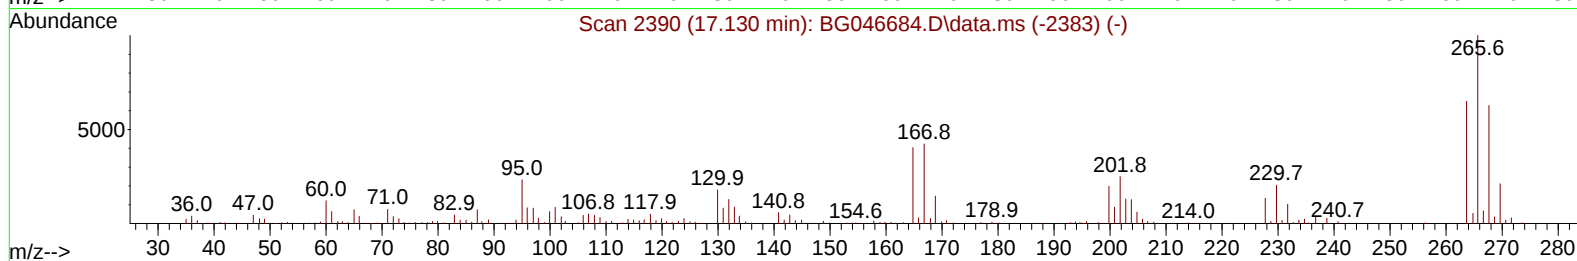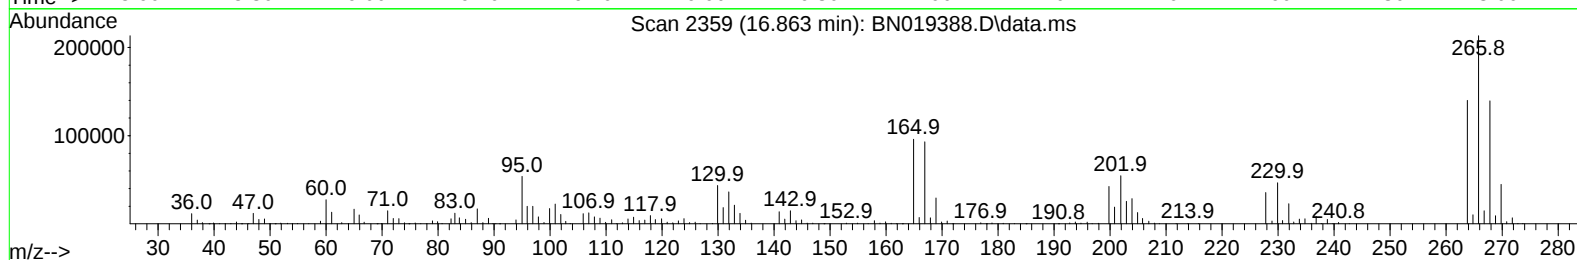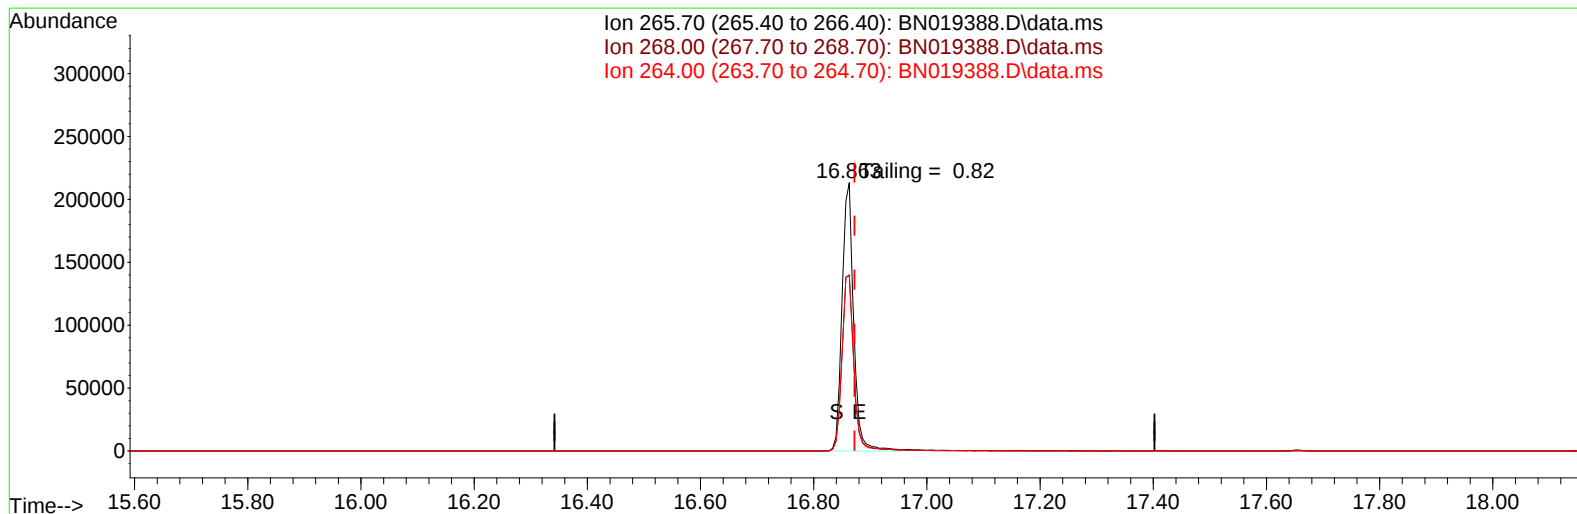

TIC: BN019388.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.009) 19527.49 ng

response 302969

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.38
264.00	61.60	65.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2022	BNA_N	<u>BN019388.D</u>
Compound Name	Response	Retention Time
DDT	936402	20.686
DDD	17053	20.245
DDE	1429	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18482	954884	1.94

Instrument :
BNA_N
ClientSampleId :
DFTPP