
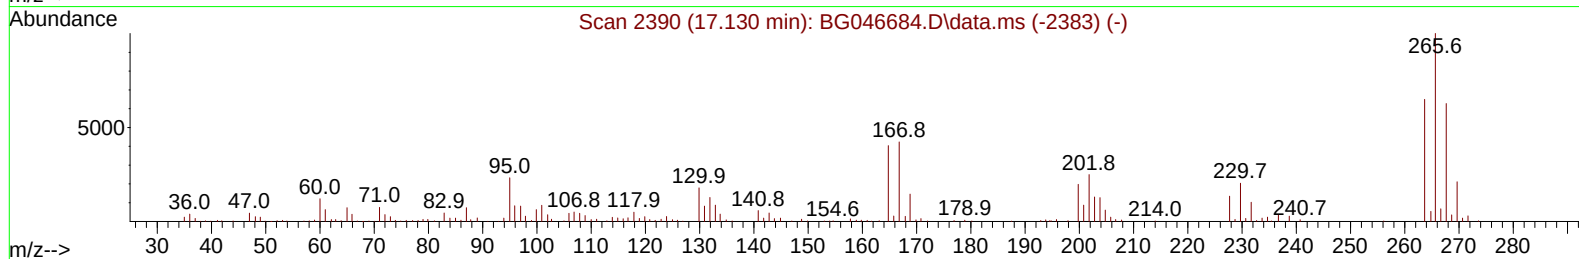
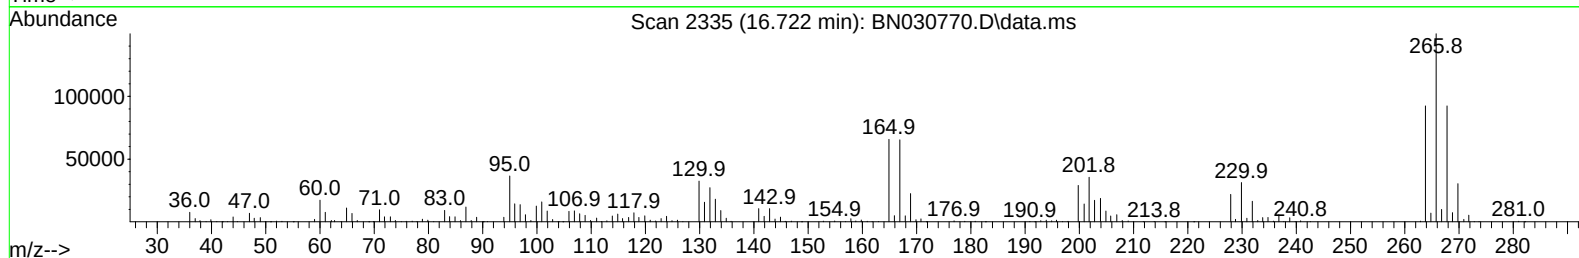


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030770.D
Acq On : 08 Apr 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 17:14:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

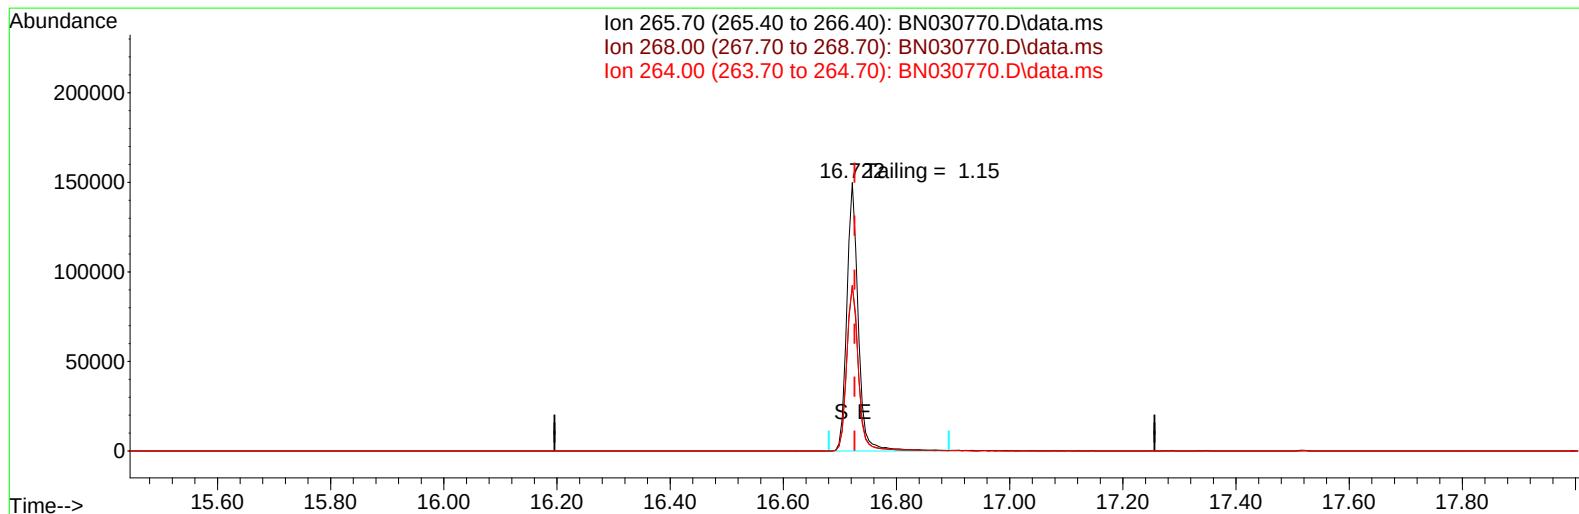

TIC: BN030770.D\data.ms

(70) Pentachlorophenol (C)




16.722min (-0.004) 21711.68 ng

response 209577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.66
264.00	61.60	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030770.D
Acq On : 08 Apr 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 17:14:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

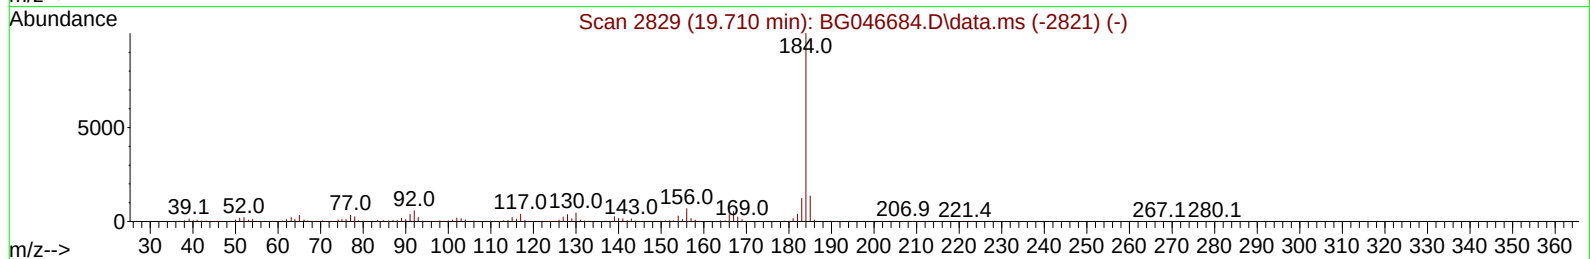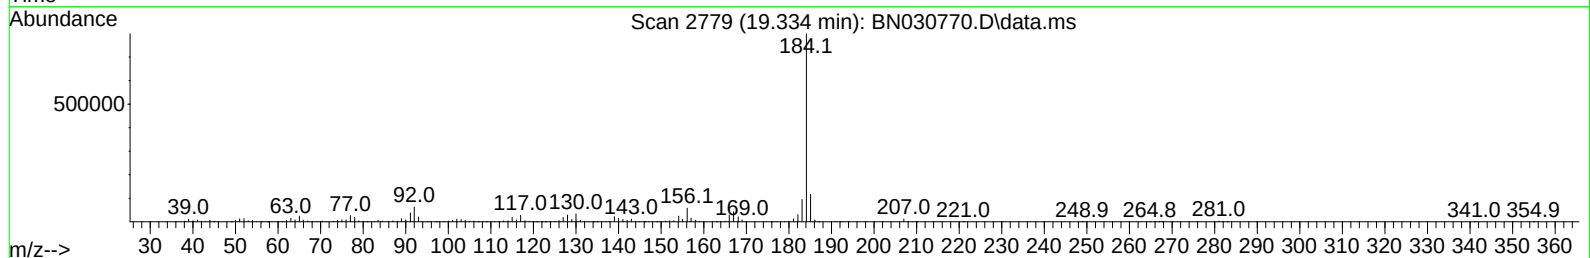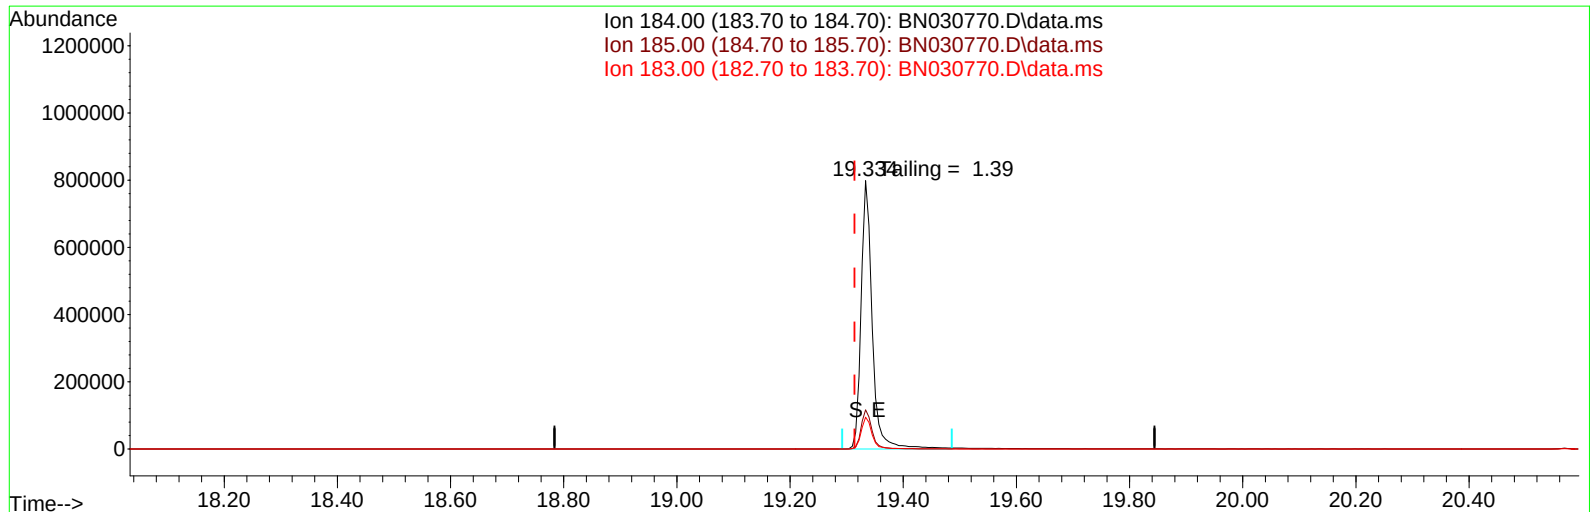

TIC: BN030770.D\data.ms

(77) Benzidine**19.334min (+ 0.019) 0.00 ng****response 1094908**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	11.88
0.00	0.00	0.00