
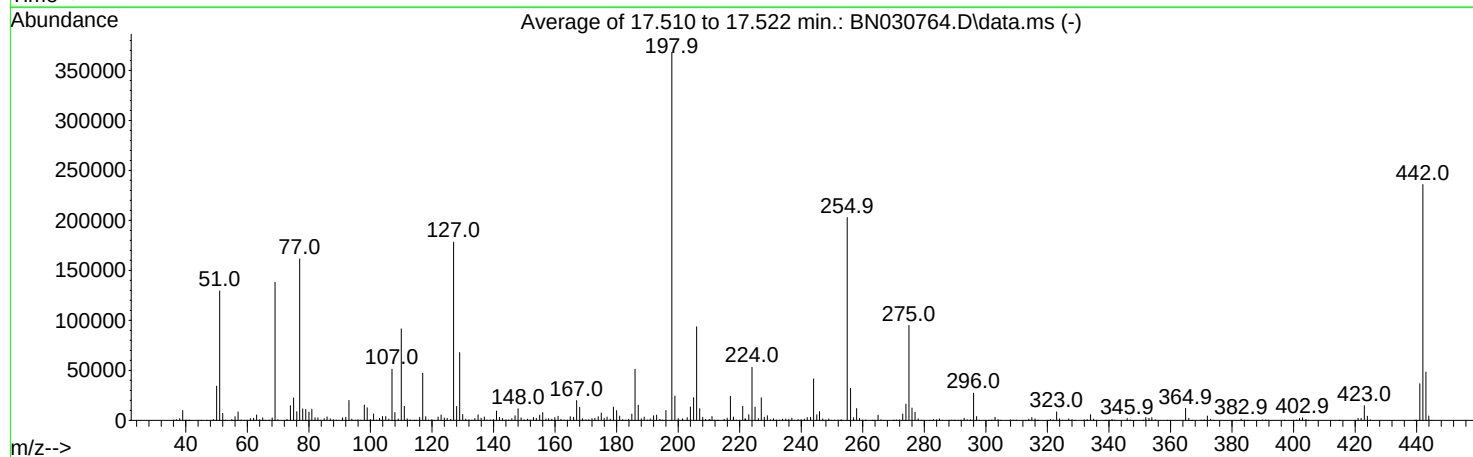


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030764.D
Acq On : 08 Apr 2024 09:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN033024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 00:04:36 2024

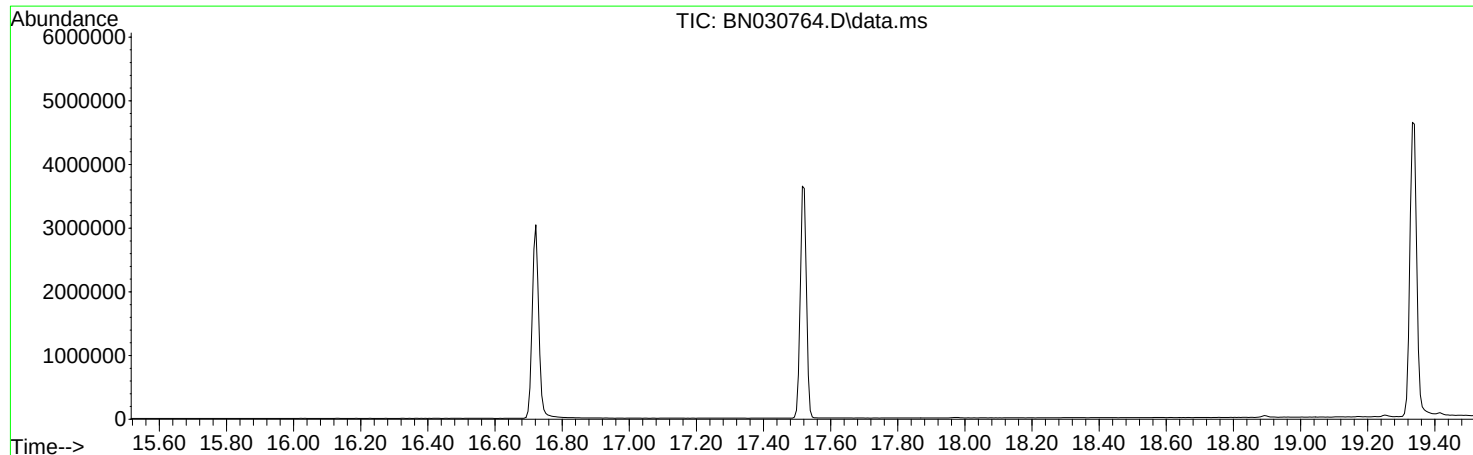




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	129448	PASS
68	69	0.00	2	1.8	2518	PASS
69	198	0.00	100	37.6	138192	PASS
70	69	0.00	2	0.5	717	PASS
127	198	10	80	48.5	178325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	367957	PASS
199	198	5	9	6.6	24312	PASS
275	198	10	60	25.8	94976	PASS
365	198	1	100	3.3	11973	PASS
441	198	0.01	100	10.0	36728	PASS
442	442	50	100	100.0	235920	PASS
443	442	15	24	20.5	48371	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030764.D
Acq On : 08 Apr 2024 09:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 09 17:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

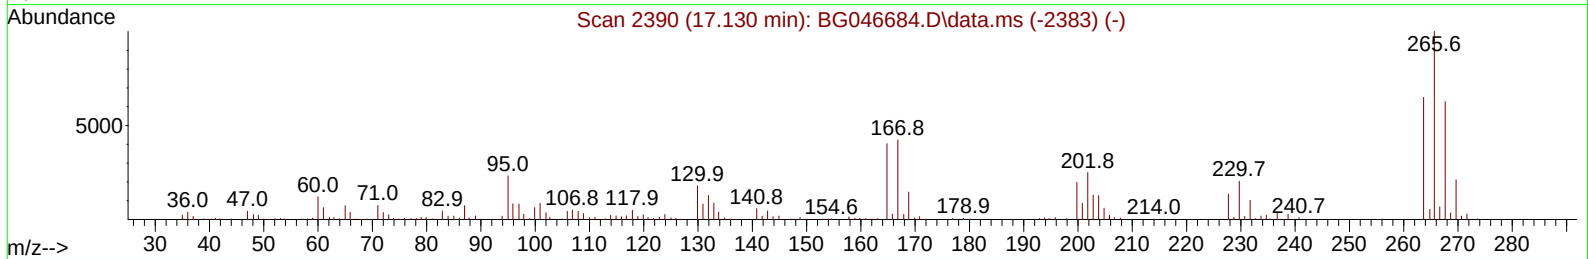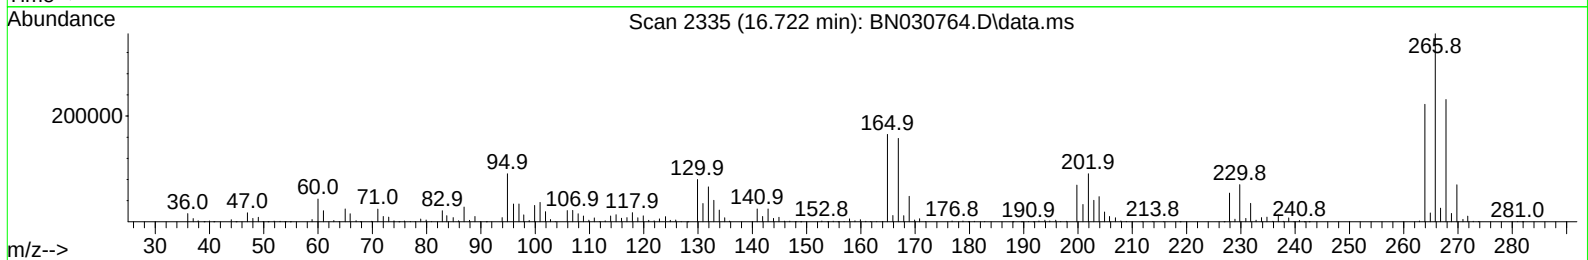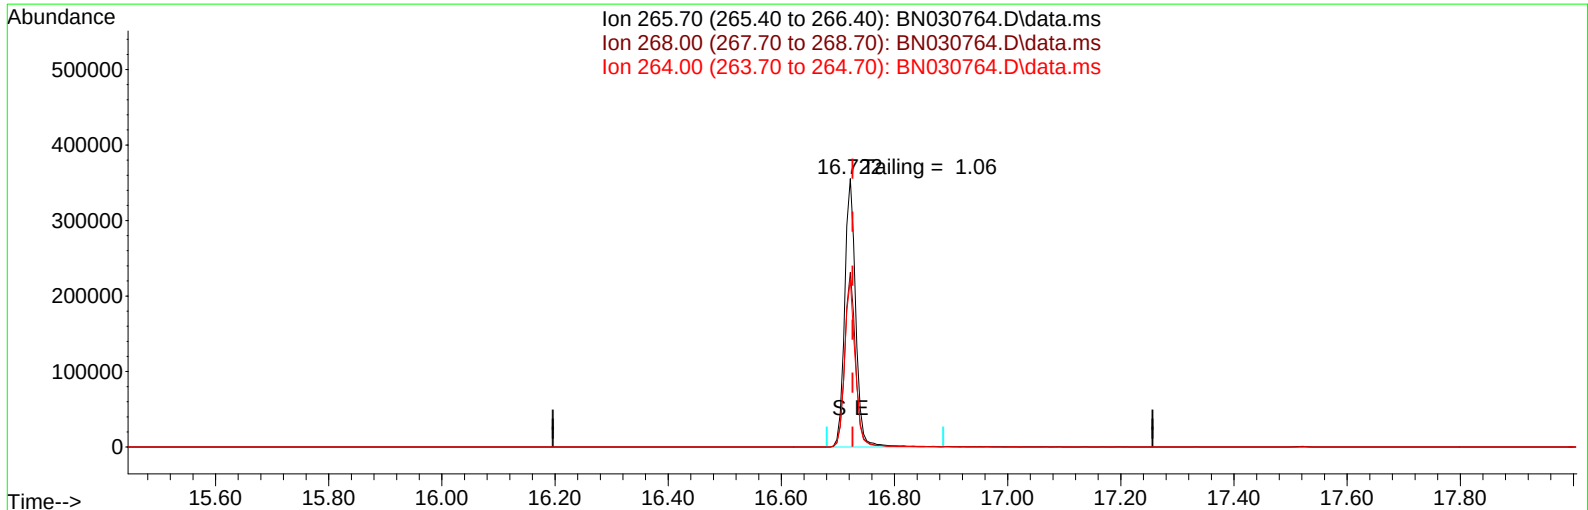

TIC: BN030764.D\data.ms

(70) Pentachlorophenol (C)

16.722min (-0.004) 26686.45 ng




response 481895

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.08
264.00	61.60	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030764.D
Acq On : 08 Apr 2024 09:35
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 09 17:09:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

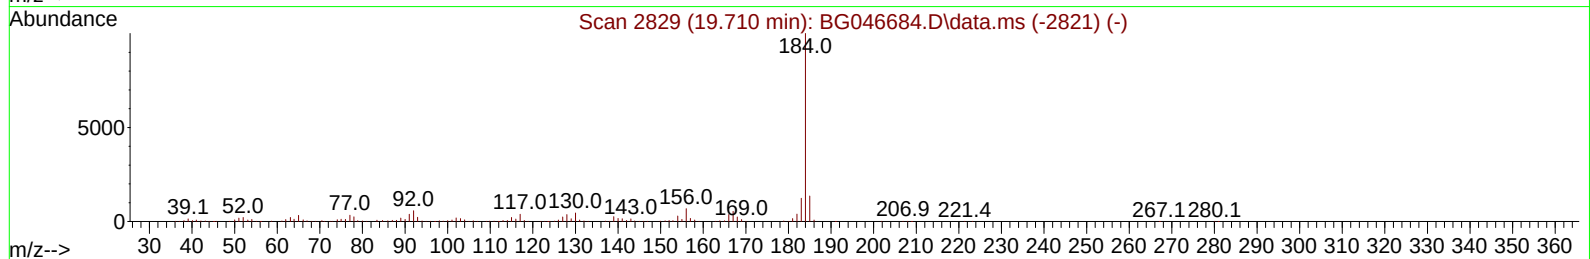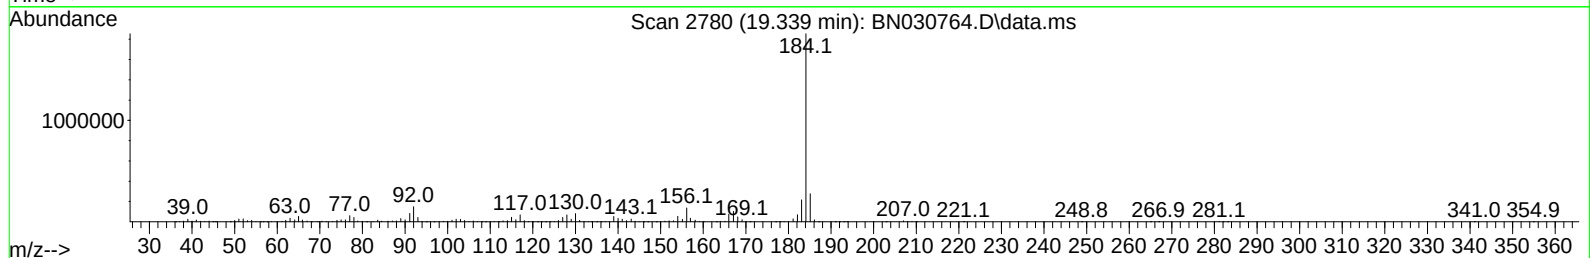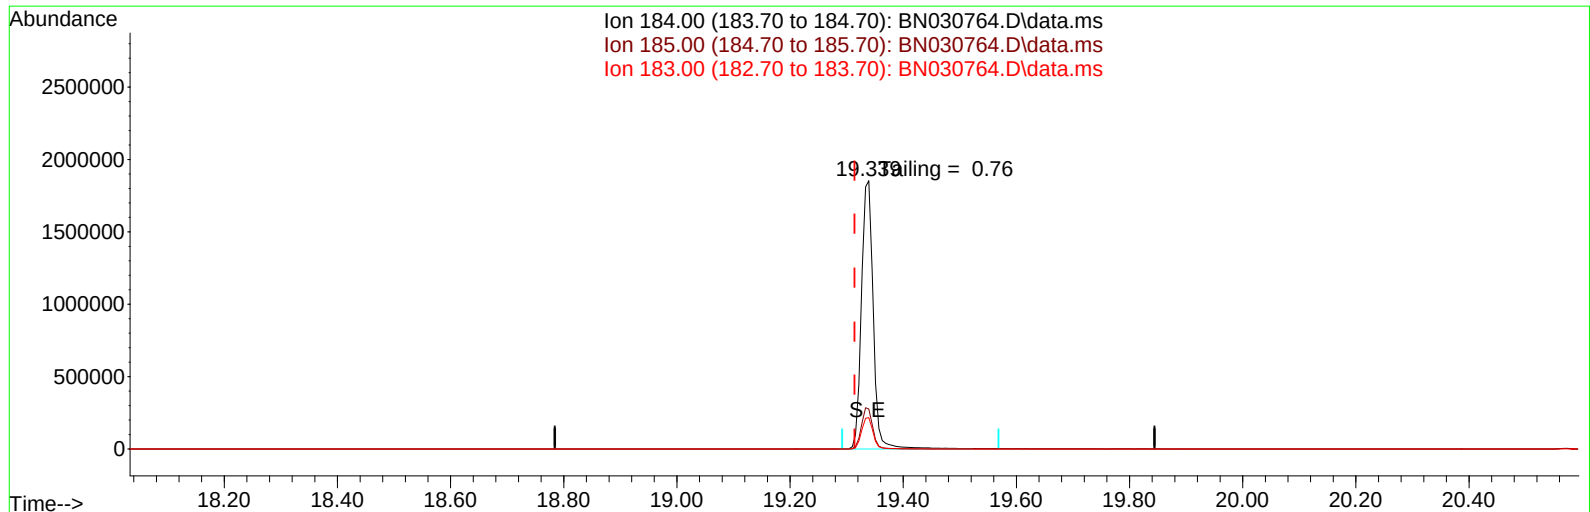

TIC: BN030764.D\data.ms

(77) Benzidine

19.339min (+ 0.025) 0.00 ng

response 2705724

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.93
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2024	BNA_N	<u>BN030764.D</u>
Compound Name	Response	Retention Time
DDT	1346489	20.569
DDD	64060	20.127
DDE	2888	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
66948	1413437	4.74

Instrument :
BNA_N
ClientSampleId :
DFTPP