


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030770.D
Acq On : 08 Apr 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN033024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 00:04:36 2024

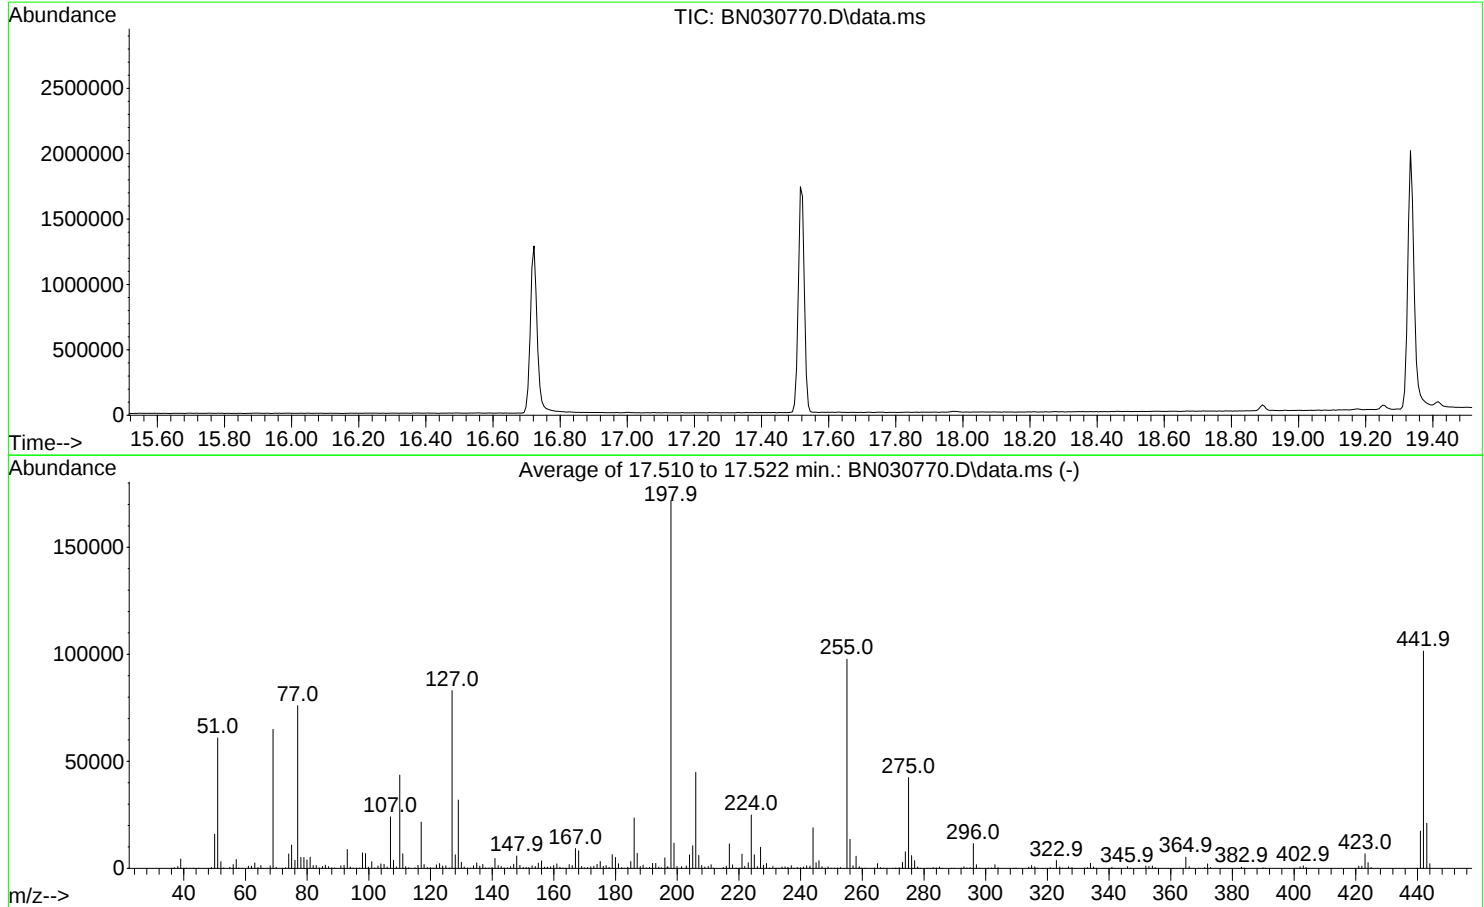




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	60901	PASS
68	69	0.00	2	1.9	1222	PASS
69	198	0.00	100	37.8	64949	PASS
70	69	0.00	2	0.7	441	PASS
127	198	10	80	48.3	83072	PASS
197	198	0.00	2	0.5	811	PASS
198	198	100	100	100.0	171861	PASS
199	198	5	9	6.9	11853	PASS
275	198	10	60	24.7	42387	PASS
365	198	1	100	3.0	5226	PASS
441	198	0.01	100	10.2	17449	PASS
442	442	50	100	100.0	101525	PASS
443	442	15	24	20.7	21065	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030770.D
Acq On : 08 Apr 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 09 17:14:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

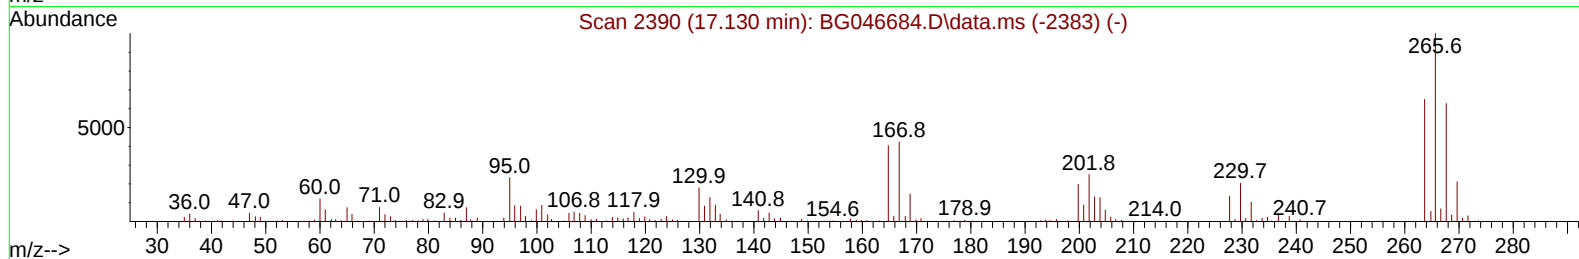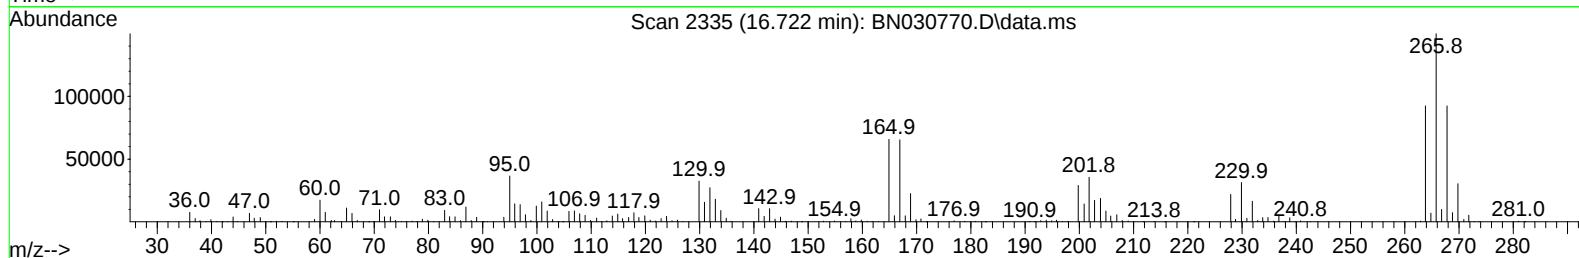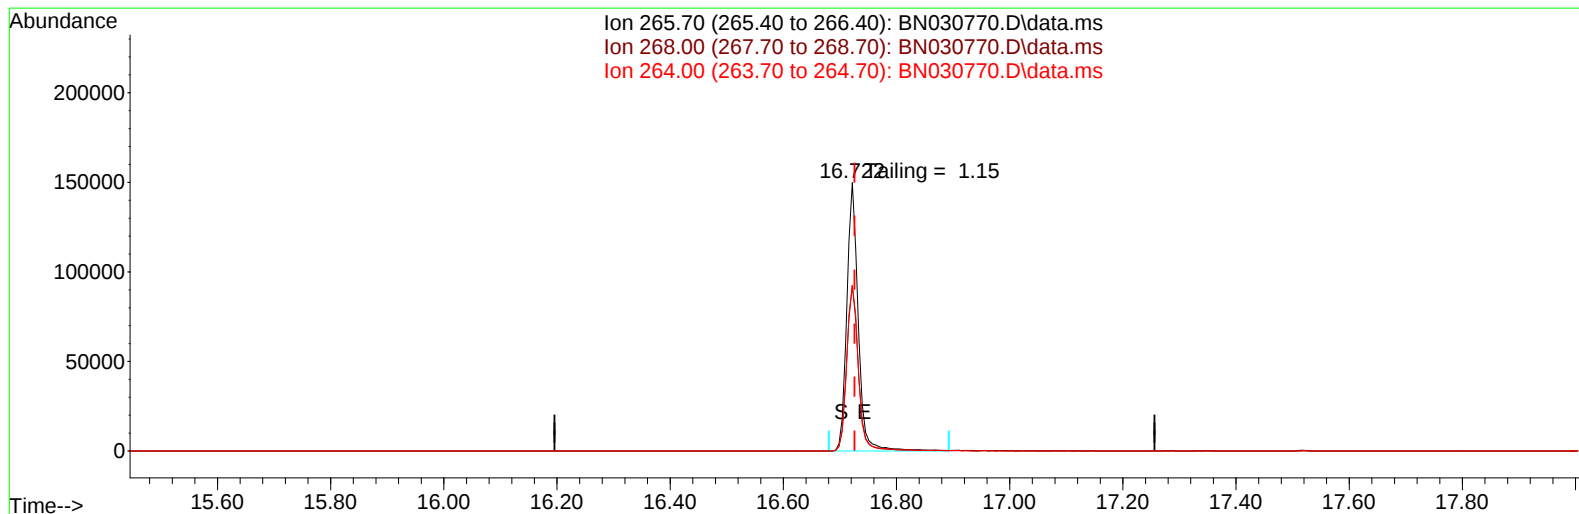

TIC: BN030770.D\data.ms

(70) Pentachlorophenol (C)

16.722min (-0.004) 21711.68 ng




response 209577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.66
264.00	61.60	61.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040824\
Data File : BN030770.D
Acq On : 08 Apr 2024 15:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 09 17:14:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

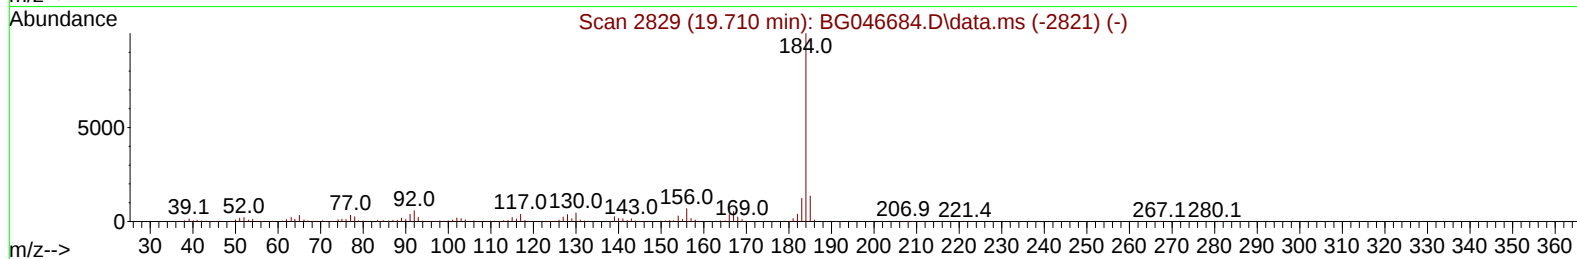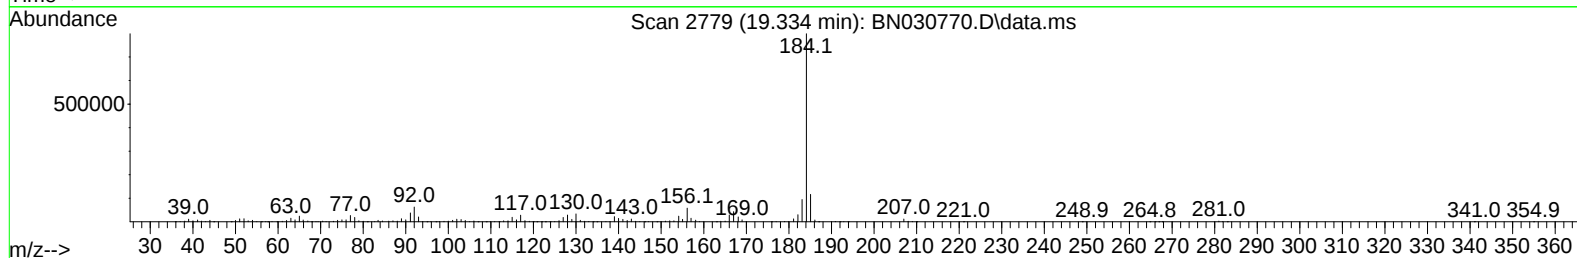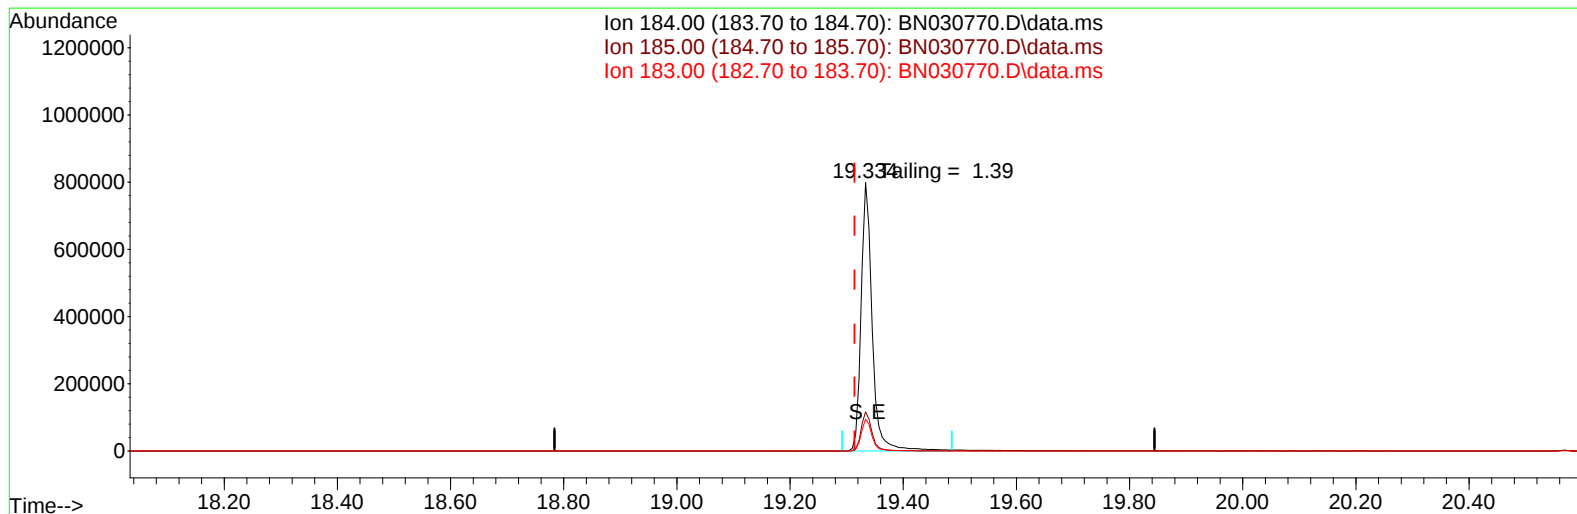

TIC: BN030770.D\data.ms

(77) Benzidine

19.334min (+ 0.019) 0.00 ng

response 1094908

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.61
183.00	13.20	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/8/2024	BNA_N	<u>BN030770.D</u>
Compound Name	Response	Retention Time
DDT	593111	20.569
DDD	41638	20.128
DDE	1468	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43106	636217	6.78

Instrument :
BNA_N
ClientSampleId :
DFTPP