
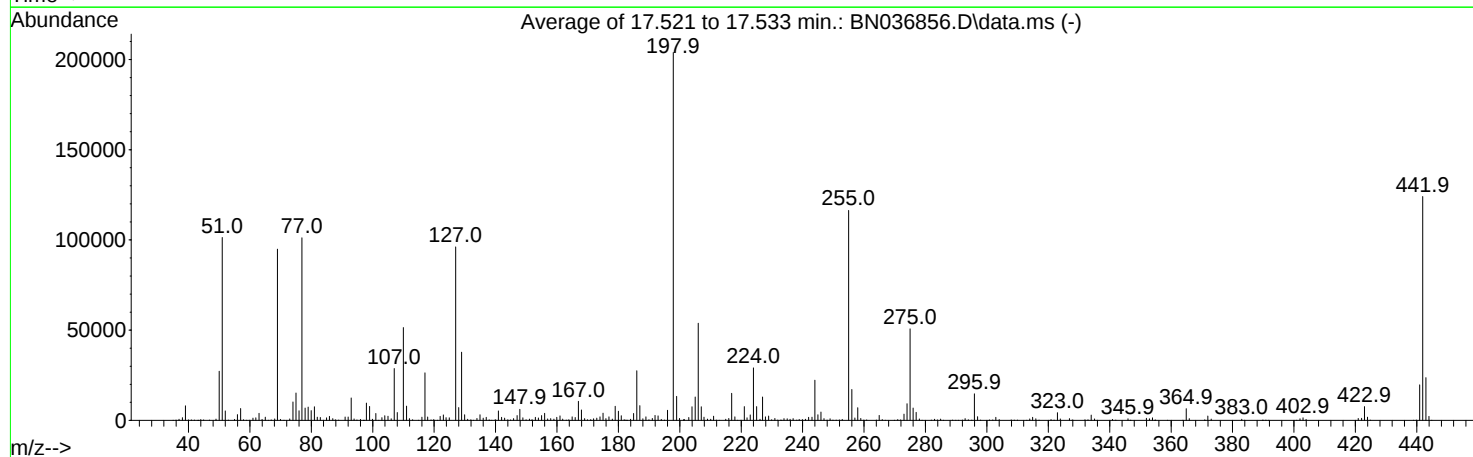


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040825\
Data File : BN036856.D
Acq On : 08 Apr 2025 09:56
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 04 17:30:43 2025

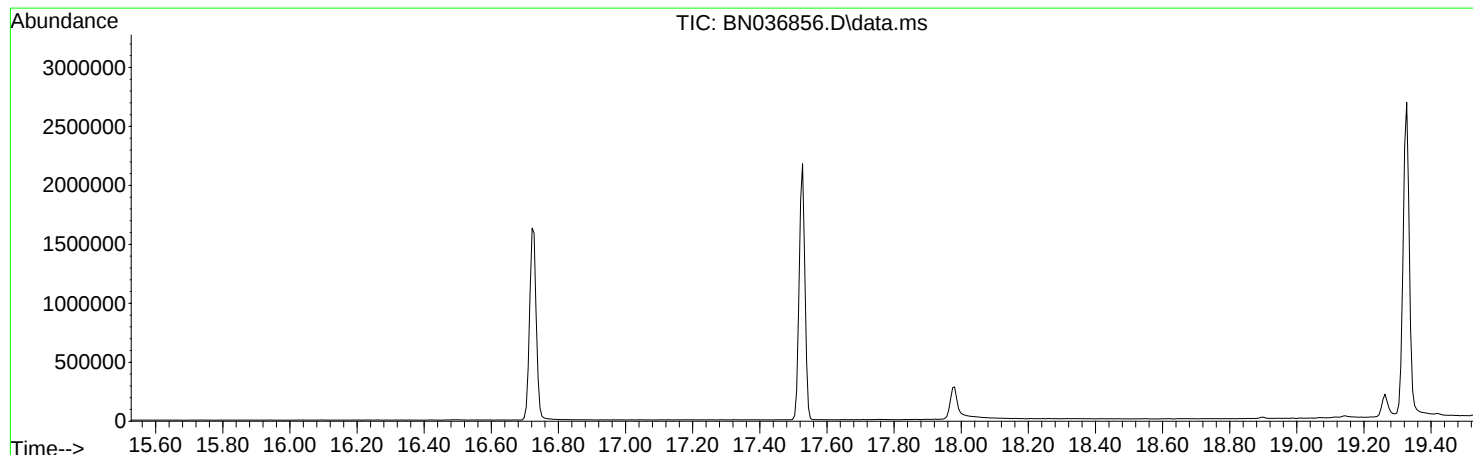

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	101421	PASS
68	69	0.00	2	0.8	771	PASS
69	198	0.00	100	46.6	94920	PASS
70	69	0.00	2	0.6	542	PASS
127	198	10	80	47.2	96163	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	203904	PASS
199	198	5	9	6.5	13269	PASS
275	198	10	60	24.9	50715	PASS
365	198	1	100	3.2	6499	PASS
441	198	0.01	100	9.7	19731	PASS
442	442	50	100	100.0	124123	PASS
443	442	15	24	19.0	23640	PASS