
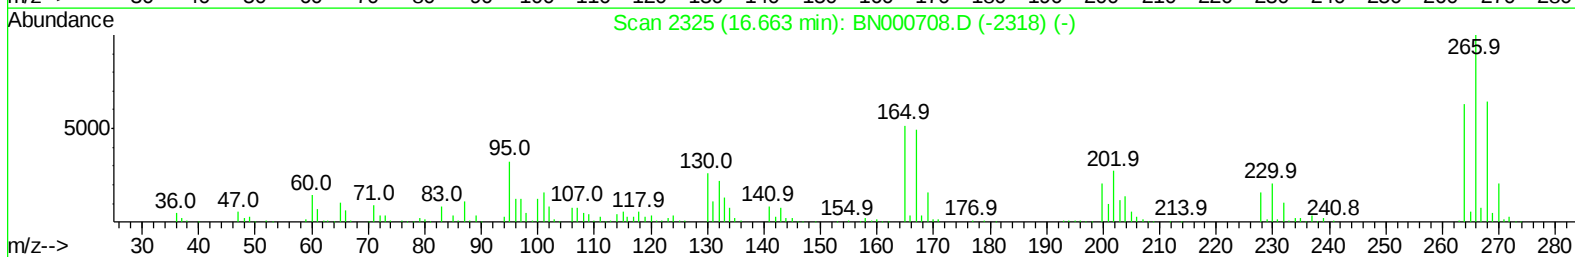
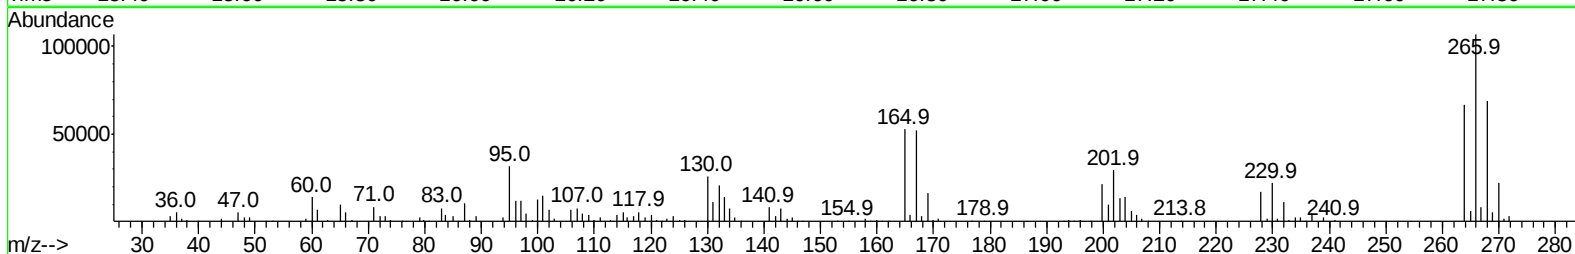


Data Path : Z:\HPCHEM1\BNA N\DATA\BN040918\
Data File : BN000713.D
Acq On : 09 Apr 2018 17:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 05:37:17 2018
Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN040918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 09 13:41:40 2018
Response via : Initial Calibration

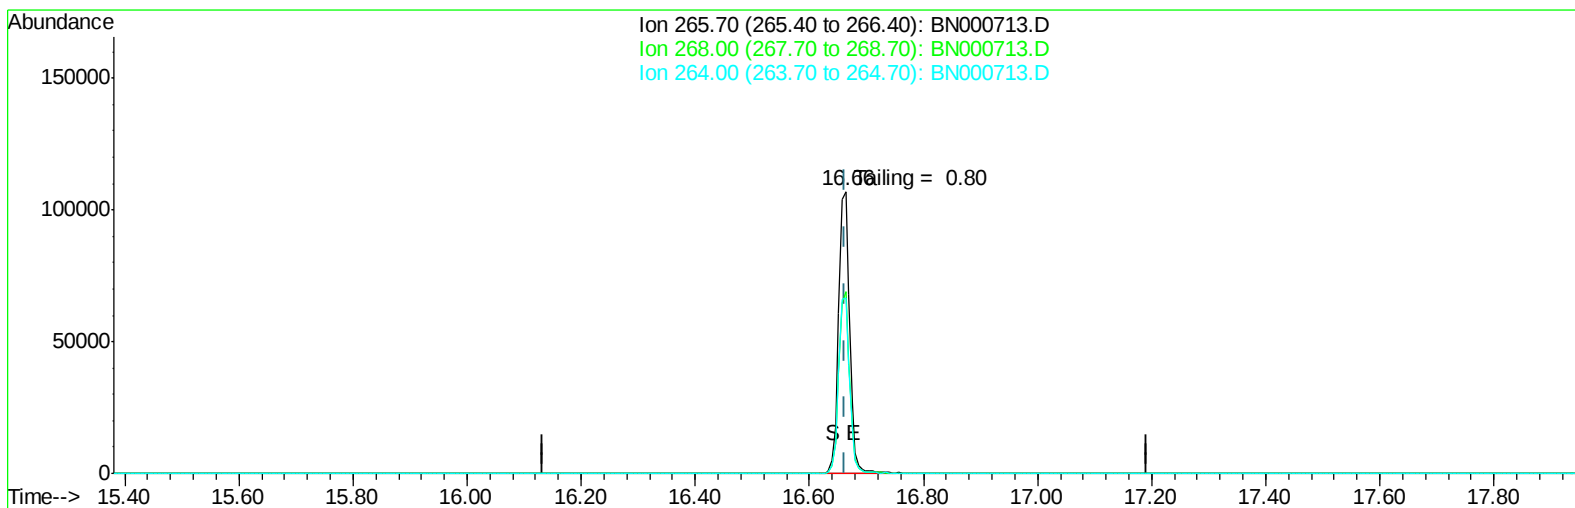

TIC: BN000713.D

(69) Pentachlorophenol (C)




16.663min (+0.000) 27004.66ng

response 143934

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.64
264.00	62.00	62.36
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA N\DATA\BN040918\
 Data File : BN000713.D
 Acq On : 09 Apr 2018 17:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 05:37:17 2018
 Quant Method : Z:\HPCHEM1\BNA N\METHODS\8270-BN040918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 09 13:41:40 2018
 Response via : Initial Calibration

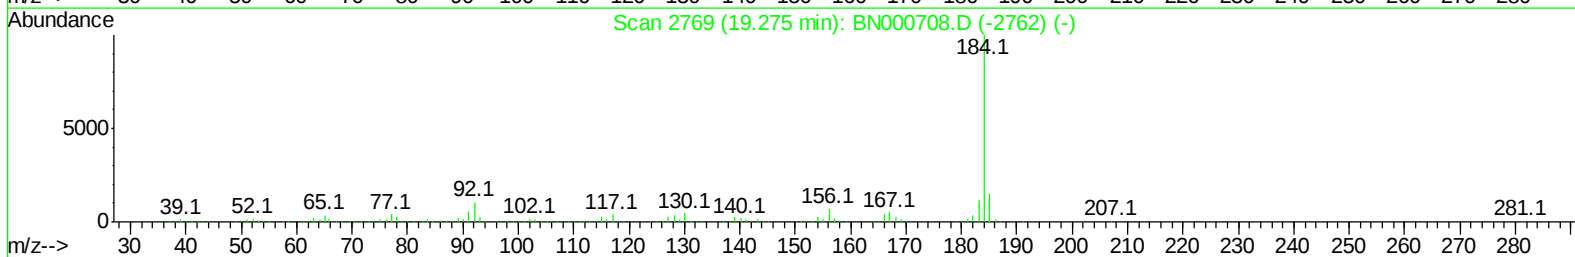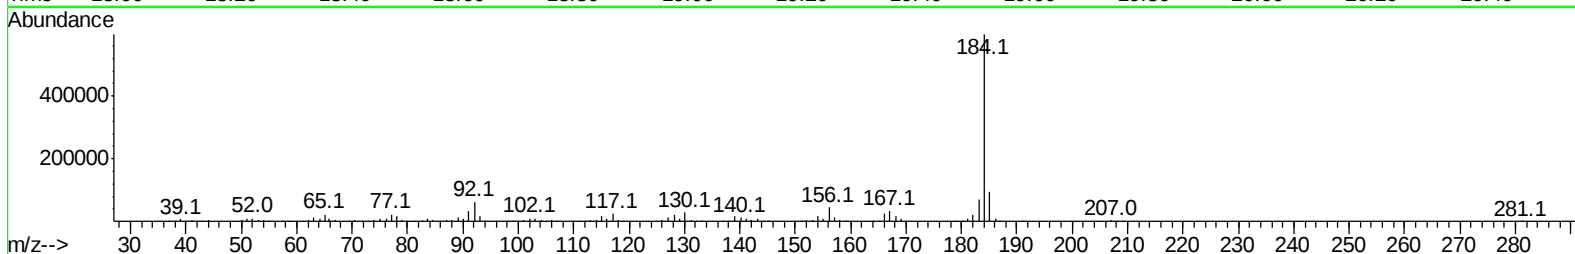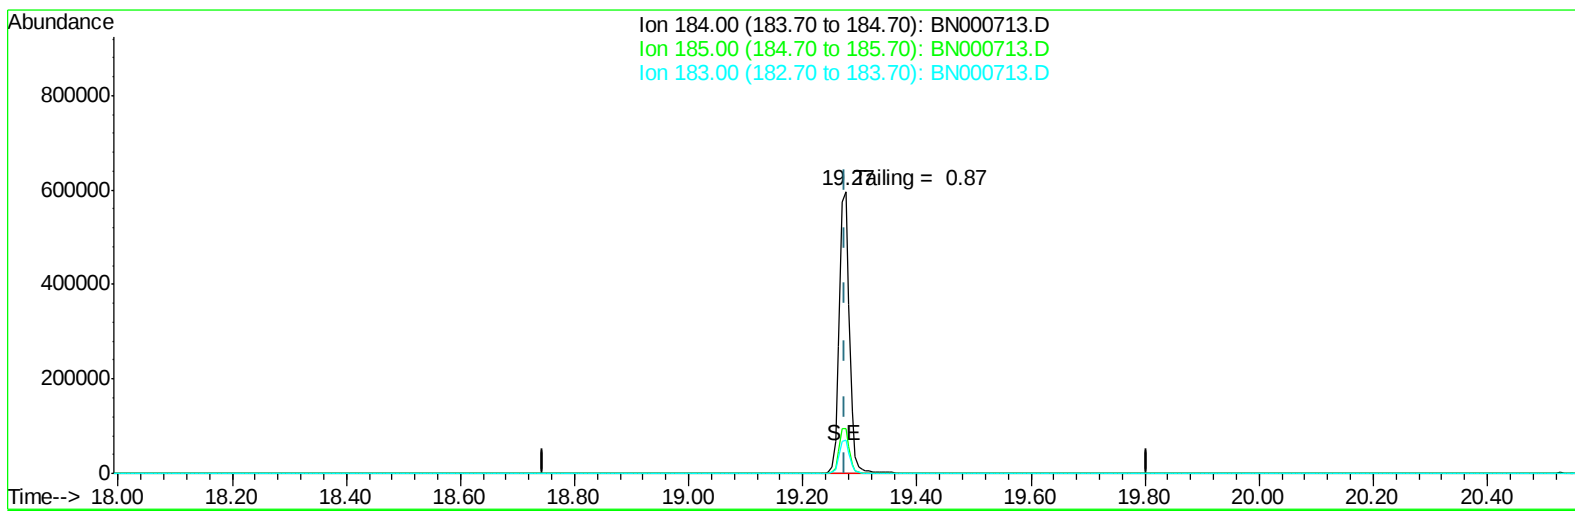

TIC: BN000713.D

(76) Benzidine

19.275min (+0.000) 0.00ng

response 744006

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.93
183.00	13.30	11.74
0.00	0.00	0.00