


Data Path : Z:\HPCHEM1\BNA N\Data\BN040918\
 Data File : BN000704.D
 Acq On : 09 Apr 2018 08:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN040918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 09 13:41:40 2018

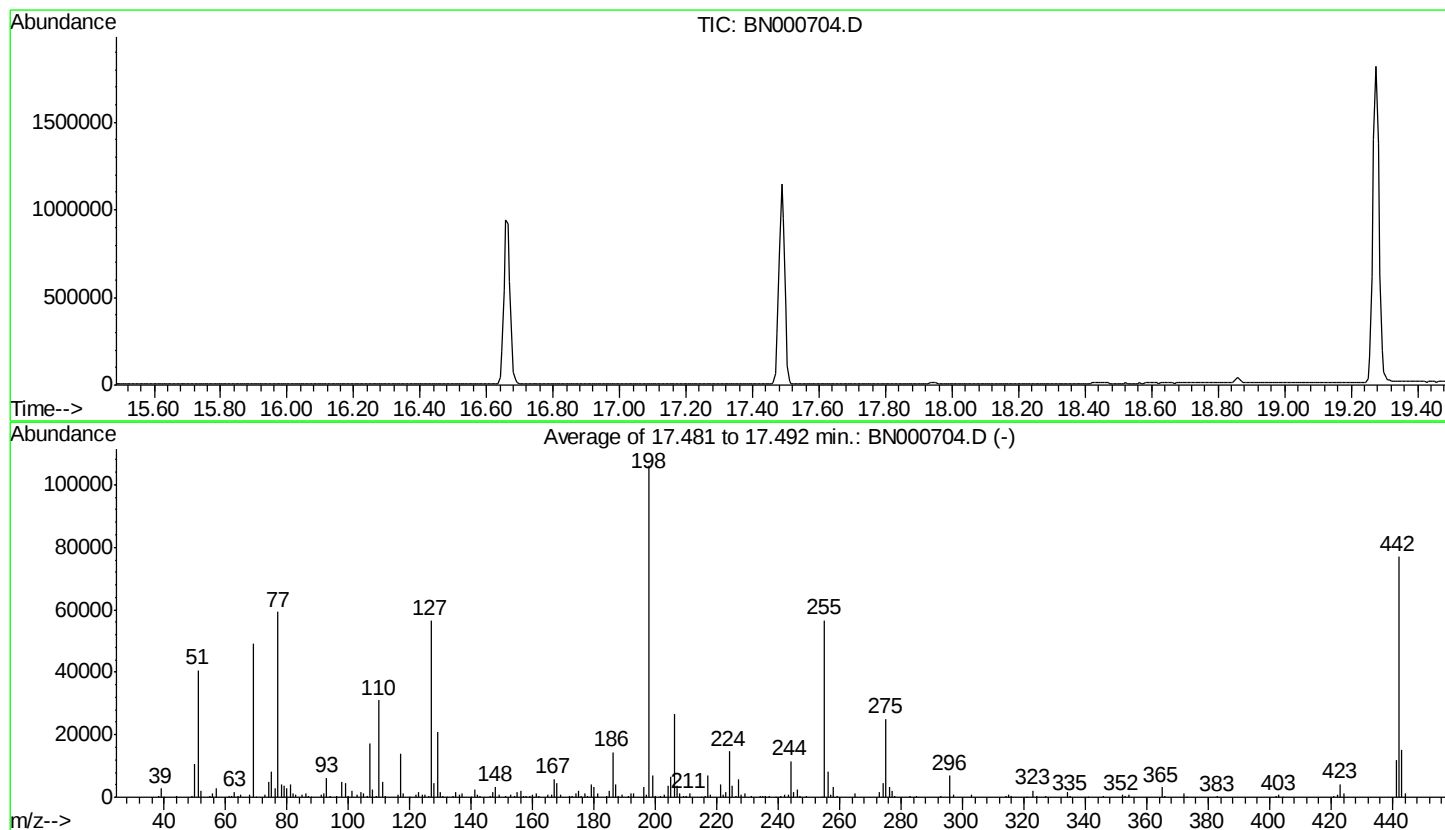

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	40581	PASS
68	69	0.00	2	1.9	928	PASS
69	198	0.00	100	46.2	49002	PASS
70	69	0.00	2	0.2	111	PASS
127	198	10	80	53.1	56376	PASS
197	198	0.00	2	0.8	815	PASS
198	198	100	100	100.0	106122	PASS
199	198	5	9	6.7	7059	PASS
275	198	10	60	23.7	25176	PASS
365	198	1	100	2.9	3096	PASS
441	443	0.01	100	79.1	12094	PASS
442	198	50	100	72.4	76832	PASS
443	442	15	24	19.9	15285	PASS