


Data Path : Z:\HPCHEM1\BNA N\Data\BN040918\
Data File : BN000713.D
Acq On : 09 Apr 2018 17:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_N\METHODS\8270-BN040918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 09 13:41:40 2018

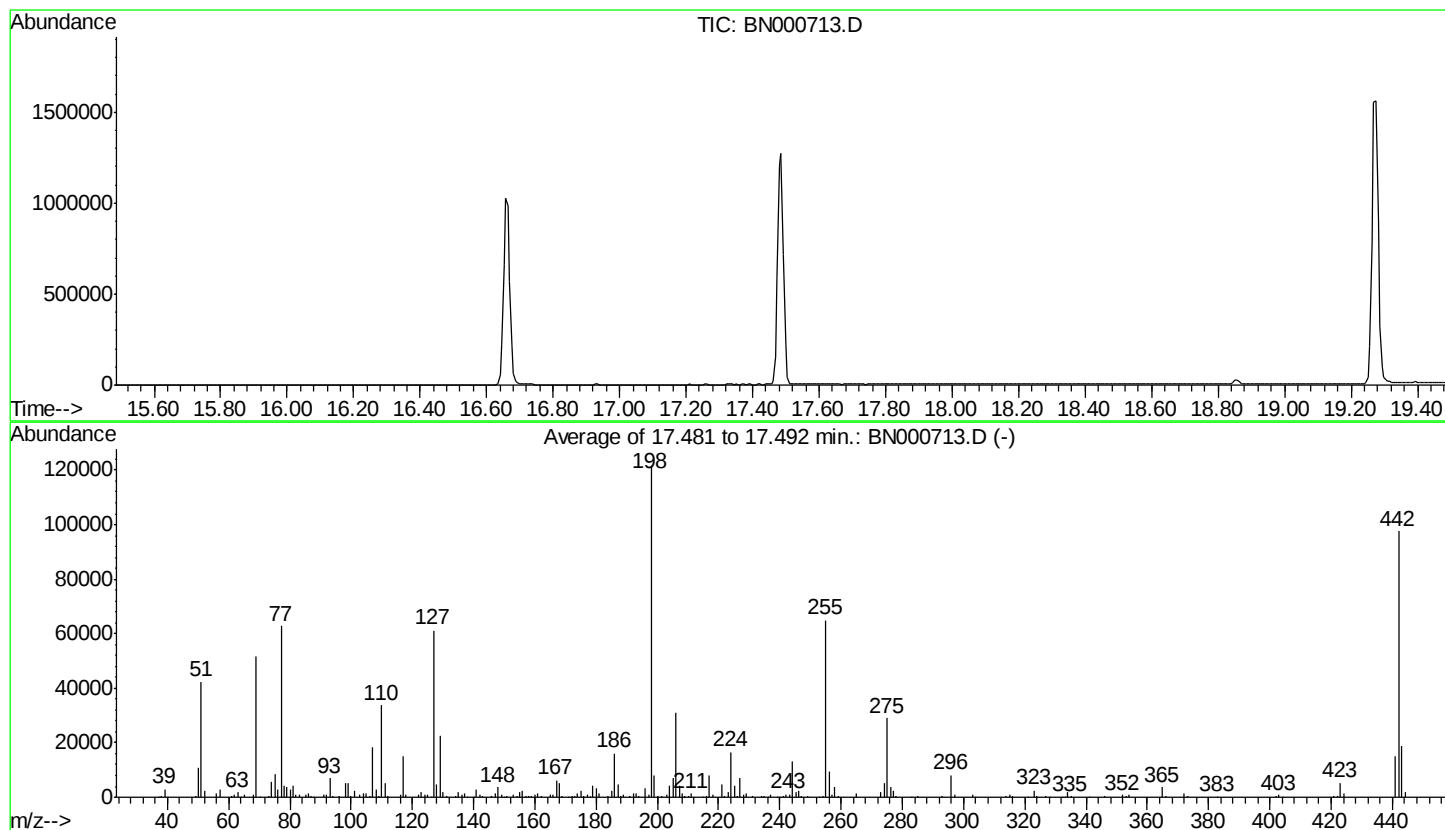

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	42338	PASS
68	69	0.00	2	1.8	915	PASS
69	198	0.00	100	42.4	51589	PASS
70	69	0.00	2	0.4	220	PASS
127	198	10	80	50.3	61186	PASS
197	198	0.00	2	0.8	924	PASS
198	198	100	100	100.0	121621	PASS
199	198	5	9	6.6	8008	PASS
275	198	10	60	23.9	29088	PASS
365	198	1	100	3.1	3745	PASS
441	443	0.01	100	79.7	14930	PASS
442	198	50	100	80.3	97637	PASS
443	442	15	24	19.2	18728	PASS