

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040919\
 Data File : BN005116.D
 Acq On : 09 Apr 2019 17:15
 Operator : JU/SJ
 Sample : PB118726BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB118726BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	379	384	391	rBB	108163	146750	45.05%	8.134%
2	6.828	647	653	659	rBV	101196	152609	46.84%	8.459%
3	7.187	708	714	720	rBB	113399	170081	52.21%	9.427%
4	7.652	788	793	798	rBB	23267	33021	10.14%	1.830%
5	7.969	841	847	852	rBB	83427	129619	39.79%	7.184%
6	8.816	985	991	997	rBB	58905	91012	27.94%	5.045%
7	10.434	1260	1266	1273	rBB	31834	49309	15.14%	2.733%
8	12.910	1681	1687	1694	rBB	174577	253476	77.81%	14.049%
9	14.298	1918	1923	1929	rBB2	45901	66726	20.48%	3.698%
10	15.798	2173	2178	2185	rBB	125945	167657	51.46%	9.293%
11	17.051	2386	2391	2397	rBB2	54843	73508	22.56%	4.074%
12	19.686	2834	2839	2844	rBV	284403	325780	100.00%	18.057%
13	21.251	3101	3105	3111	rBV	58588	72589	22.28%	4.023%
14	23.486	3478	3485	3493	rBV	40989	72038	22.11%	3.993%


Sum of corrected areas: 1804175

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040919\
Data File : BN005116.D
Acq On : 09 Apr 2019 17:15
Operator : JU/SJ
Sample : PB118726BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118726BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

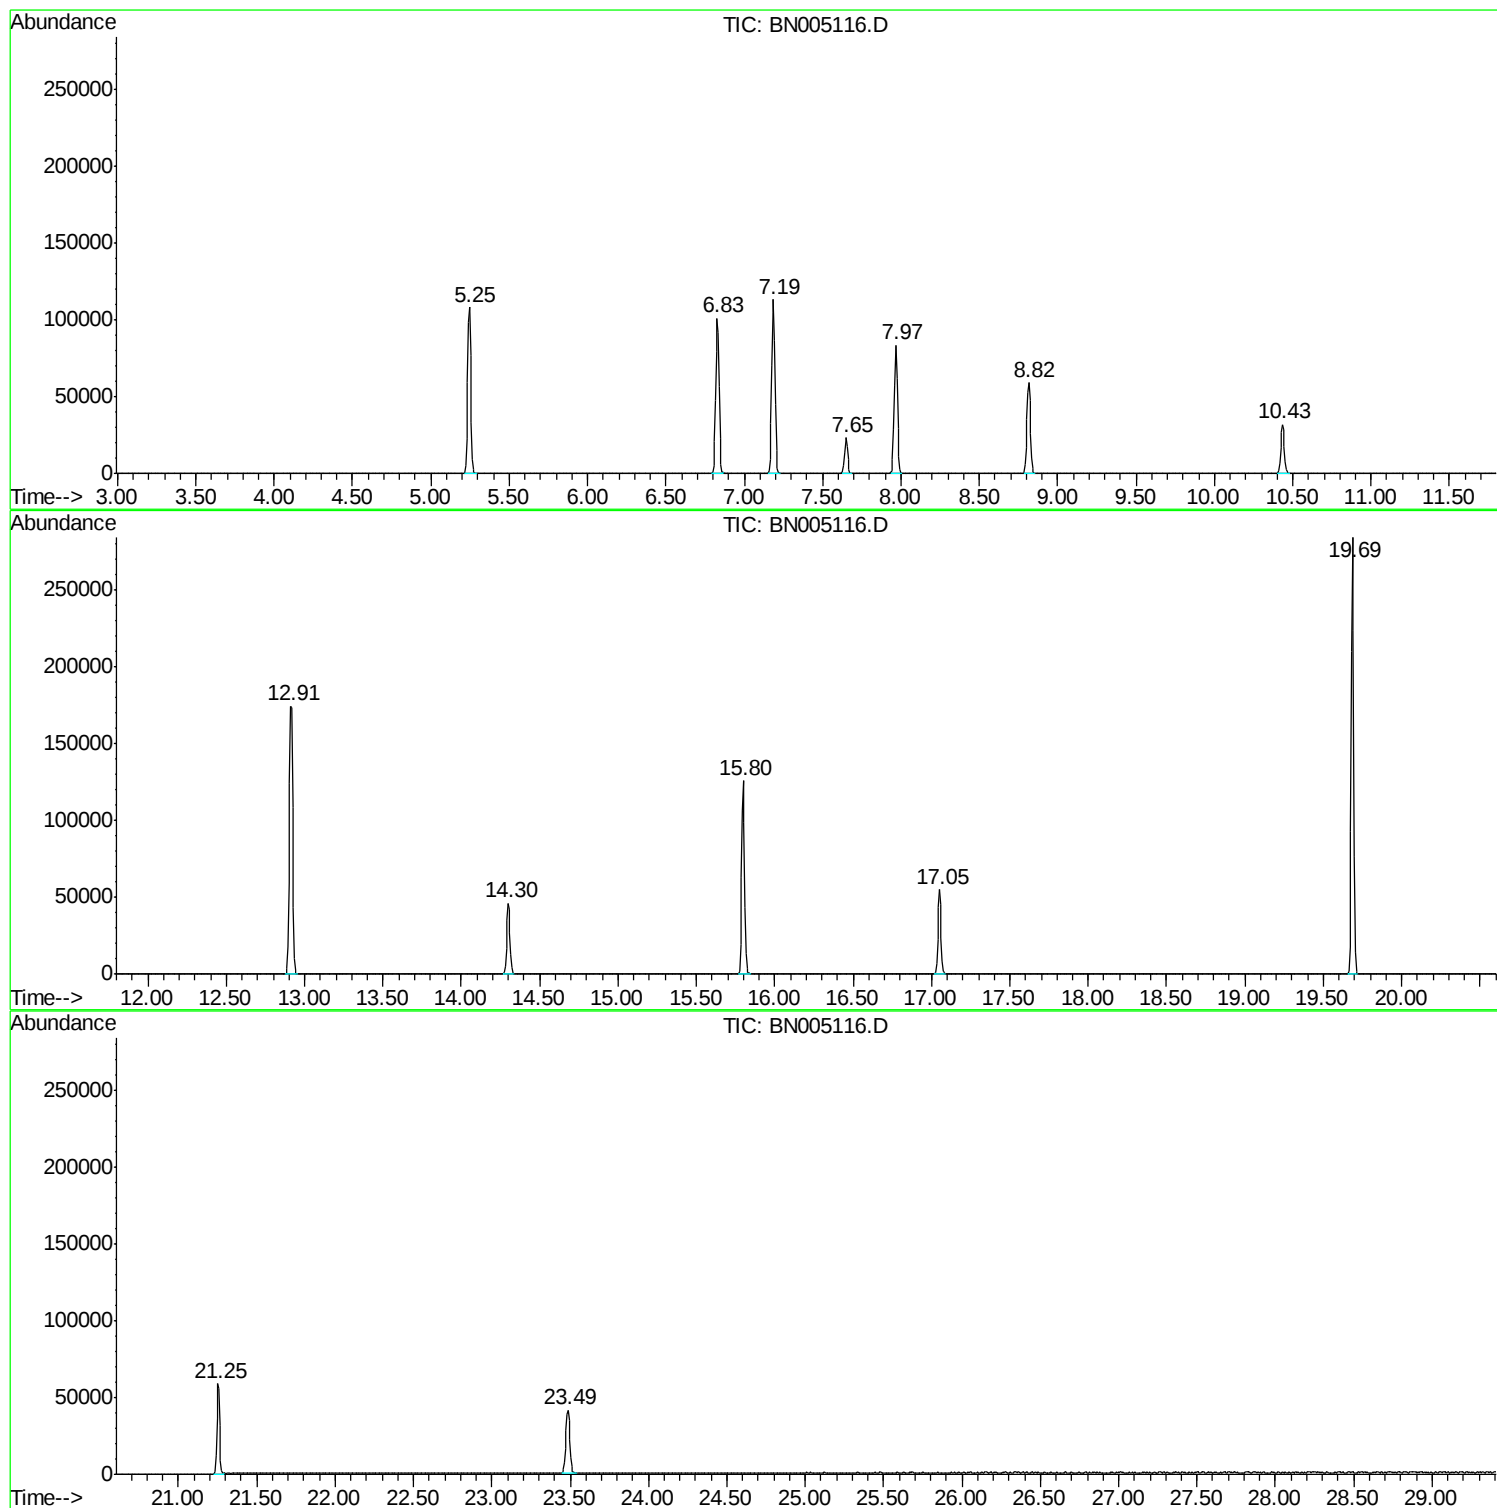

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040919\
Data File : BN005116.D
Acq On : 09 Apr 2019 17:15
Operator : JU/SJ
Sample : PB118726BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118726BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	103.01 ng	170081	1,4-Dichlorobenzene-d4	7.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	16
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	12
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

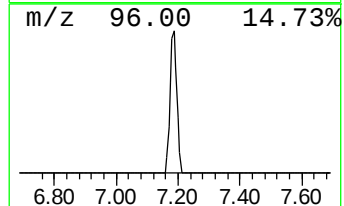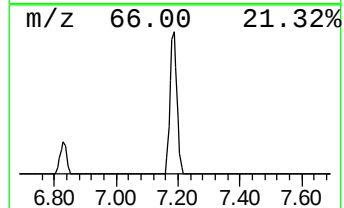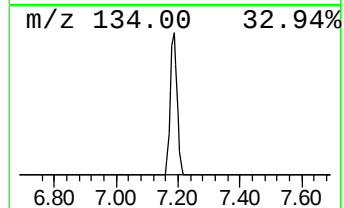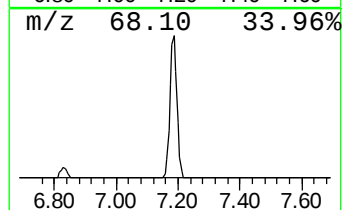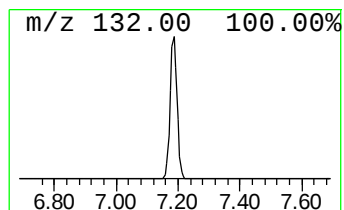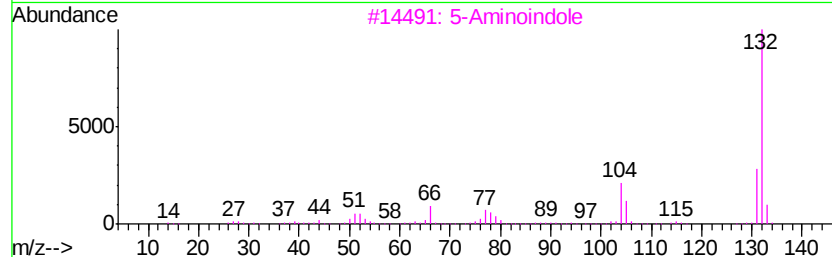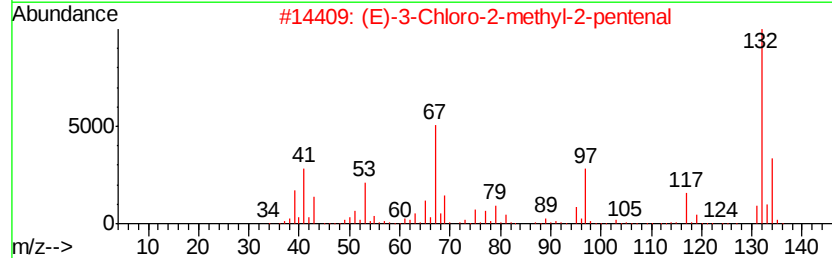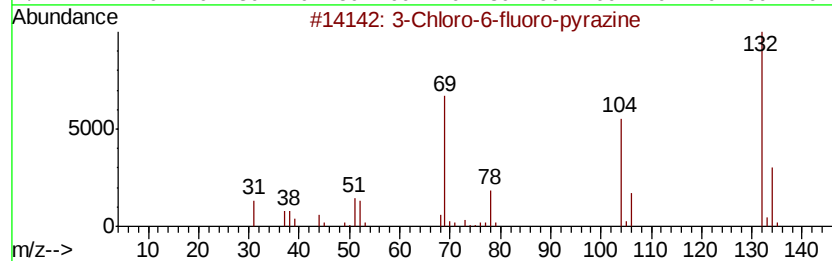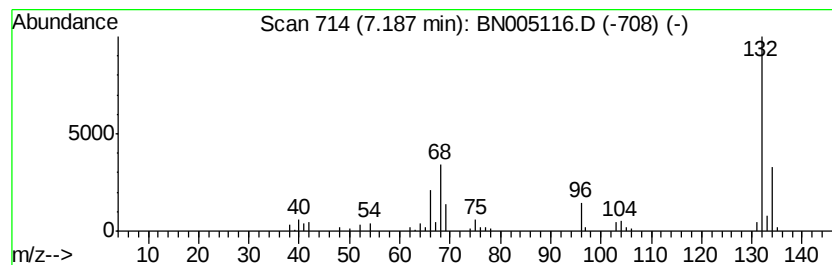

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040919\
Data File : BN005116.D
Acq On : 09 Apr 2019 17:15
Operator : JU/SJ
Sample : PB118726BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB118726BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	103.0	ng	170081	1	7.65	33021	20.0