


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040919\
 Data File : BN005113.D
 Acq On : 09 Apr 2019 14:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-BN032619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 27 05:27:09 2019

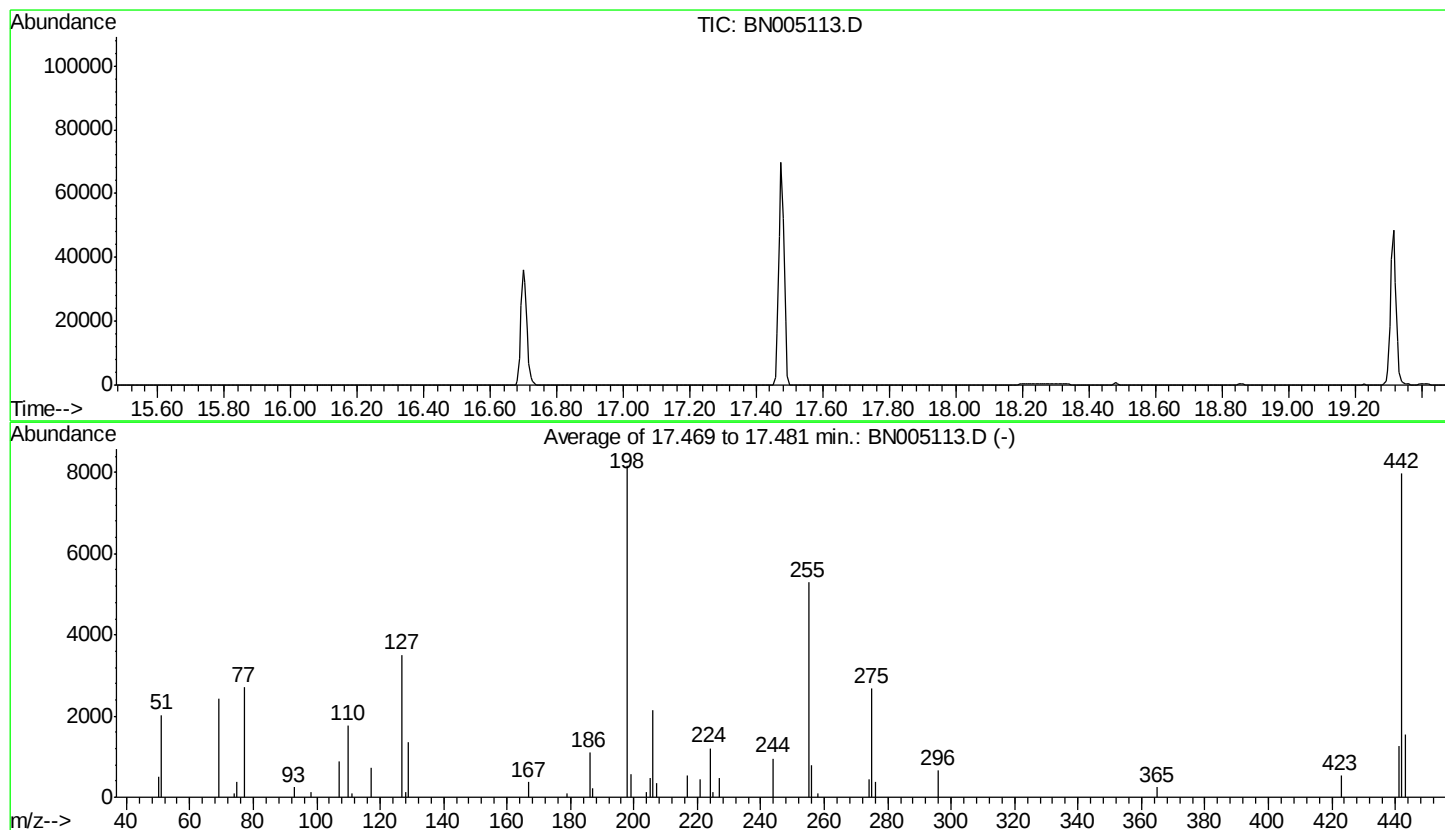

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	2023	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.9	2442	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	3507	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8170	PASS
199	198	5	9	7.0	569	PASS
275	198	10	60	32.7	2668	PASS
365	198	1	100	3.1	250	PASS
441	198	0.01	100	15.5	1268	PASS
442	198	50	100	97.6	7973	PASS
443	442	15	24	19.3	1536	PASS