

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
 Data File : BN014248.D
 Acq On : 09 Apr 2021 11:32
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Apr 09 12:50:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 12:42:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	7627	0.40	ng	0.00
7) Naphthalene-d8	10.492	136	28100	0.40	ng	0.00
13) Acenaphthene-d10	14.346	164	15531	0.40	ng	0.00
19) Phenanthrene-d10	17.092	188	34557	0.40	ng	0.00
29) Chrysene-d12	21.282	240	34779	0.40	ng	0.00
36) Perylene-d12	23.520	264	33156	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.316	112	3676	0.18	ng	0.00
5) Phenol-d6	6.879	99	4499	0.16	ng	0.00
8) Nitrobenzene-d5	8.857	82	3292	0.17	ng	0.00
11) 2-Methylnaphthalene-d10	12.084	152	8356	0.18	ng	0.00
14) 2,4,6-Tribromophenol	15.831	330	1107	0.14	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	10898	0.20	ng	0.00
27) Fluoranthene-d10	19.124	212	19279	0.19	ng	0.00
31) Terphenyl-d14	19.729	244	15060	0.19	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.279	88	2000	0.24	ng	94
3) n-Nitrosodimethylamine	3.633	42	661	0.14	ng	# 80
6) bis(2-Chloroethyl)ether	7.153	93	3635	0.19	ng	98
9) Naphthalene	10.543	128	13531	0.19	ng	99
10) Hexachlorobutadiene	10.834	225	2788	0.20	ng	# 98
12) 2-Methylnaphthalene	12.160	142	8837	0.17	ng	99
16) Acenaphthylene	14.067	152	10637	0.15	ng	99
17) Acenaphthene	14.409	154	8276	0.19	ng	100
18) Fluorene	15.399	166	10406	0.18	ng	100
20) 4,6-Dinitro-2-methylph...	15.463	198	706	0.21	ng	# 39
21) 4-Bromophenyl-phenylether	16.289	248	3406	0.18	ng	98
22) Hexachlorobenzene	16.398	284	4341	0.21	ng	100
23) Atrazine	16.556	200	2426	0.13	ng	99
24) Pentachlorophenol	16.739	266	1156	0.13	ng	98
25) Phenanthrene	17.128	178	18249	0.20	ng	100
26) Anthracene	17.226	178	14530	0.16	ng	99
28) Fluoranthene	19.153	202	20753	0.19	ng	99
30) Pyrene	19.521	202	21586	0.19	ng	100
32) Benzo(a)anthracene	21.271	228	18112	0.16	ng	99
33) Chrysene	21.314	228	20385	0.19	ng	96
34) Bis(2-ethylhexyl)phtha...	21.218	149	6329	0.09	ng	# 97
35) Indeno(1,2,3-cd)pyrene	25.772	276	25635	0.20	ng	99
37) Benzo(b)fluoranthene	22.849	252	20955	0.19	ng	# 94
38) Benzo(k)fluoranthene	22.894	252	22555	0.22	ng	# 93
39) Benzo(a)pyrene	23.421	252	17936	0.18	ng	# 90
40) Dibenzo(a,h)anthracene	25.786	278	21228	0.21	ng	95
41) Benzo(g,h,i)perylene	26.457	276	20884	0.20	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
Data File : BN014248.D
Acq On : 09 Apr 2021 11:32
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Apr 09 12:50:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 12:42:56 2021
Response via : Initial Calibration







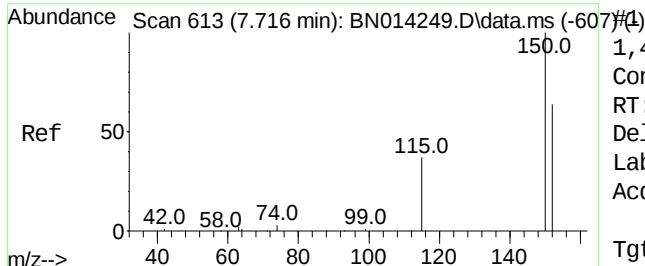

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.716 min Scan# 613
 Delta R.T. 0.000 min
 Lab File: BN014248.D
 Acq: 09 Apr 2021 11:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:	152	Resp:	7627
Ion	Ratio	Lower	Upper
152	100		
150	157.1	124.8	187.2
115	60.2	48.6	73.0



1,4-Dioxane
 Concen: 0.24 ng
 RT: 3.279 min Scan# 62
 Delta R.T. -0.008 min
 Lab File: BN014248.D
 Acq: 09 Apr 2021 11:32

Tgt Ion:	88	Resp:	2000
Ion	Ratio	Lower	Upper
88	100		
58	58.4	52.5	78.7
43	27.3	21.8	32.8









n-Nitrosodimethylamine
Concen: 0.14 ng
RT: 3.633 min Scan# 106
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion: 42 Resp: 661
Ion Ratio Lower Upper
42 100
74 163.2 111.2 166.8
44 22.2 12.5 18.7#



2-Fluorophenol
Concen: 0.18 ng
RT: 5.316 min Scan# 315
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion: 112 Resp: 3676
Ion Ratio Lower Upper
112 100
64 53.0 43.4 65.0
63 29.5 23.5 35.3







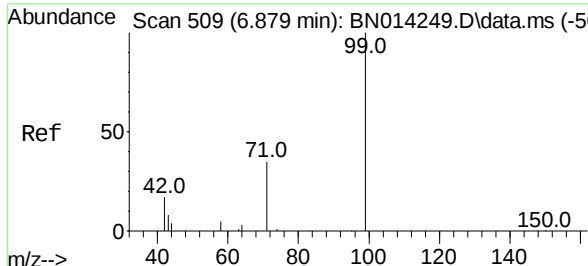

Phenol-d6
 Concen: 0.16 ng
 RT: 6.879 min Scan# 509
 Delta R.T. -0.000 min
 Lab File: BN014248.D
 Acq: 09 Apr 2021 11:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	99	Resp:	4499
Ion	Ratio	Lower	Upper
99	100		
42	18.5	15.3	22.9
71	34.2	27.5	41.3

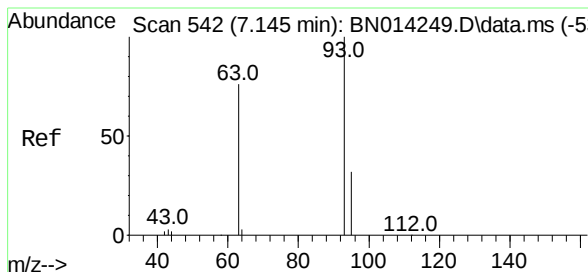


bis(2-Chloroethyl)ether
 Concen: 0.19 ng
 RT: 7.153 min Scan# 543
 Delta R.T. 0.008 min
 Lab File: BN014248.D
 Acq: 09 Apr 2021 11:32

Tgt Ion:	93	Resp:	3635
Ion	Ratio	Lower	Upper
93	100		
63	73.6	58.3	87.5
95	35.4	27.0	40.4






Abundance Scan 859 (10.492 min): BN014249.D\data.ms (-8547-)




Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 859
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	136	Resp:	28100
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.0	13.4
54	6.6	4.8	7.2
68	5.8	4.4	6.6






Abundance Scan 730 (8.857 min): BN014249.D\data.ms (-7277-)



Nitrobenzene-d5
Concen: 0.17 ng
RT: 8.857 min Scan# 730
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	82	Resp:	3292
Ion Ratio	Lower	Upper	
82	100		
128	39.8	29.7	44.5
54	47.6	36.5	54.7





Abundance Scan 863 (10.543 min): BN014249.D\data.ms (-857) (-)

Naphthalene
Concen: 0.19 ng
RT: 10.543 min Scan# 863
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:	128	Resp:	13531
Ion	Ratio	Lower	Upper
128	100		
129	11.6	9.0	13.6
127	13.3	10.5	15.7





Abundance Scan 863 (10.543 min): BN014248.D\data.ms (-855) (-)




Abundance Scan 886 (10.834 min): BN014249.D\data.ms (-886) (-)

Hexachlorobutadiene
Concen: 0.20 ng
RT: 10.834 min Scan# 886
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:	225	Resp:	2788
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.0	51.9	77.9




Abundance Scan 886 (10.834 min): BN014248.D\data.ms (-878) (-)





Abundance Scan 1069 (12.084 min): BN014249.D\data.ms (-1035) (-)

2-Methylnaphthalene-d10
Concen: 0.18 ng
RT: 12.084 min Scan# 1069
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2



Tgt Ion:152 Resp: 8356
Ion Ratio Lower Upper
152 100
151 20.0 16.1 24.1






Abundance Scan 1069 (12.084 min): BN014248.D\data.ms (-1024) (-)




Abundance Scan 1086 (12.160 min): BN014249.D\data.ms (-1012) (-)

2-Methylnaphthalene
Concen: 0.17 ng
RT: 12.160 min Scan# 1086
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:142 Resp: 8837
Ion Ratio Lower Upper
142 100
141 89.1 70.6 106.0
115 36.9 28.6 42.8

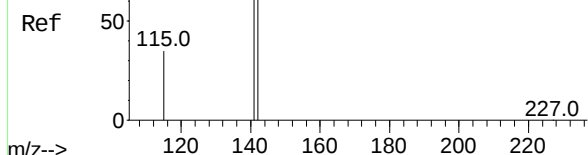


Abundance Scan 1086 (12.160 min): BN014248.D\data.ms (-1064) (-)






Abundance Scan 1309 (14.346 min): BN014249.D\data.ms (-1293) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1309
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

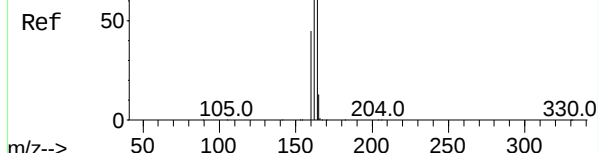





Tgt Ion:	164	Resp:	15531
Ion Ratio	Lower	Upper	
164	100		
162	100.6	79.8	119.8
160	46.5	36.6	54.8




Abundance Scan 1426 (15.831 min): BN014249.D\data.ms (-1418) (-)

2,4,6-Tribromophenol
Concen: 0.14 ng
RT: 15.831 min Scan# 1426
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:	330	Resp:	1107
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	31.8	25.4	38.0






Abundance Scan 1200 (12.963 min): BN014249.D\data.ms (-1195) (-)




2-Fluorobiphenyl
Concen: 0.20 ng
RT: 12.963 min Scan# 1200
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	172	Resp:	10898
Ion Ratio	Lower	Upper	
172	100		
171	35.6	28.6	42.8
170	24.8	19.7	29.5






Abundance Scan 1287 (14.067 min): BN014249.D\data.ms (-1216) (-)



Acenaphthylene
Concen: 0.15 ng
RT: 14.067 min Scan# 1287
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	152	Resp:	10637
Ion Ratio	Lower	Upper	
152	100		
151	19.4	15.7	23.5
153	13.0	10.6	16.0





Abundance Scan 1314 (14.410 min): BN014249.D\data.ms (-1310) (-)

Acenaphthene
Concen: 0.19 ng
RT: 14.409 min Scan# 1314
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:	154	Resp:	8276
Ion Ratio	Lower	Upper	
154	100		
153	110.1	88.1	132.1
152	54.7	43.8	65.6




Abundance Scan 1314 (14.409 min): BN014248.D\data.ms (-1306) (-)





Abundance Scan 1392 (15.399 min): BN014249.D\data.ms (-1395) (-)


Fluorene
Concen: 0.18 ng
RT: 15.399 min Scan# 1392
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32



Tgt Ion:	166	Resp:	10406
Ion Ratio	Lower	Upper	
166	100		
165	97.5	78.0	117.0
167	13.5	10.6	16.0




Abundance Scan 1392 (15.399 min): BN014248.D\data.ms (-1376) (-)






Abundance Scan 1529 (17.091 min): BN014249.D\data.ms (-1514) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.092 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampled :
SSTDIC0.2

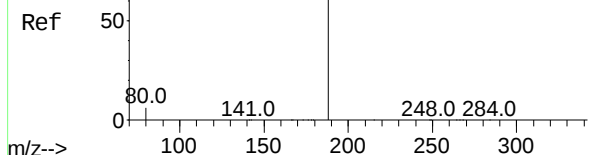




Tgt Ion:	188	Resp:	34557
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	7.3	5.5	8.3




Abundance Scan 1397 (15.463 min): BN014249.D\data.ms (-1324) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.21 ng
RT: 15.463 min Scan# 1397
Delta R.T. -0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:	198	Resp:	706
Ion Ratio	Lower	Upper	
198	100		
51	165.7	76.0	114.0#
105	101.7	53.5	80.3#






Abundance Scan 1463 (16.288 min): BN014249.D\data.ms (-1427) (-)




4-Bromophenyl-phenylether
Concen: 0.18 ng
RT: 16.289 min Scan# 1463
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	248	Resp:	3406
Ion	Ratio	Lower	Upper
248	100		
250	97.2	76.9	115.3
141	55.2	41.4	62.0






Abundance Scan 1472 (16.398 min): BN014249.D\data.ms (-1422) (-)




Hexachlorobenzene
Concen: 0.21 ng
RT: 16.398 min Scan# 1472
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:	284	Resp:	4341
Ion	Ratio	Lower	Upper
284	100		
142	32.4	26.2	39.4
249	29.8	23.8	35.8





Abundance Scan 1485 (16.556 min): BN014249.D\data.ms (-1485) (-)




Atrazine
Concen: 0.13 ng
RT: 16.556 min Scan# 1485
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	200	Resp:	2426
Ion Ratio	Lower	Upper	
200	100		
173	26.7	20.9	31.3
215	48.6	39.2	58.8



Abundance Scan 1485 (16.556 min): BN014248.D\data.ms (-1444) (-)





Abundance Scan 1500 (16.738 min): BN014249.D\data.ms (-1495) (-)




Pentachlorophenol
Concen: 0.13 ng
RT: 16.739 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	266	Resp:	1156
Ion Ratio	Lower	Upper	
266	100		
264	64.8	50.3	75.5
268	65.8	51.8	77.8



Abundance Scan 1500 (16.739 min): BN014248.D\data.ms (-1492) (-)





Abundance Scan 1532 (17.128 min): BN014249.D\data.ms (-1525) (-)




Phenanthrene
Concen: 0.20 ng
RT: 17.128 min Scan# 1532
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:	178	Resp:	18249
Ion	Ratio	Lower	Upper
178	100		
176	19.4	15.3	22.9
179	15.3	12.3	18.5


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Abundance Scan 1532 (17.128 min): BN014248.D\data.ms (-1507) (-)





Abundance Scan 1540 (17.225 min): BN014249.D\data.ms (-1526) (-)




Anthracene
Concen: 0.16 ng
RT: 17.226 min Scan# 1540
Delta R.T. 0.000 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	178	Resp:	14530
Ion	Ratio	Lower	Upper
178	100		
176	18.4	15.0	22.4
179	15.2	12.3	18.5



Abundance Scan 1540 (17.226 min): BN014248.D\data.ms (-1532) (-)





Abundance Scan 1830 (19.126 min): BN014249.D\data.ms (-1829) (-)

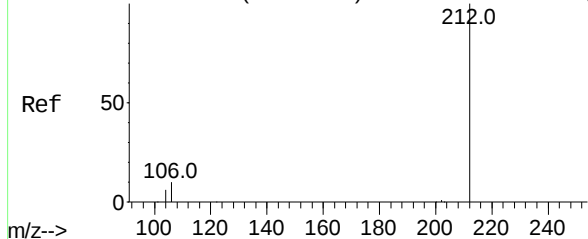


Fluoranthene-d10
Concen: 0.19 ng
RT: 19.124 min Scan# 1828
Delta R.T. -0.002 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	212	Resp:	19279
Ion	Ratio	Lower	Upper
212	100		
106	11.6	9.1	13.7
104	6.5	5.1	7.7



Abundance Scan 1828 (19.124 min): BN014248.D\data.ms (-1788) (-)





Abundance Scan 1836 (19.156 min): BN014249.D\data.ms (-1828) (-)




Fluoranthene
Concen: 0.19 ng
RT: 19.153 min Scan# 1834
Delta R.T. -0.002 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	202	Resp:	20753
Ion	Ratio	Lower	Upper
202	100		
101	9.5	7.8	11.8
203	17.0	13.8	20.6



Abundance Scan 1834 (19.153 min): BN014248.D\data.ms (-1794) (-)






Abundance Scan 2127 (21.279 min): BN014249.D\data.ms (-2127) (-)

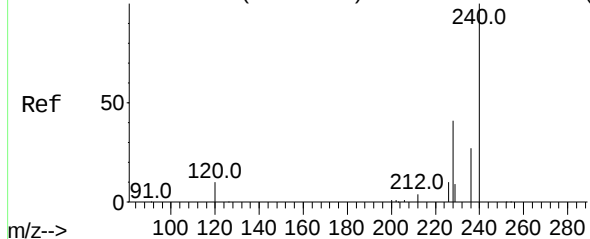


Chrysene-d12
Concen: 0.40 ng
RT: 21.282 min Scan# 2126
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:	240	Resp:	34779
Ion	Ratio	Lower	Upper
240	100		
120	9.9	9.4	14.2
236	26.8	21.7	32.5






Abundance Scan 1909 (19.518 min): BN014249.D\data.ms (-1839) (-)

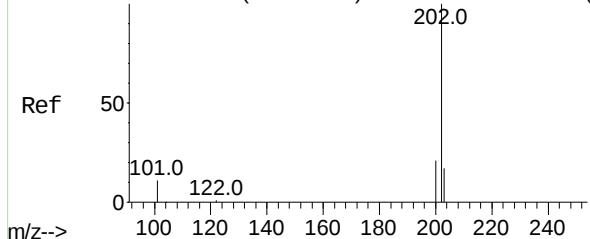

Pyrene
Concen: 0.19 ng
RT: 19.521 min Scan# 1908
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	202	Resp:	21586
Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.5	24.7
203	17.6	13.9	20.9





Abundance Scan 1952 (19.732 min): BN014249.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 0.19 ng
RT: 19.729 min Scan# 1950
Delta R.T. -0.002 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

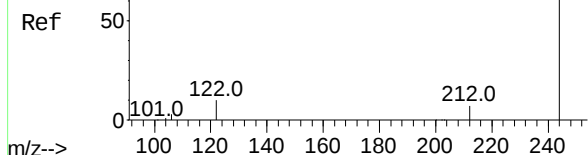

Tgt Ion:	244	Resp:	15060
Ion	Ratio	Lower	Upper
244	100		
212	7.8	6.1	9.1
122	11.5	8.2	12.4





Abundance Scan 1950 (19.729 min): BN014248.D\data.ms (-1920) (-)




Abundance Scan 2126 (21.268 min): BN014249.D\data.ms (-2120) (-)

Benzo(a)anthracene
Concen: 0.16 ng
RT: 21.271 min Scan# 2125
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion:	228	Resp:	18112
Ion	Ratio	Lower	Upper
228	100		
226	26.1	21.0	31.6
229	20.5	16.0	24.0



Abundance Scan 2125 (21.271 min): BN014248.D\data.ms (-2106) (-)




Abundance Scan 2131 (21.322 min): BN014249.D\data.ms (-2128) (-)




Chrysene
Concen: 0.19 ng
RT: 21.314 min Scan# 2129
Delta R.T. -0.008 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Abundance Scan 2129 (21.314 min): BN014248.D\data.ms




Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.3	23.0	34.4
229	19.2	16.0	24.0



Abundance Scan 2129 (21.314 min): BN014248.D\data.ms (-2120) (-)





Abundance Scan 2121 (21.215 min): BN014249.D\data.ms (-2118) (-)




Bis(2-ethylhexyl)phthalate
Concen: 0.09 ng
RT: 21.218 min Scan# 2120
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.7	22.3	33.5
279	7.8	4.0	6.0#

Abundance Scan 2120 (21.218 min): BN014248.D\data.ms




Abundance Scan 2120 (21.218 min): BN014248.D\data.ms (-2110) (-)





Abundance Scan 3216 (25.769 min): BN014249.D\data.ms (-3185) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.20 ng
RT: 25.772 min Scan# 3215
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.8	17.9	26.9
277	25.0	19.9	29.9




Abundance Scan 3215 (25.772 min): BN014248.D\data.ms (-3185) (-)





Abundance Scan 2558 (23.517 min): BN014249.D\data.ms (-2536) (-)


Perylene-d12
Concen: 0.40 ng
RT: 23.520 min Scan# 2557
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32




Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.8	29.8
265	43.8	35.3	52.9



Abundance Scan 2557 (23.520 min): BN014248.D\data.ms (-2512) (-)





Abundance Scan 2362 (22.846 min): BN014249.D\data.ms (-2362) (-)

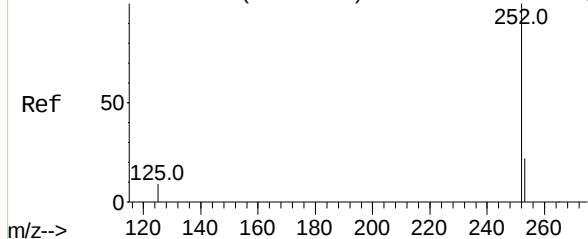


Benzo(b)fluoranthene
Concen: 0.19 ng
RT: 22.849 min Scan# 2361
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	252	Resp:	20955
Ion Ratio	Lower	Upper	
252	100		
253	26.1	18.8	28.2
125	13.9	8.6	13.0#



Abundance Scan 2361 (22.849 min): BN014248.D\data.ms (-2302) (-)





Abundance Scan 2375 (22.891 min): BN014249.D\data.ms (-2375) (-)

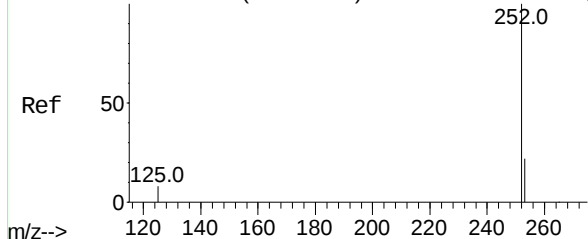


Benzo(k)fluoranthene
Concen: 0.22 ng
RT: 22.894 min Scan# 2374
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Tgt Ion:	252	Resp:	22555
Ion Ratio	Lower	Upper	
252	100		
253	26.4	19.0	28.4
125	14.8	8.8	13.2#




Abundance Scan 2374 (22.894 min): BN014248.D\data.ms (-2286) (-)





Abundance Scan 2530 (23.421 min): BN014249.D\data.ms (-2530) (-)

Benzo(a)pyrene
Concen: 0.18 ng
RT: 23.421 min Scan# 2528
Delta R.T. -0.001 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

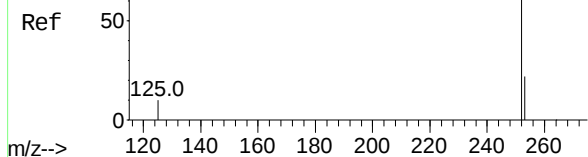

Tgt Ion	Ratio	Lower	Upper
252	100		
253	28.7	19.9	29.9
125	18.4	10.4	15.6#





Abundance Scan 2528 (23.421 min): BN014248.D\data.ms (-2470) (-)




Abundance Scan 3221 (25.787 min): BN014249.D\data.ms (-3219) (-)

Dibenzo(a,h)anthracene
Concen: 0.21 ng
RT: 25.786 min Scan# 3219
Delta R.T. -0.001 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32


Tgt Ion	Ratio	Lower	Upper
278	100		
139	16.2	11.9	17.9
279	27.6	19.9	29.9



Abundance Scan 3219 (25.786 min): BN014248.D\data.ms (-3196) (-)




Abundance Scan 3416 (26.454 min): BN014249.D\data.ms (-3356) (-)



Benzo(g,h,i)perylene
Concen: 0.20 ng
RT: 26.457 min Scan# 3415
Delta R.T. 0.003 min
Lab File: BN014248.D
Acq: 09 Apr 2021 11:32

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2



Tgt Ion:	276	Resp:	20884
Ion Ratio	Lower	Upper	
276	100		
277	25.8	19.3	28.9
138	20.4	15.7	23.5

