

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
 Data File : BN014249.D
 Acq On : 09 Apr 2021 12:08
 Operator : CG/JU
 Sample : SSTDICC0.4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Quant Time: Apr 09 12:43:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 12:42:56 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	7961	0.40	ng	0.00
7) Naphthalene-d8	10.492	136	28969	0.40	ng	0.00
13) Acenaphthene-d10	14.346	164	16527	0.40	ng	0.00
19) Phenanthrene-d10	17.091	188	36860	0.40	ng	0.00
29) Chrysene-d12	21.279	240	36491	0.40	ng	0.00
36) Perylene-d12	23.517	264	32428	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.316	112	8228	0.39	ng	0.00
5) Phenol-d6	6.879	99	10138	0.35	ng	0.00
8) Nitrobenzene-d5	8.857	82	7605	0.38	ng	0.00
11) 2-Methylnaphthalene-d10	12.084	152	19063	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.831	330	2677	0.31	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	25038	0.44	ng	0.00
27) Fluoranthene-d10	19.126	212	45469	0.42	ng	0.00
31) Terphenyl-d14	19.732	244	35620	0.44	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.287	88	4117	0.47	ng	98
3) n-Nitrosodimethylamine	3.633	42	1830	0.38	ng	98
6) bis(2-Chloroethyl)ether	7.145	93	8310	0.42	ng	100
9) Naphthalene	10.543	128	30771	0.42	ng	100
10) Hexachlorobutadiene	10.834	225	6141	0.44	ng	# 100
12) 2-Methylnaphthalene	12.160	142	20355	0.39	ng	100
16) Acenaphthylene	14.067	152	25360	0.34	ng	100
17) Acenaphthene	14.410	154	19214	0.41	ng	100
18) Fluorene	15.399	166	24696	0.41	ng	100
20) 4,6-Dinitro-2-methylph...	15.463	198	1712	0.47	ng	100
21) 4-Bromophenyl-phenylether	16.288	248	8089	0.40	ng	100
22) Hexachlorobenzene	16.398	284	10160	0.46	ng	100
23) Atrazine	16.556	200	5601	0.28	ng	100
24) Pentachlorophenol	16.738	266	2871	0.31	ng	100
25) Phenanthrene	17.128	178	43195	0.44	ng	100
26) Anthracene	17.225	178	35261	0.37	ng	100
28) Fluoranthene	19.156	202	49423	0.43	ng	100
30) Pyrene	19.518	202	50126	0.43	ng	100
32) Benzo(a)anthracene	21.268	228	44472	0.38	ng	100
33) Chrysene	21.322	228	49704	0.44	ng	100
34) Bis(2-ethylhexyl)phtha...	21.215	149	14080	0.20	ng	100
35) Indeno(1,2,3-cd)pyrene	25.769	276	54166	0.39	ng	100
37) Benzo(b)fluoranthene	22.846	252	50245	0.47	ng	100
38) Benzo(k)fluoranthene	22.891	252	48314	0.47	ng	100
39) Benzo(a)pyrene	23.421	252	39994	0.41	ng	100
40) Dibenzo(a,h)anthracene	25.787	278	45942	0.46	ng	100
41) Benzo(g,h,i)perylene	26.454	276	48192	0.47	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
Data File : BN014249.D
Acq On : 09 Apr 2021 12:08
Operator : CG/JU
Sample : SSTDICC0.4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Apr 09 12:43:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 12:42:56 2021
Response via : Initial Calibration




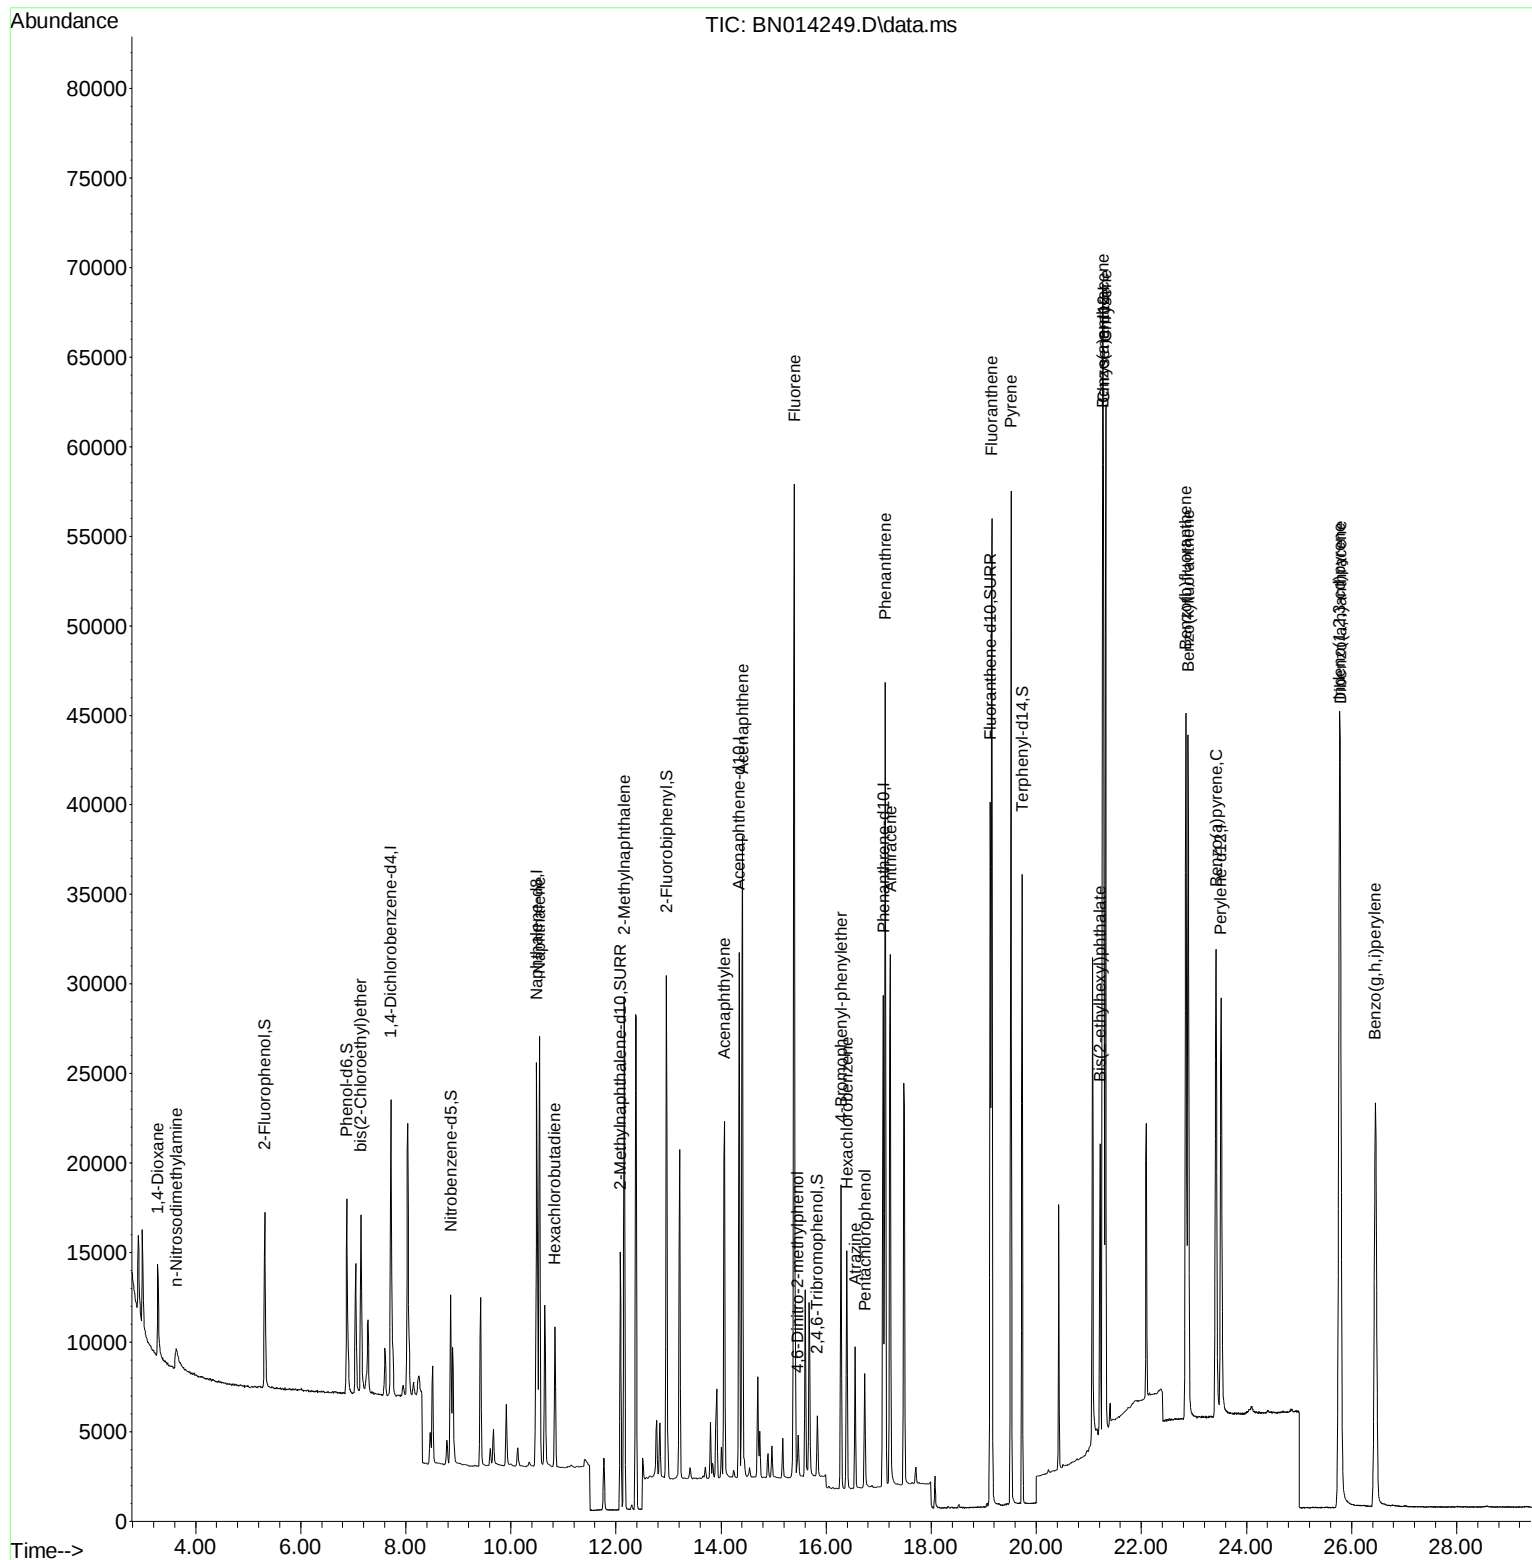


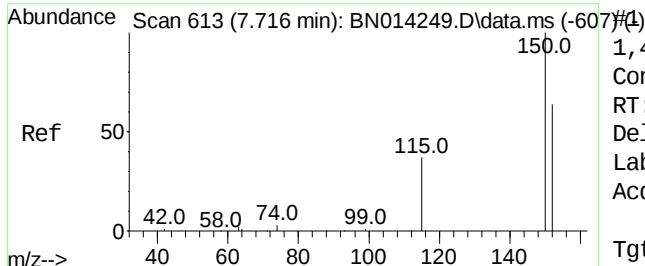

1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.716 min Scan# 613
 Delta R.T. 0.000 min
 Lab File: BN014249.D
 Acq: 09 Apr 2021 12:08




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:	152	Resp:	7961
Ion	Ratio	Lower	Upper
152	100		
150	156.0	124.8	187.2
115	60.8	48.6	73.0

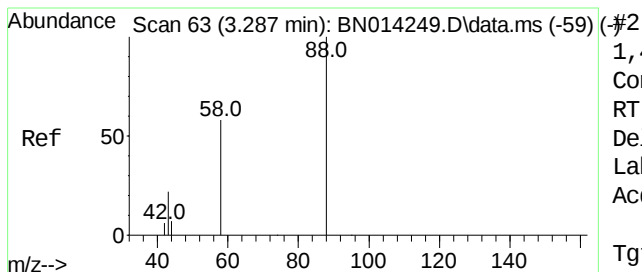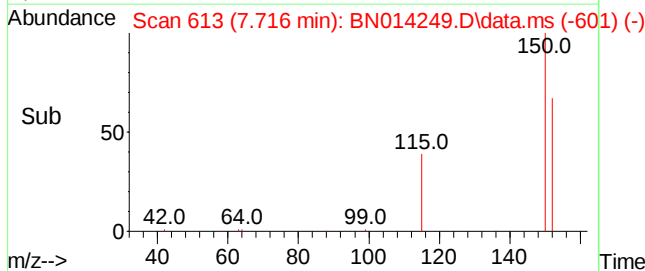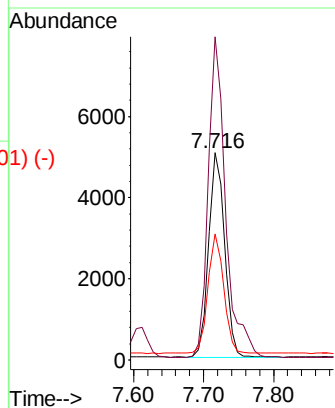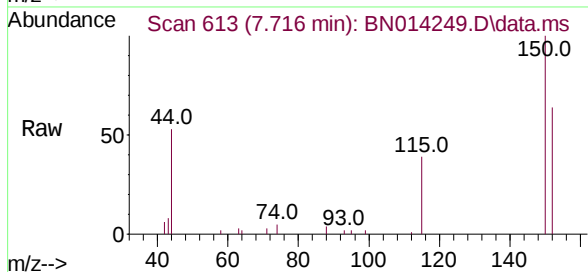

1,4-Dioxane
 Concen: 0.47 ng
 RT: 3.287 min Scan# 63
 Delta R.T. 0.000 min
 Lab File: BN014249.D
 Acq: 09 Apr 2021 12:08

Tgt Ion:	88	Resp:	4117
Ion	Ratio	Lower	Upper
88	100		
58	67.5	52.5	78.7
43	26.1	21.8	32.8


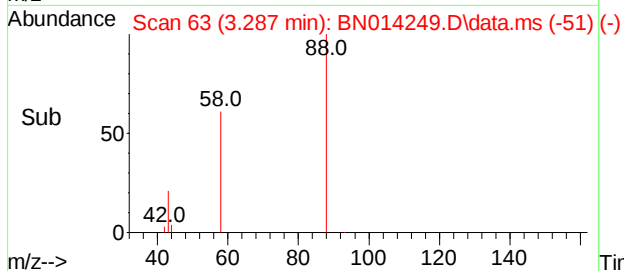
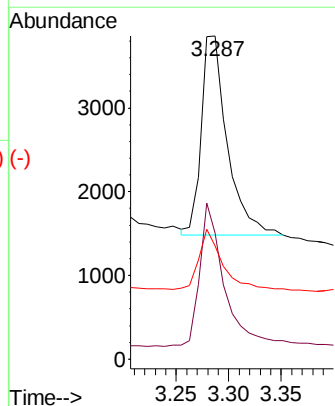



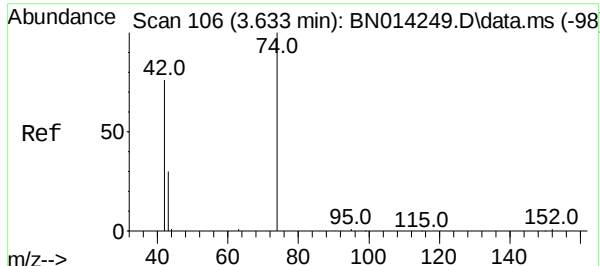

n-Nitrosodimethylamine
 Concen: 0.38 ng
 RT: 3.633 min Scan# 106
 Delta R.T. 0.000 min
 Lab File: BN014249.D
 Acq: 09 Apr 2021 12:08




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4


Tgt Ion:	42	Resp:	1830
Ion	Ratio	Lower	Upper
42	100		
74	136.9	111.2	166.8
44	16.0	12.5	18.7

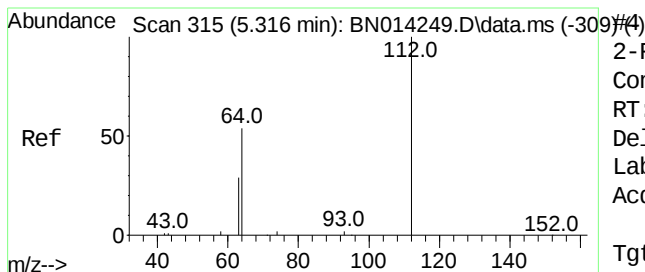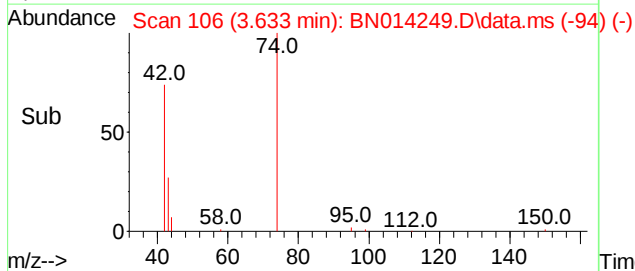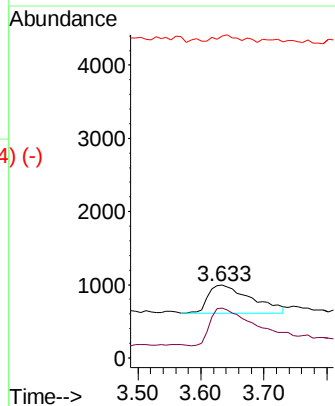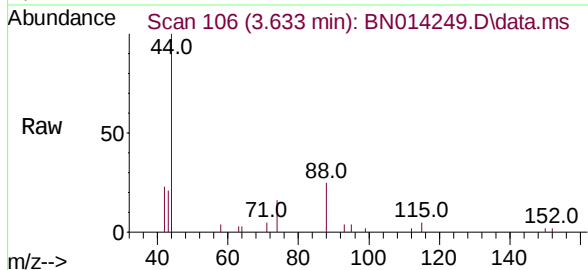

2-Fluorophenol
 Concen: 0.39 ng
 RT: 5.316 min Scan# 315
 Delta R.T. 0.000 min
 Lab File: BN014249.D
 Acq: 09 Apr 2021 12:08

Tgt Ion:	112	Resp:	8228
Ion	Ratio	Lower	Upper
112	100		
64	54.2	43.4	65.0
63	29.4	23.5	35.3


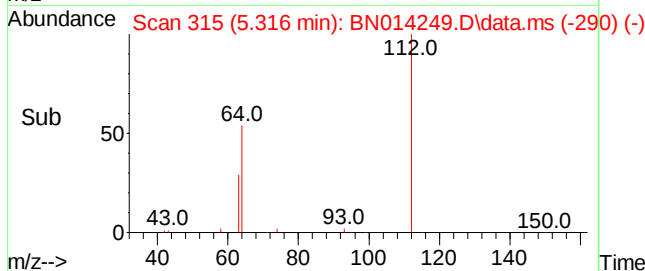
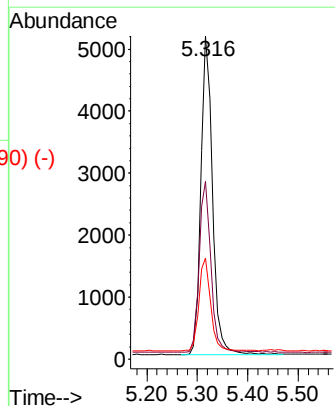



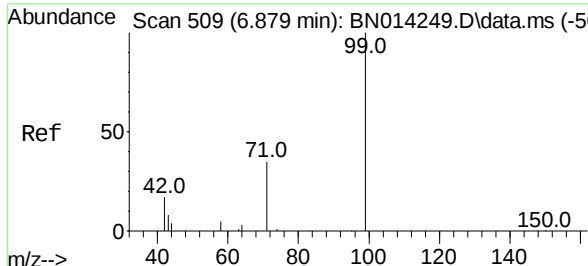

Phenol-d6
 Concen: 0.35 ng
 RT: 6.879 min Scan# 509
 Delta R.T. 0.000 min
 Lab File: BN014249.D
 Acq: 09 Apr 2021 12:08




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion:	99	Resp:	10138
Ion	Ratio	Lower	Upper
99	100		
42	19.1	15.3	22.9
71	34.4	27.5	41.3

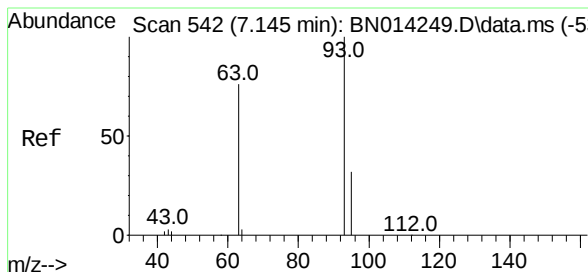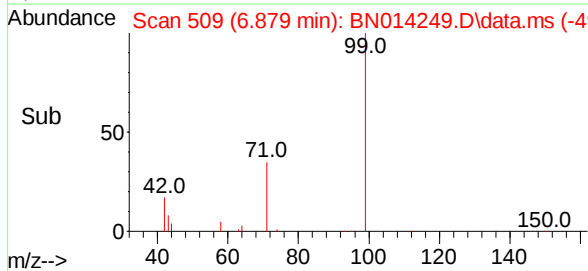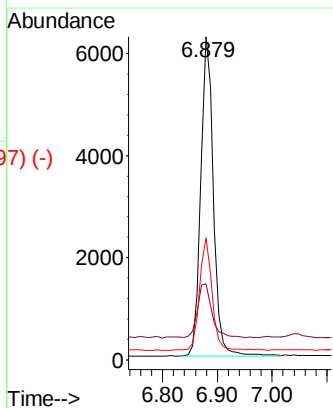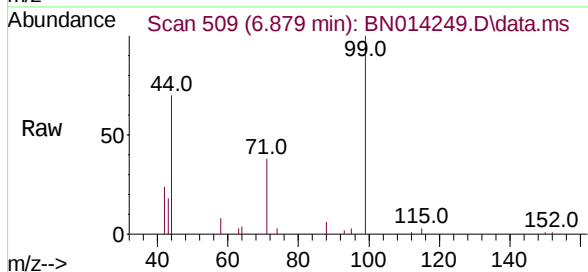


bis(2-Chloroethyl)ether
 Concen: 0.42 ng
 RT: 7.145 min Scan# 542
 Delta R.T. 0.000 min
 Lab File: BN014249.D
 Acq: 09 Apr 2021 12:08

Tgt Ion:	93	Resp:	8310
Ion	Ratio	Lower	Upper
93	100		
63	72.9	58.3	87.5
95	33.7	27.0	40.4

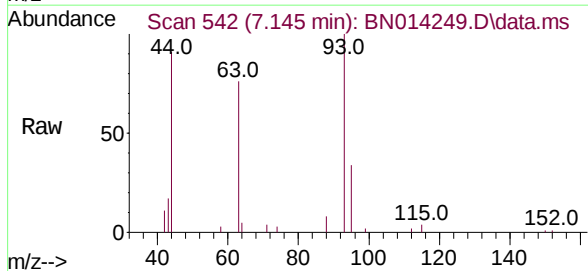




Abundance Scan 859 (10.492 min): BN014249.D\data.ms (-8547-)

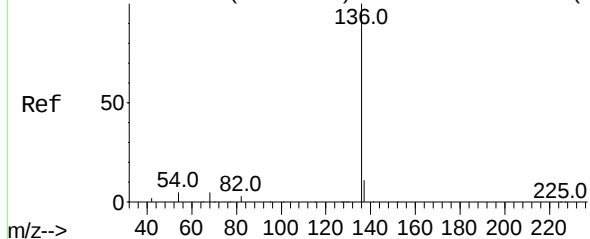


Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 859
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	136	Resp:	28969
Ion Ratio	Lower	Upper	
136	100		
137	11.2	9.0	13.4
54	6.0	4.8	7.2
68	5.5	4.4	6.6

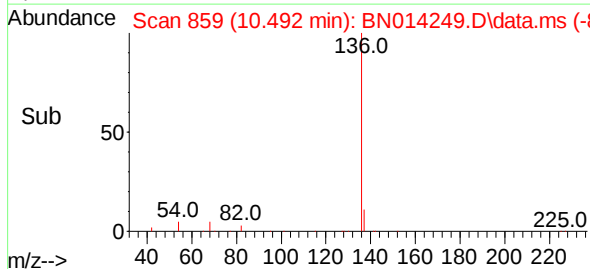
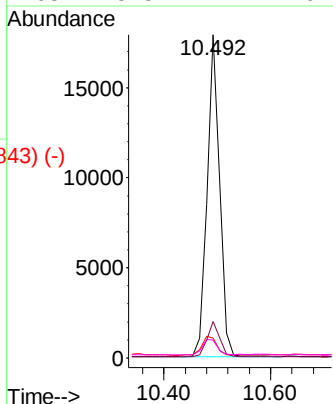
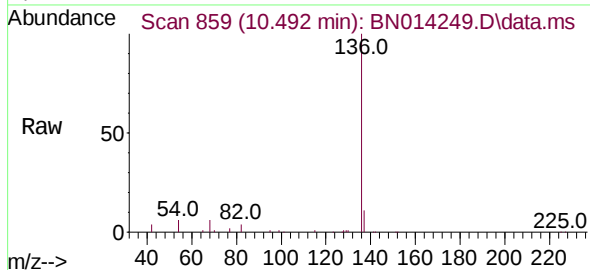


Abundance Scan 730 (8.857 min): BN014249.D\data.ms (-7277-)

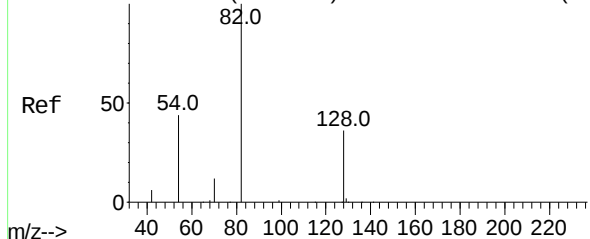

Nitrobenzene-d5
Concen: 0.38 ng
RT: 8.857 min Scan# 730
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Tgt Ion:	82	Resp:	7605
Ion Ratio	Lower	Upper	
82	100		
128	37.1	29.7	44.5
54	45.6	36.5	54.7

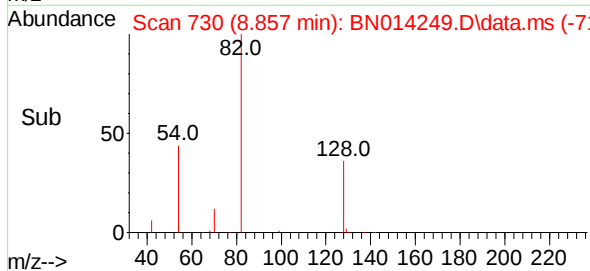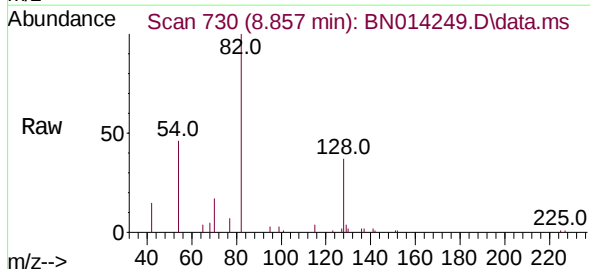




Abundance Scan 863 (10.543 min): BN014249.D\data.ms (-857) (-)

Naphthalene
Concen: 0.42 ng
RT: 10.543 min Scan# 863
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

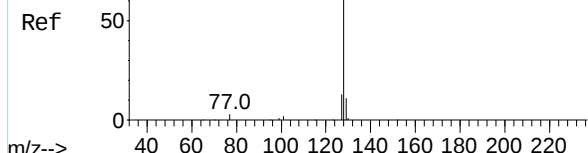


Tgt Ion:	128	Resp:	30771
Ion Ratio	Lower	Upper	
128	100		
129	11.3	9.0	13.6
127	13.1	10.5	15.7



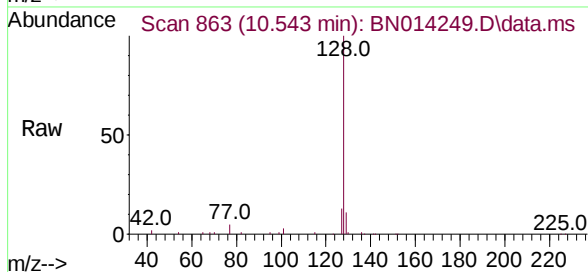


Abundance Scan 886 (10.834 min): BN014249.D\data.ms (-886) (-)

Hexachlorobutadiene
Concen: 0.44 ng
RT: 10.834 min Scan# 886
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

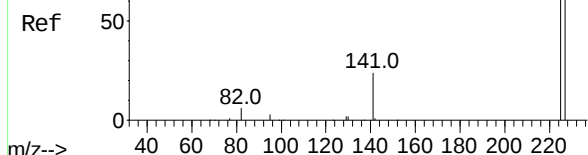


Tgt Ion:	225	Resp:	6141
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	64.9	51.9	77.9

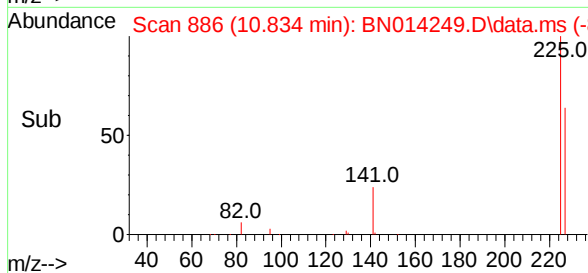



Abundance Scan 1069 (12.084 min): BN014249.D\data.ms (-1015) (-)

2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.084 min Scan# 1069
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

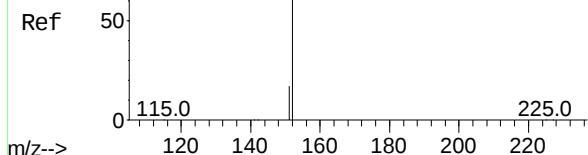

Tgt Ion:152 Resp: 19063
Ion Ratio Lower Upper
152 100
151 20.1 16.1 24.1

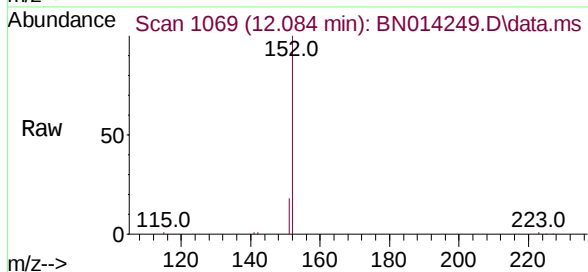




Abundance Scan 1069 (12.084 min): BN014249.D\data.ms (-1024) (-)

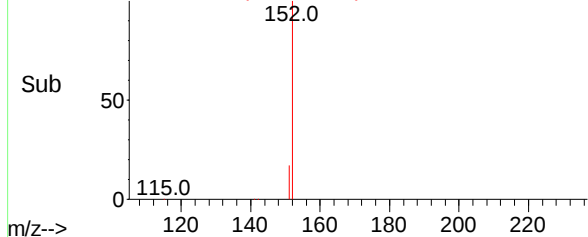


Abundance Scan 1086 (12.160 min): BN014249.D\data.ms (-1016) (-)

2-Methylnaphthalene
Concen: 0.39 ng
RT: 12.160 min Scan# 1086
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:142 Resp: 20355
Ion Ratio Lower Upper
142 100
141 88.3 70.6 106.0
115 35.7 28.6 42.8

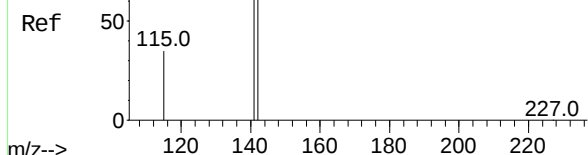


Abundance Scan 1086 (12.160 min): BN014249.D\data.ms (-1064) (-)

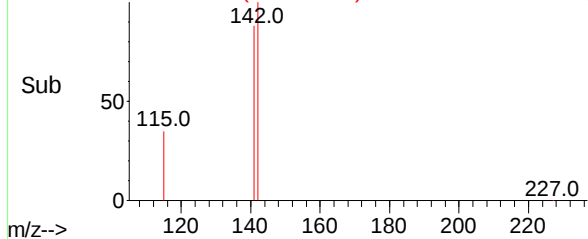




Abundance Scan 1309 (14.346 min): BN014249.D\data.ms (-1293) (-)

Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

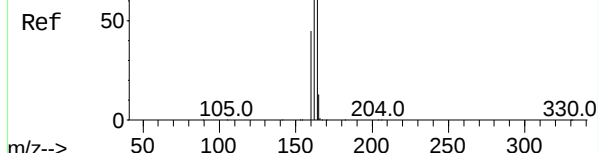





Tgt Ion:	164	Resp:	16527
Ion Ratio	Lower	Upper	
164	100		
162	99.8	79.8	119.8
160	45.7	36.6	54.8

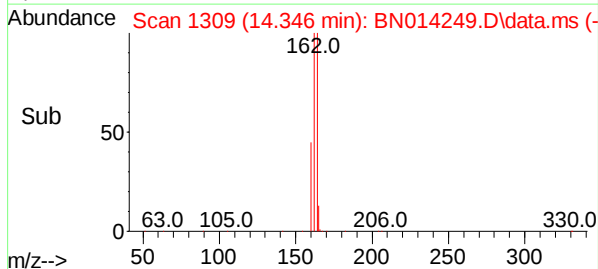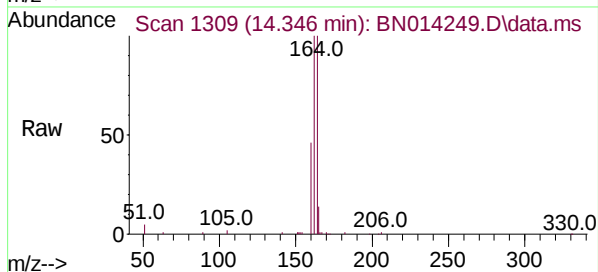


Abundance Scan 1426 (15.831 min): BN014249.D\data.ms (-1418) (-)

2,4,6-Tribromophenol
Concen: 0.31 ng
RT: 15.831 min Scan# 1426
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:	330	Resp:	2677
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	31.7	25.4	38.0

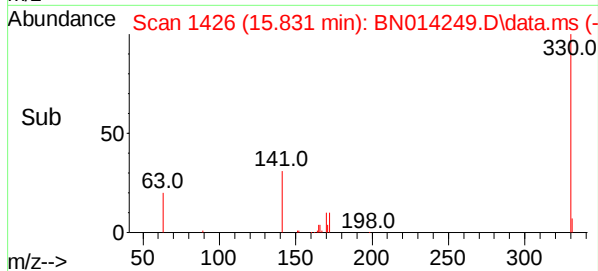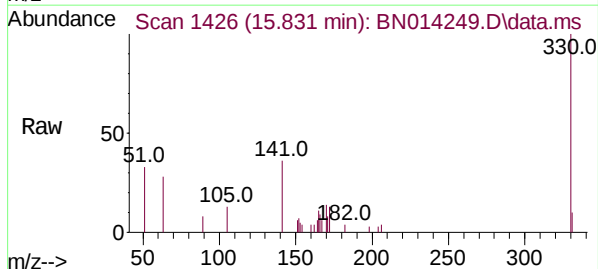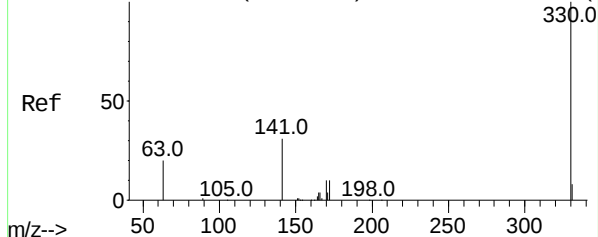



Abundance Scan 1200 (12.963 min): BN014249.D\data.ms (-1195) (-)

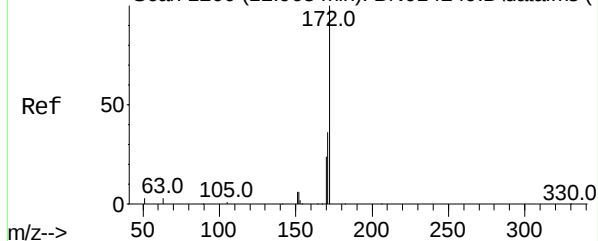


2-Fluorobiphenyl
Concen: 0.44 ng
RT: 12.963 min Scan# 1200
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	172	Resp:	25038
Ion Ratio	Lower	Upper	
172	100		
171	35.7	28.6	42.8
170	24.6	19.7	29.5

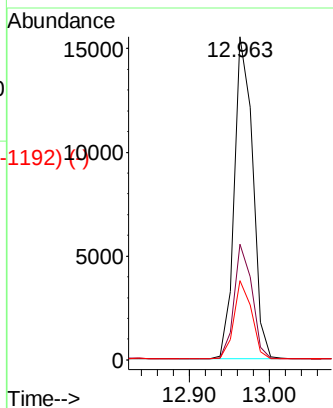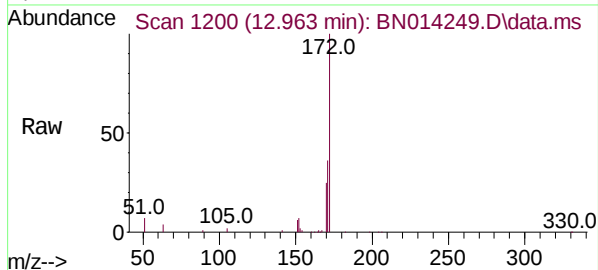

Abundance Scan 1200 (12.963 min): BN014249.D\data.ms (-1192) (-)


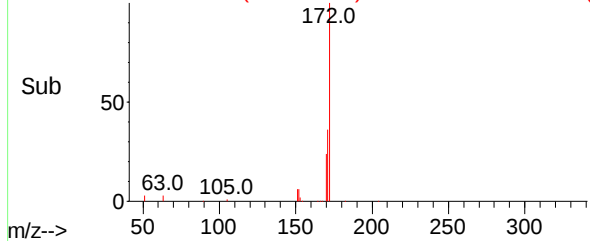


Abundance Scan 1287 (14.067 min): BN014249.D\data.ms (-1271) (-)

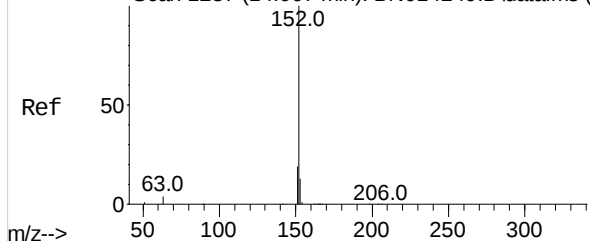


Acenaphthylene
Concen: 0.34 ng
RT: 14.067 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:	152	Resp:	25360
Ion Ratio	Lower	Upper	
152	100		
151	19.5	15.7	23.5
153	13.3	10.6	16.0

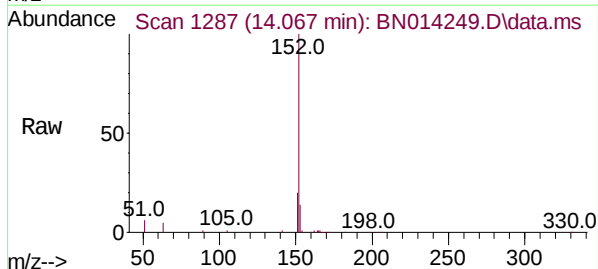


Abundance Scan 1287 (14.067 min): BN014249.D\data.ms (-1271) (-)

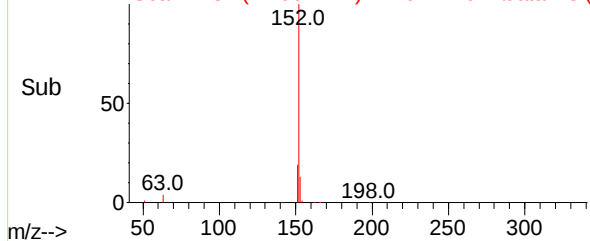



Abundance Scan 1314 (14.410 min): BN014249.D\data.ms (-1310) (-)

Acenaphthene
Concen: 0.41 ng
RT: 14.410 min Scan# 1314
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

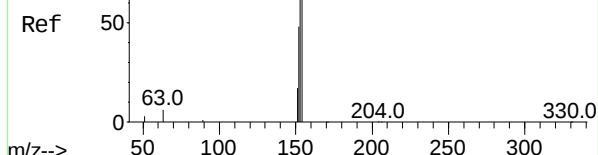

Tgt Ion:	154	Resp:	19214
Ion Ratio	Lower	Upper	
154	100		
153	110.1	88.1	132.1
152	54.7	43.8	65.6

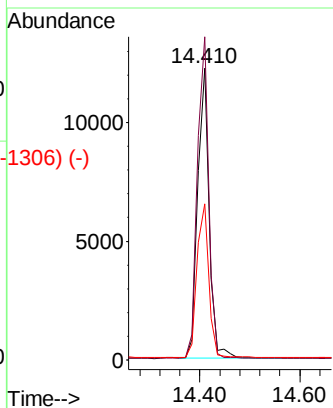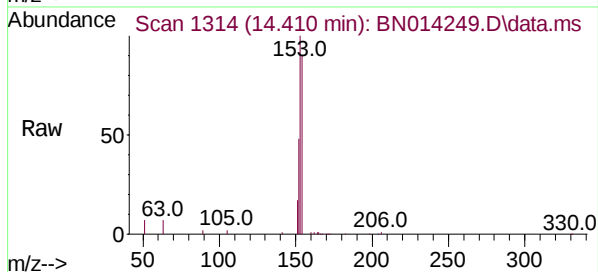



Abundance Scan 1314 (14.410 min): BN014249.D\data.ms (-1306) (-)

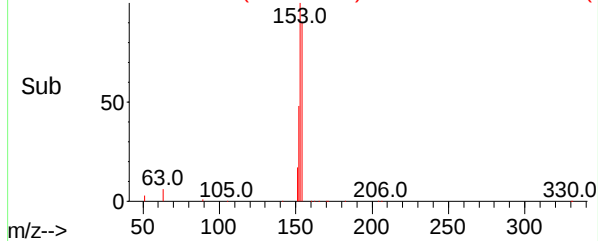


Abundance Scan 1392 (15.399 min): BN014249.D\data.ms (-1395) (-)

Fluorene
Concen: 0.41 ng
RT: 15.399 min Scan# 1392
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:	166	Resp:	24696
Ion Ratio	Lower	Upper	
166	100		
165	97.5	78.0	117.0
167	13.3	10.6	16.0

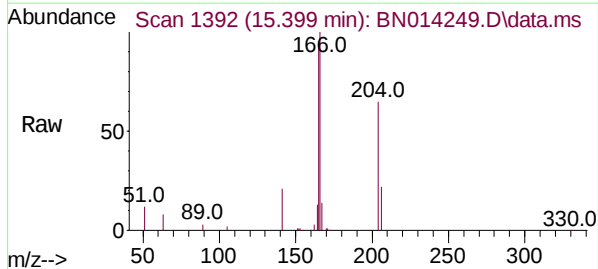


Abundance Scan 1392 (15.399 min): BN014249.D\data.ms (-1376) (-)

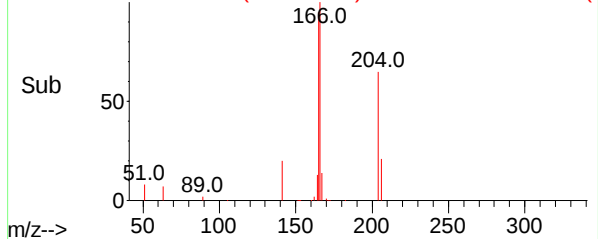




Abundance Scan 1529 (17.091 min): BN014249.D\data.ms (-1514) (-)

Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1529
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

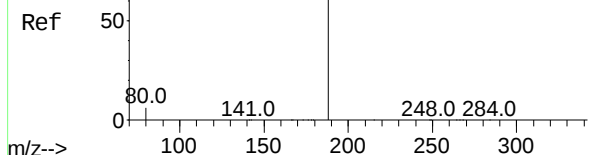





Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.9	5.5	8.3

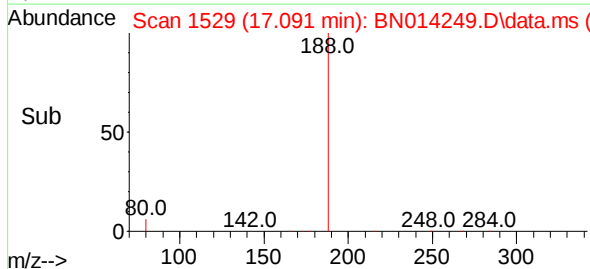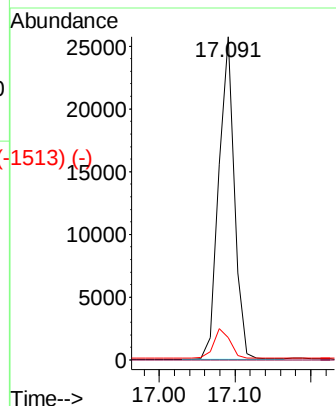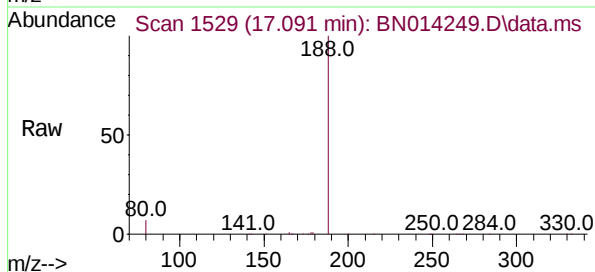

Abundance Scan 1397 (15.463 min): BN014249.D\data.ms (-1324) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.47 ng
RT: 15.463 min Scan# 1397
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Tgt Ion	Ratio	Lower	Upper
198	100		
51	95.0	76.0	114.0
105	66.9	53.5	80.3

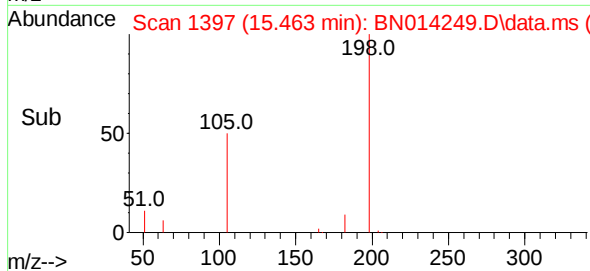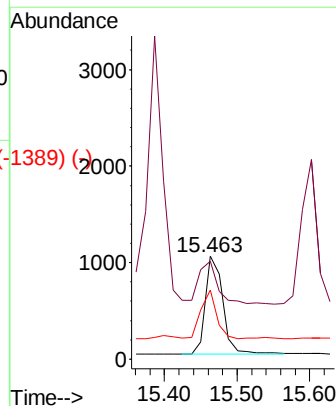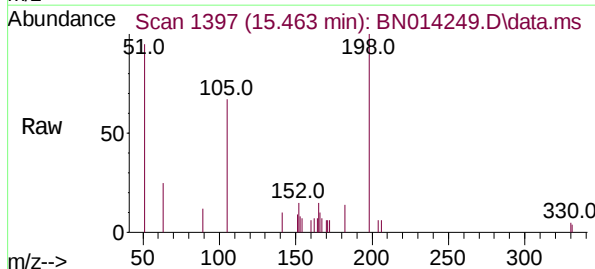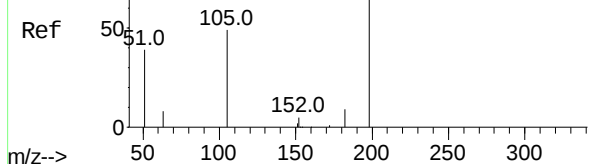




Abundance Scan 1463 (16.288 min): BN014249.D\data.ms (-1427) (-)

4-Bromophenyl-phenylether
Concen: 0.40 ng
RT: 16.288 min Scan# 1463
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

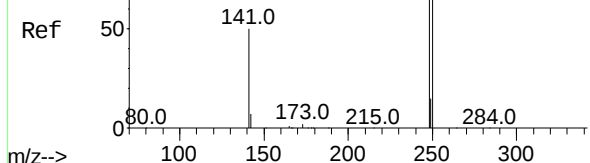


Tgt Ion:	248	Resp:	8089
Ion Ratio	Lower	Upper	
248	100		
250	96.1	76.9	115.3
141	51.7	41.4	62.0

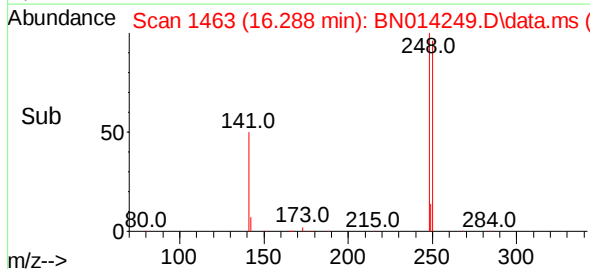
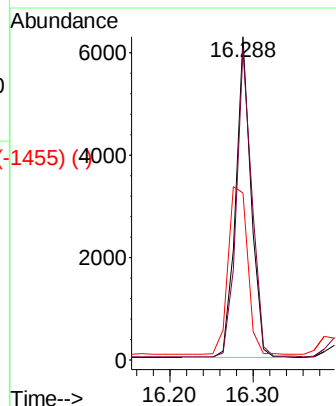
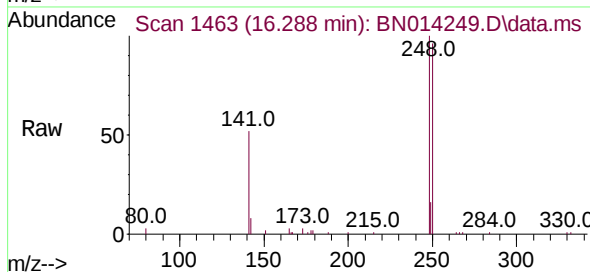


Abundance Scan 1472 (16.398 min): BN014249.D\data.ms (-1428) (-)

Hexachlorobenzene
Concen: 0.46 ng
RT: 16.398 min Scan# 1472
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

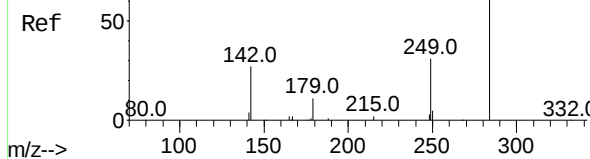


Tgt Ion:	284	Resp:	10160
Ion Ratio	Lower	Upper	
284	100		
142	32.8	26.2	39.4
249	29.8	23.8	35.8

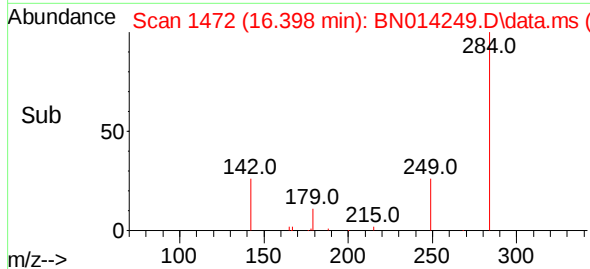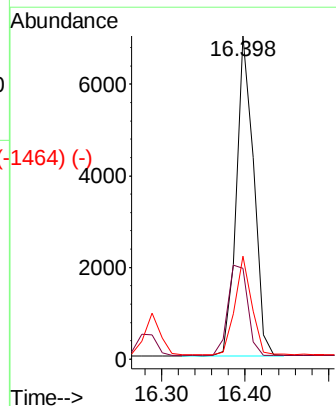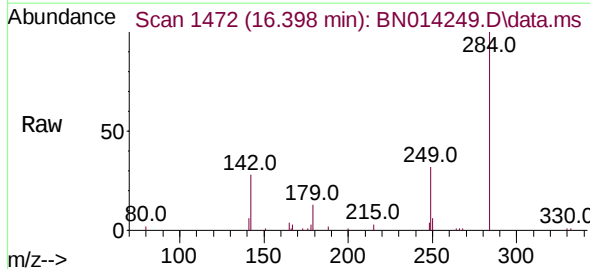



Abundance Scan 1485 (16.556 min): BN014249.D\data.ms (-1485) (-)

Atrazine
Concen: 0.28 ng
RT: 16.556 min Scan# 1485
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

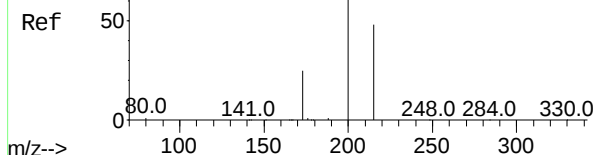

Tgt Ion	Ratio	Lower	Upper
200	100		
173	26.1	20.9	31.3
215	49.0	39.2	58.8

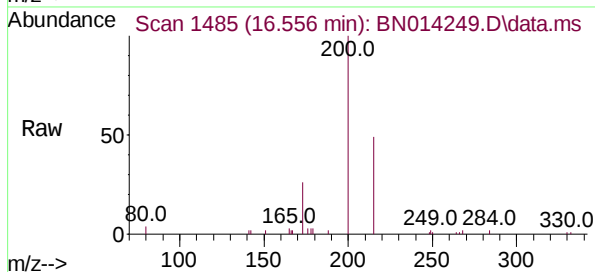



Abundance Scan 1485 (16.556 min): BN014249.D\data.ms (-1444) (-)

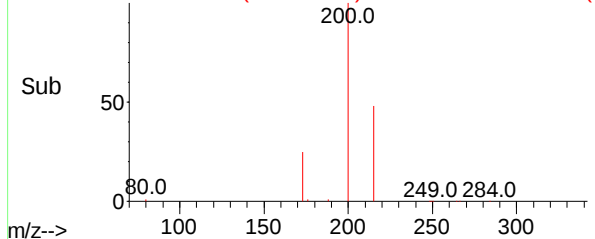


Abundance Scan 1500 (16.738 min): BN014249.D\data.ms (-1495) (-)

Pentachlorophenol
Concen: 0.31 ng
RT: 16.738 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.9	50.3	75.5
268	64.8	51.8	77.8

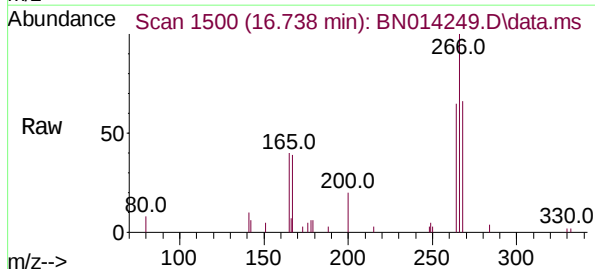


Abundance Scan 1500 (16.738 min): BN014249.D\data.ms (-1492) (-)

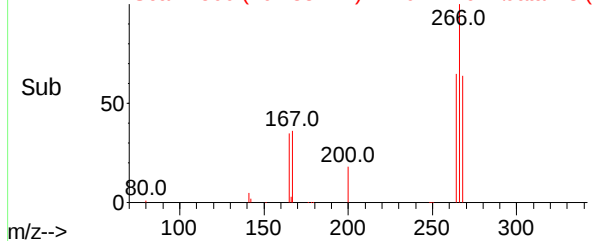




Abundance Scan 1532 (17.128 min): BN014249.D\data.ms (-1525) (-)

Phenanthrene
Concen: 0.44 ng
RT: 17.128 min Scan# 1532
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

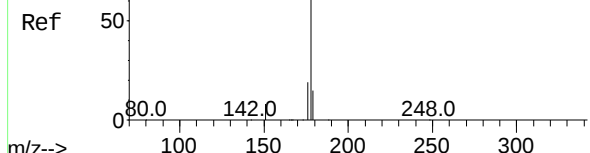





Tgt Ion:	178	Resp:	43195
Ion Ratio	Lower	Upper	
178	100		
176	19.1	15.3	22.9
179	15.4	12.3	18.5

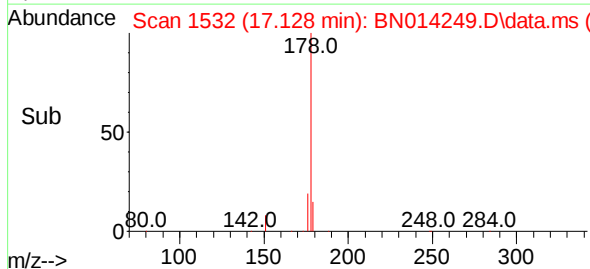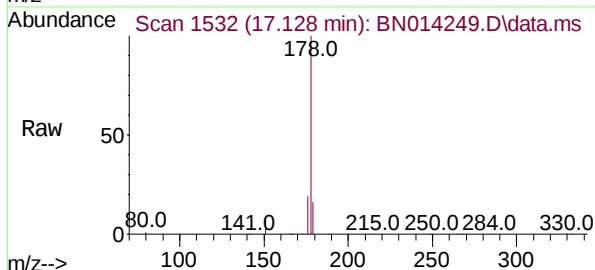


Abundance Scan 1540 (17.225 min): BN014249.D\data.ms (-1526) (-)

Anthracene
Concen: 0.37 ng
RT: 17.225 min Scan# 1540
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:	178	Resp:	35261
Ion Ratio	Lower	Upper	
178	100		
176	18.7	15.0	22.4
179	15.4	12.3	18.5

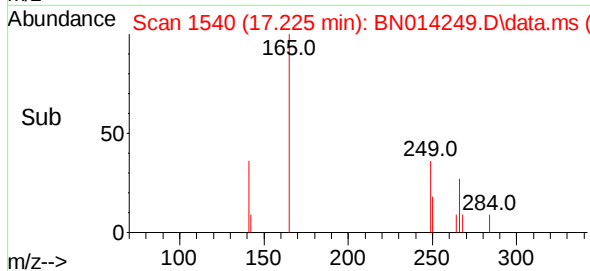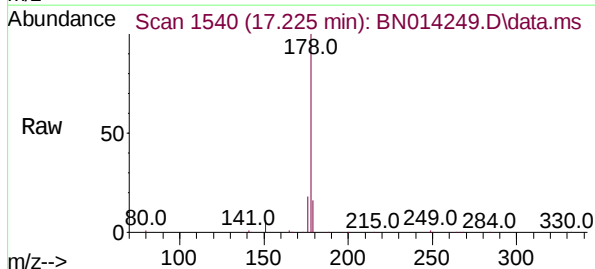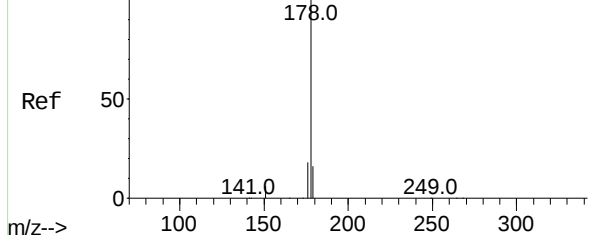




Abundance Scan 1830 (19.126 min): BN014249.D\data.ms (-1797) (-)

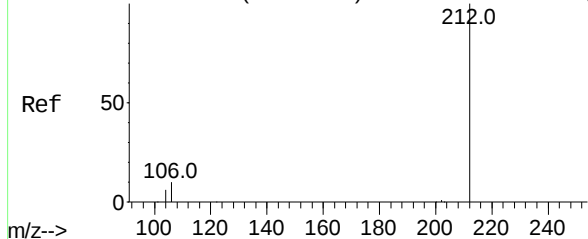


Fluoranthene-d10
Concen: 0.42 ng
RT: 19.126 min Scan# 1830
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	212	Resp:	45469
Ion Ratio	Lower	Upper	
212	100		
106	11.4	9.1	13.7
104	6.4	5.1	7.7



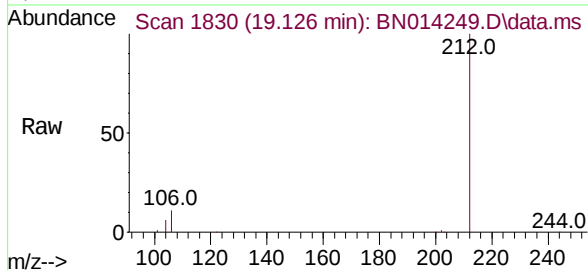


Abundance Scan 1836 (19.156 min): BN014249.D\data.ms (-1798) (-)

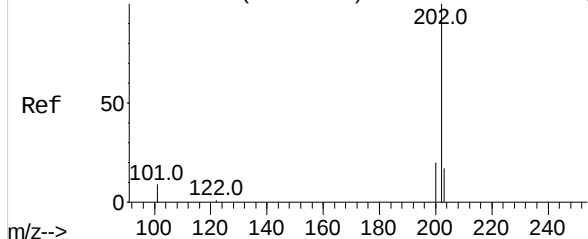


Fluoranthene
Concen: 0.43 ng
RT: 19.156 min Scan# 1836
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:	202	Resp:	49423
Ion Ratio	Lower	Upper	
202	100		
101	9.8	7.8	11.8
203	17.2	13.8	20.6

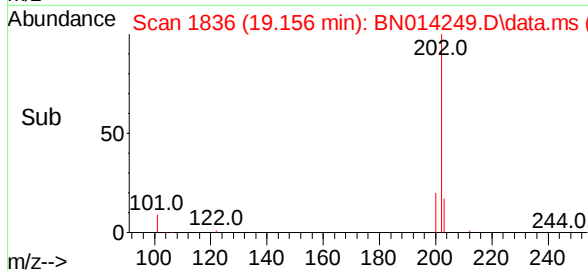




Abundance Scan 2127 (21.279 min): BN014249.D\data.ms (-2108) (-)

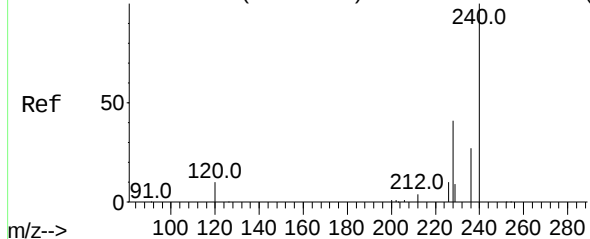


Chrysene-d12
Concen: 0.40 ng
RT: 21.279 min Scan# 2127
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	240	Resp:	36491
Ion	Ratio	Lower	Upper
240	100		
120	11.8	9.4	14.2
236	27.1	21.7	32.5

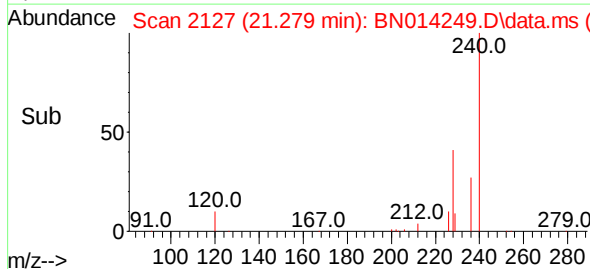
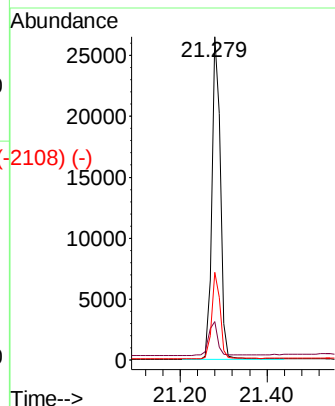
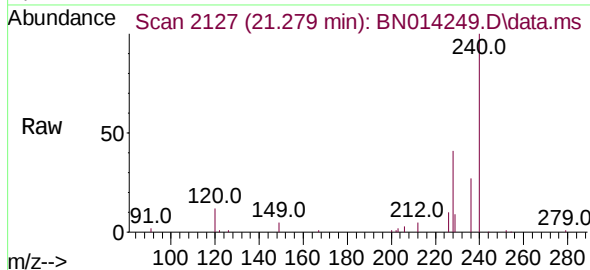


Abundance Scan 1909 (19.518 min): BN014249.D\data.ms (-1869) (-)

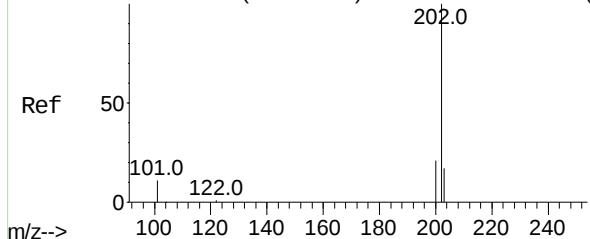

Pyrene
Concen: 0.43 ng
RT: 19.518 min Scan# 1909
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Tgt Ion:	202	Resp:	50126
Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.5	24.7
203	17.4	13.9	20.9

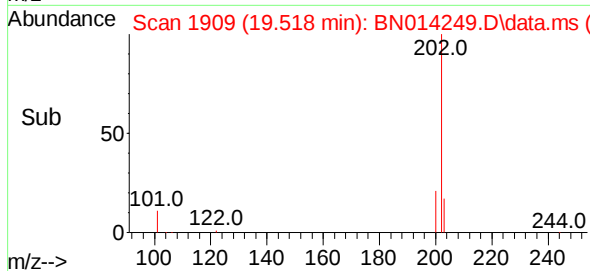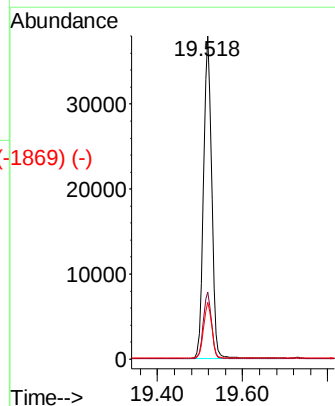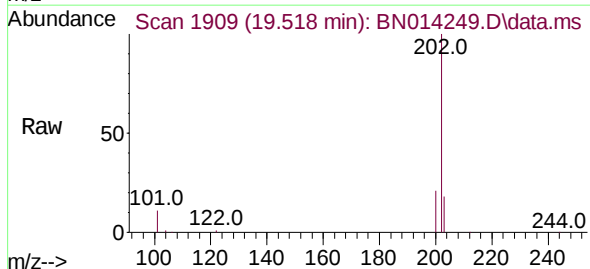




Abundance Scan 1952 (19.732 min): BN014249.D\data.ms (-1934) (-)

Terphenyl-d14
Concen: 0.44 ng
RT: 19.732 min Scan# 1952
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

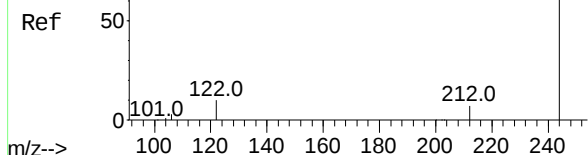





Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.6	6.1	9.1
122	10.3	8.2	12.4

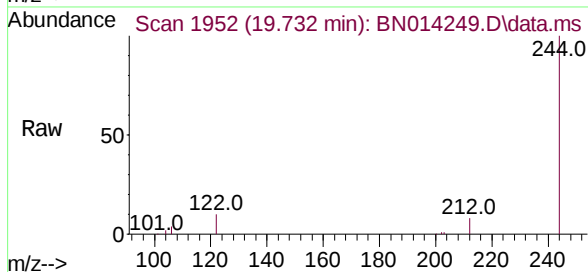


Abundance Scan 2126 (21.268 min): BN014249.D\data.ms (-2120) (-)

Benzo(a)anthracene
Concen: 0.38 ng
RT: 21.268 min Scan# 2126
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.3	21.0	31.6
229	20.0	16.0	24.0

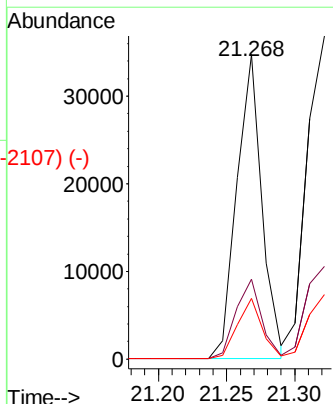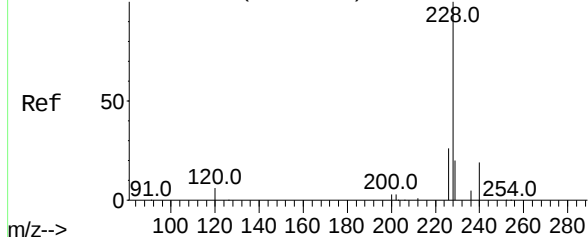




Abundance Scan 2131 (21.322 min): BN014249.D\data.ms (-2128) (-)

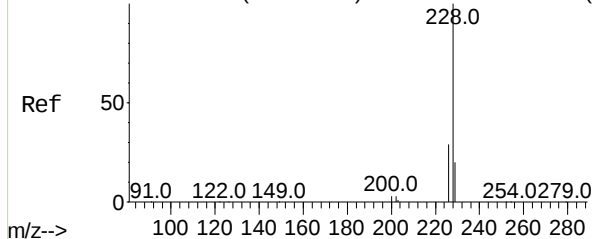


Chrysene
Concen: 0.44 ng
RT: 21.322 min Scan# 2131
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	228	Resp:	49704
Ion Ratio	Lower	Upper	
228	100		
226	28.7	23.0	34.4
229	20.0	16.0	24.0

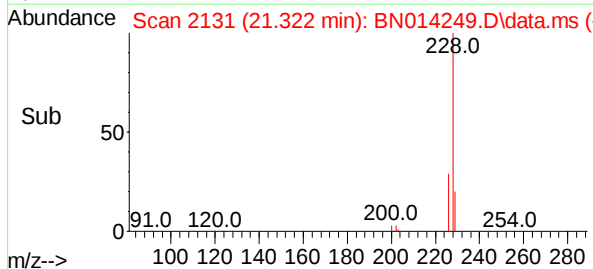

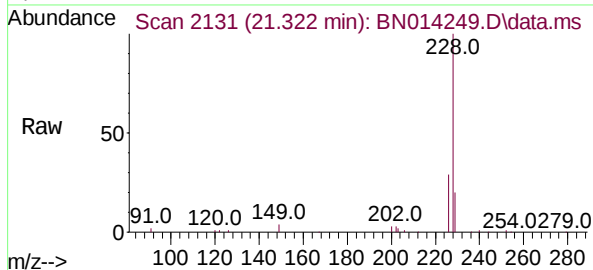


Abundance Scan 2121 (21.215 min): BN014249.D\data.ms (-2128) (-)

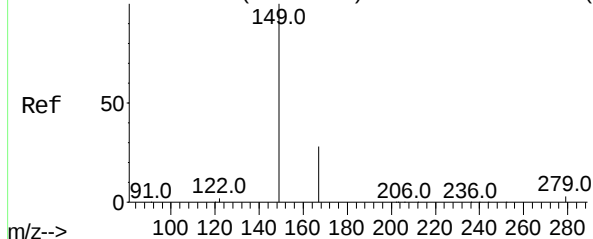

Bis(2-ethylhexyl)phthalate
Concen: 0.20 ng
RT: 21.215 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Tgt Ion:	149	Resp:	14080
Ion Ratio	Lower	Upper	
149	100		
167	27.7	22.3	33.5
279	4.7	4.0	6.0

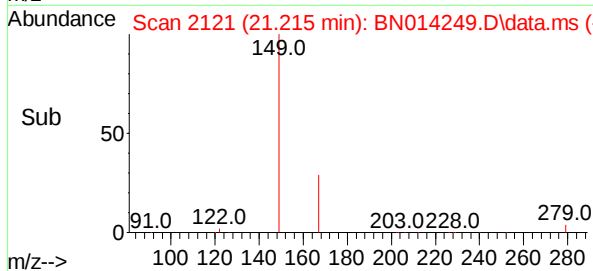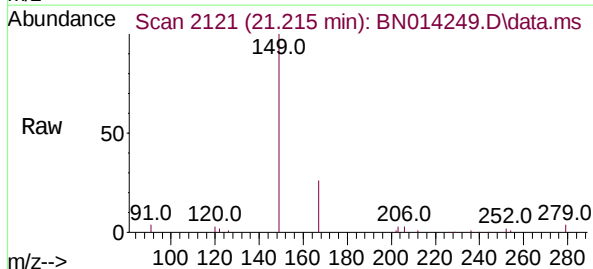




Abundance Scan 3216 (25.769 min): BN014249.D\data.ms (-3185) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.39 ng
RT: 25.769 min Scan# 3216
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

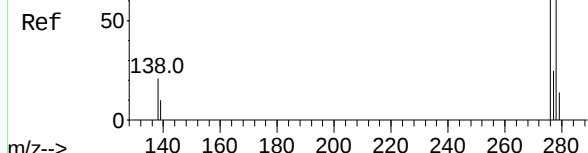


Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.4	17.9	26.9
277	24.9	19.9	29.9



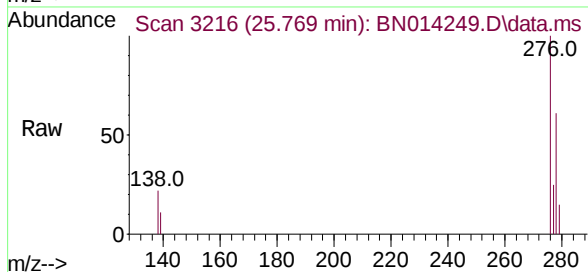


Abundance Scan 2558 (23.517 min): BN014249.D\data.ms (-2536) (-)


Perylene-d12
Concen: 0.40 ng
RT: 23.517 min Scan# 2558
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

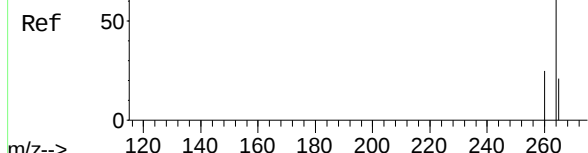

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.8	29.8
265	44.1	35.3	52.9

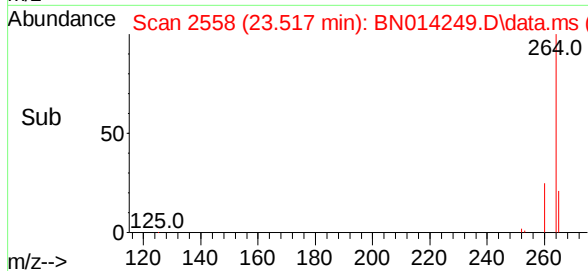



Abundance Scan 2362 (22.846 min): BN014249.D\data.ms (-2362) (-)

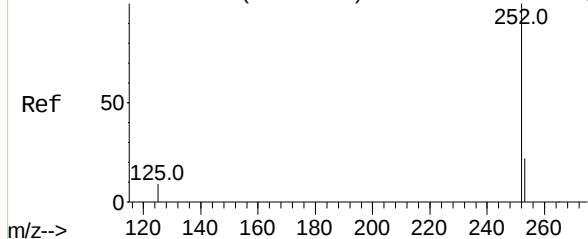


Benzo(b)fluoranthene
Concen: 0.47 ng
RT: 22.846 min Scan# 2362
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	252	Resp:	50245
Ion Ratio	Lower	Upper	
252	100		
253	23.5	18.8	28.2
125	10.8	8.6	13.0

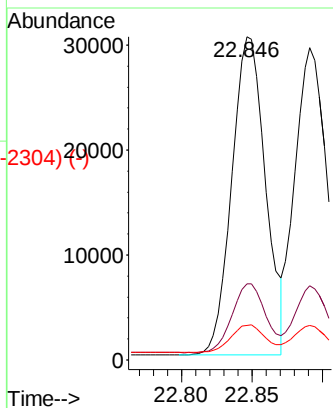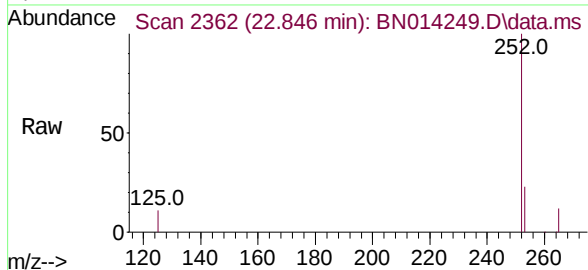

Abundance Scan 2362 (22.846 min): BN014249.D\data.ms (-2304) (-)


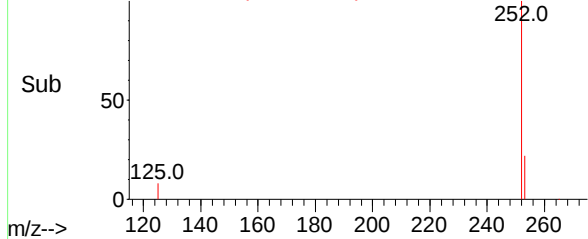


Abundance Scan 2375 (22.891 min): BN014249.D\data.ms (-2368) (-)

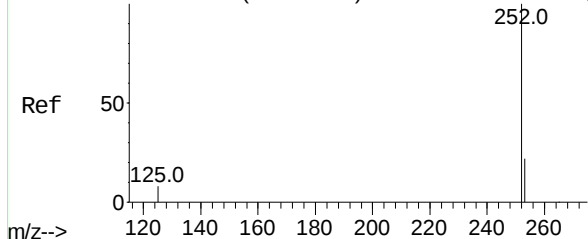


Benzo(k)fluoranthene
Concen: 0.47 ng
RT: 22.891 min Scan# 2375
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion:	252	Resp:	48314
Ion Ratio	Lower	Upper	
252	100		
253	23.7	19.0	28.4
125	11.0	8.8	13.2

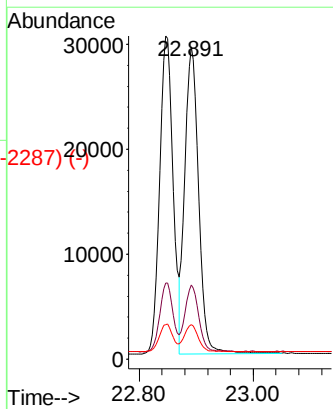


Abundance Scan 2375 (22.891 min): BN014249.D\data.ms (-2287) (-)

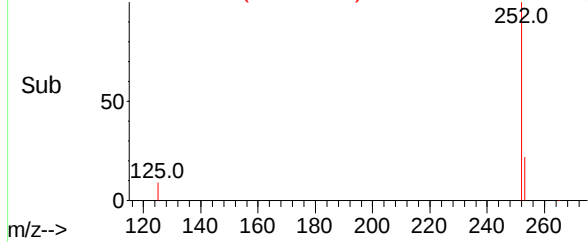



Abundance Scan 2530 (23.421 min): BN014249.D\data.ms (-2530) (-)

Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.421 min Scan# 2530
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08


Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

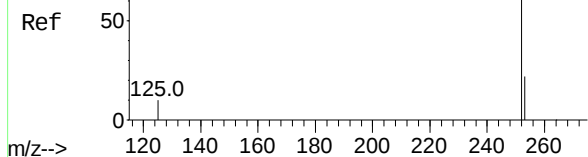

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.9	19.9	29.9
125	13.0	10.4	15.6

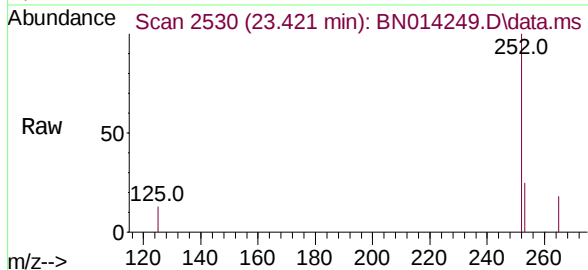




Abundance Scan 2530 (23.421 min): BN014249.D\data.ms (-2472) (-)

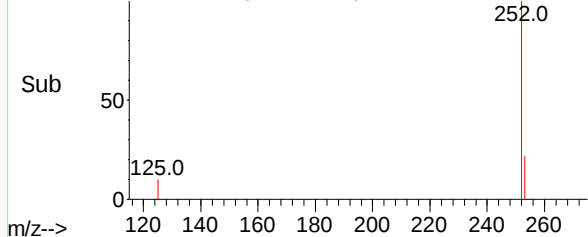


Abundance Scan 3221 (25.787 min): BN014249.D\data.ms (-3221) (-)

Dibenzo(a,h)anthracene
Concen: 0.46 ng
RT: 25.787 min Scan# 3221
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Tgt Ion	Ratio	Lower	Upper
278	100		
139	14.9	11.9	17.9
279	24.9	19.9	29.9

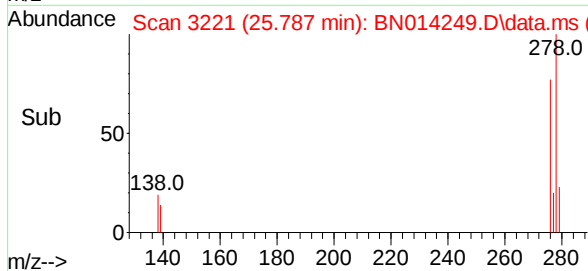

Abundance Scan 3416 (26.454 min): BN014249.D\data.ms (-3358) (-)

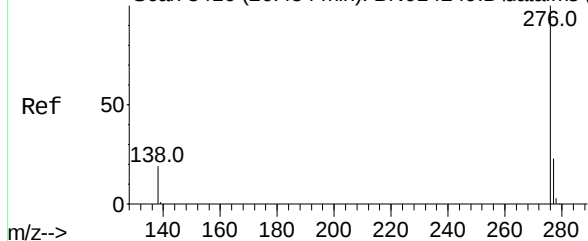

Benzo(g,h,i)perylene
Concen: 0.47 ng
RT: 26.454 min Scan# 3416
Delta R.T. 0.000 min
Lab File: BN014249.D
Acq: 09 Apr 2021 12:08

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:	276	Resp:	48192
Ion	Ratio	Lower	Upper
276	100		
277	24.1	19.3	28.9
138	19.6	15.7	23.5

