
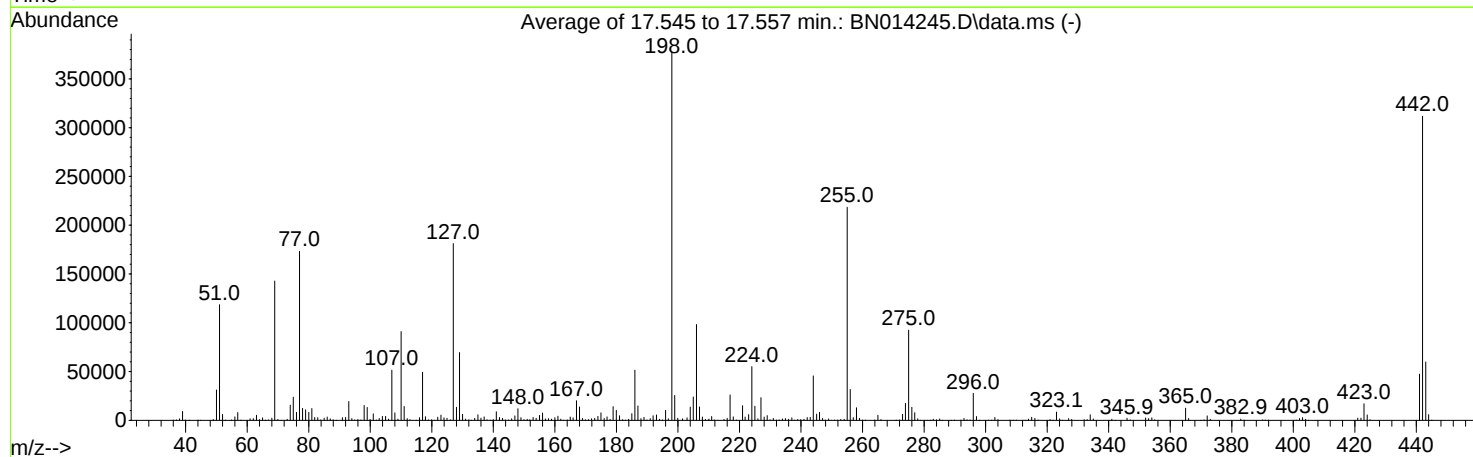


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
 Data File : BN014245.D
 Acq On : 09 Apr 2021 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 09 15:06:44 2021

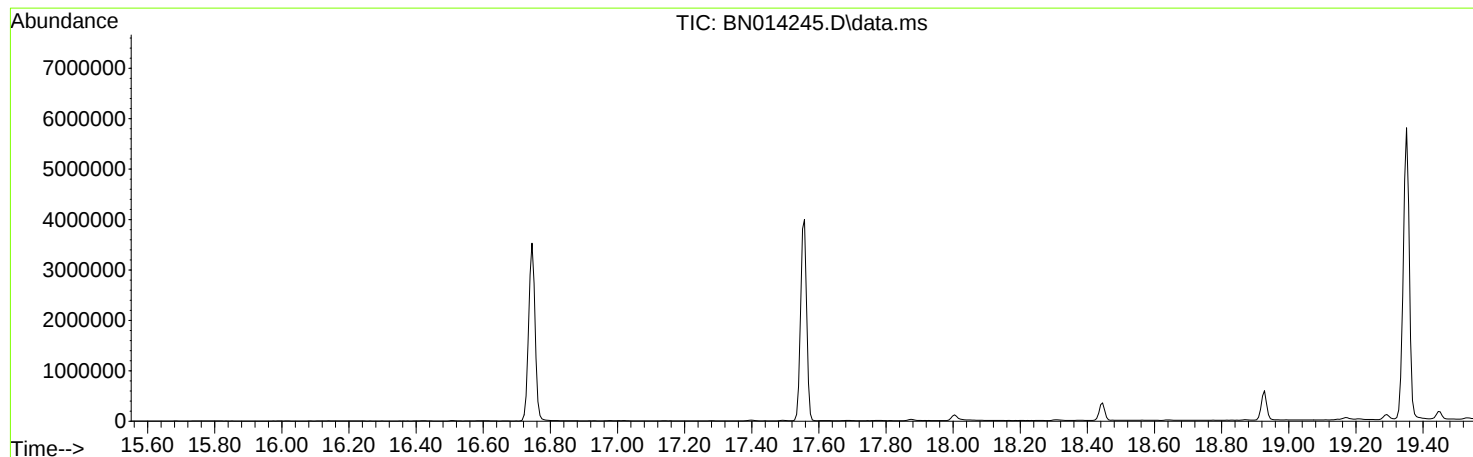

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	118613	PASS
68	69	0.00	2	1.7	2378	PASS
69	198	0.00	100	37.9	142811	PASS
70	69	0.00	2	0.6	926	PASS
127	198	10	80	48.1	181155	PASS
197	198	0.00	2	0.5	1725	PASS
198	198	100	100	100.0	377003	PASS
199	198	5	9	6.8	25595	PASS
275	198	10	60	24.5	92549	PASS
365	198	1	100	3.3	12528	PASS
441	198	0.01	100	12.6	47435	PASS
442	442	50	100	100.0	311701	PASS
443	442	15	24	19.2	59813	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/9/2021	BNA_N	<u>BN014245.D</u>
Compound Name	Response	Retention Time
DDT	1759525	20.598
DDD	12402	20.151
DDE	1765	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14167	1773692	0.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
 Data File : BN014245.D
 Acq On : 09 Apr 2021 08:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 09 09:55:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 09 09:55:03 2021
 Response via : Initial Calibration

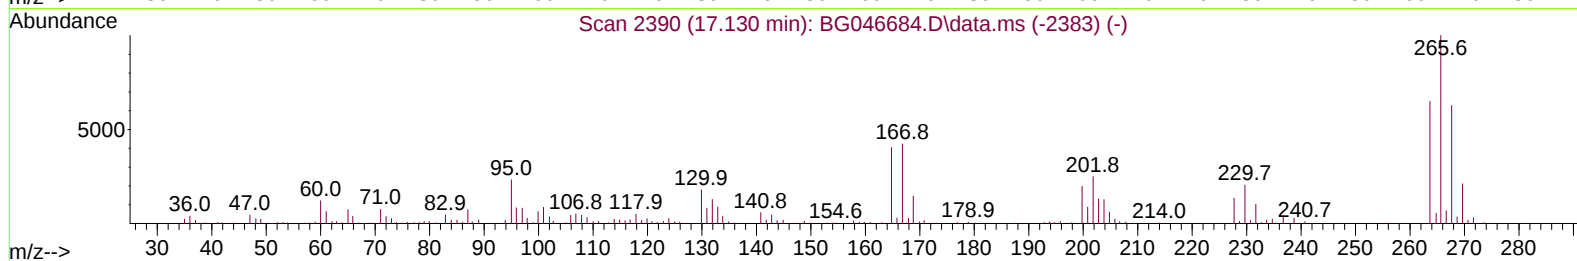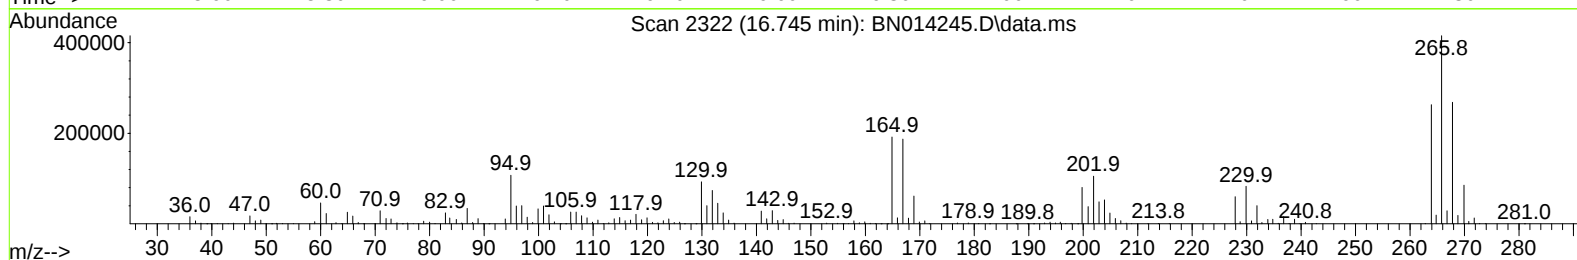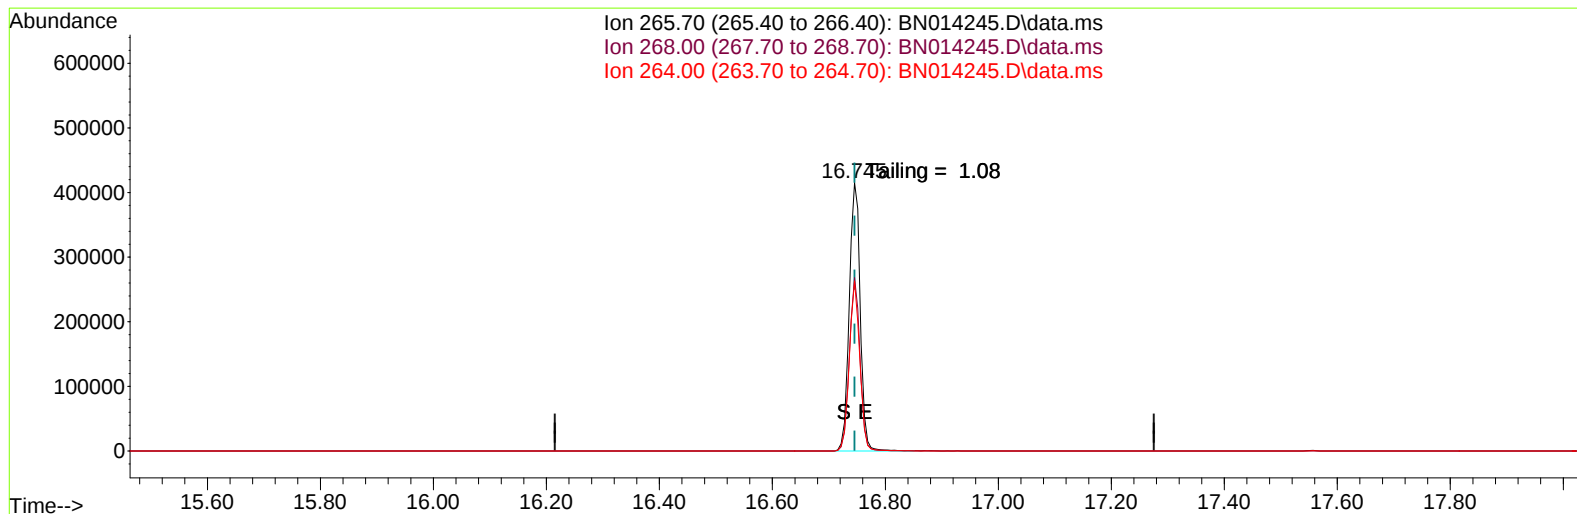

TIC: BN014245.D\data.ms

(70) Pentachlorophenol (C)

16.745min (0.000) 28184.99 ng




response 561377

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.59
264.00	61.60	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040921\
Data File : BN014245.D
Acq On : 09 Apr 2021 08:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 09 09:55:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 09 09:55:03 2021
Response via : Initial Calibration

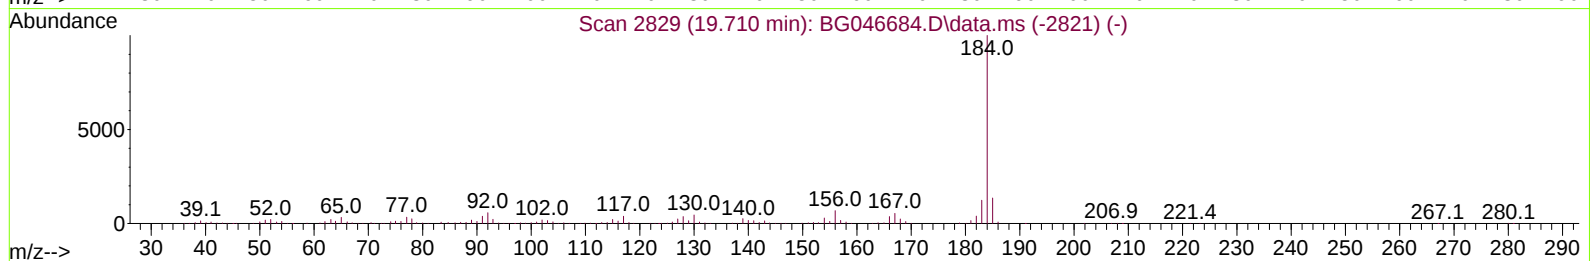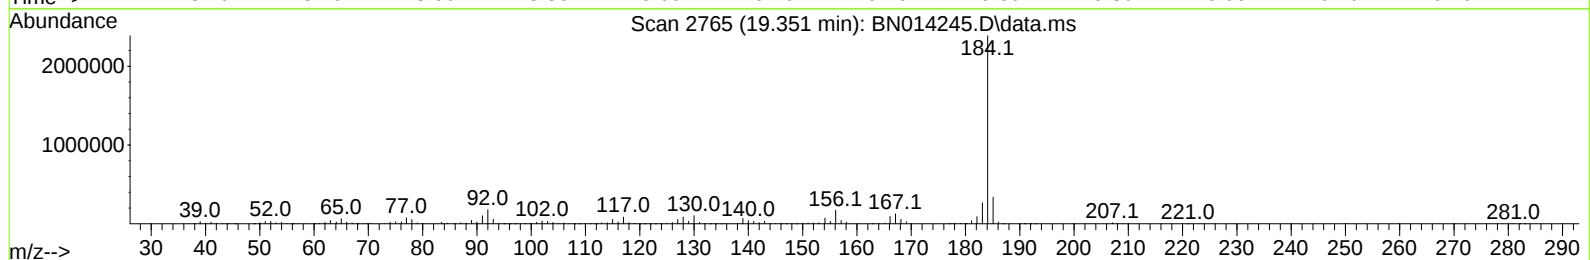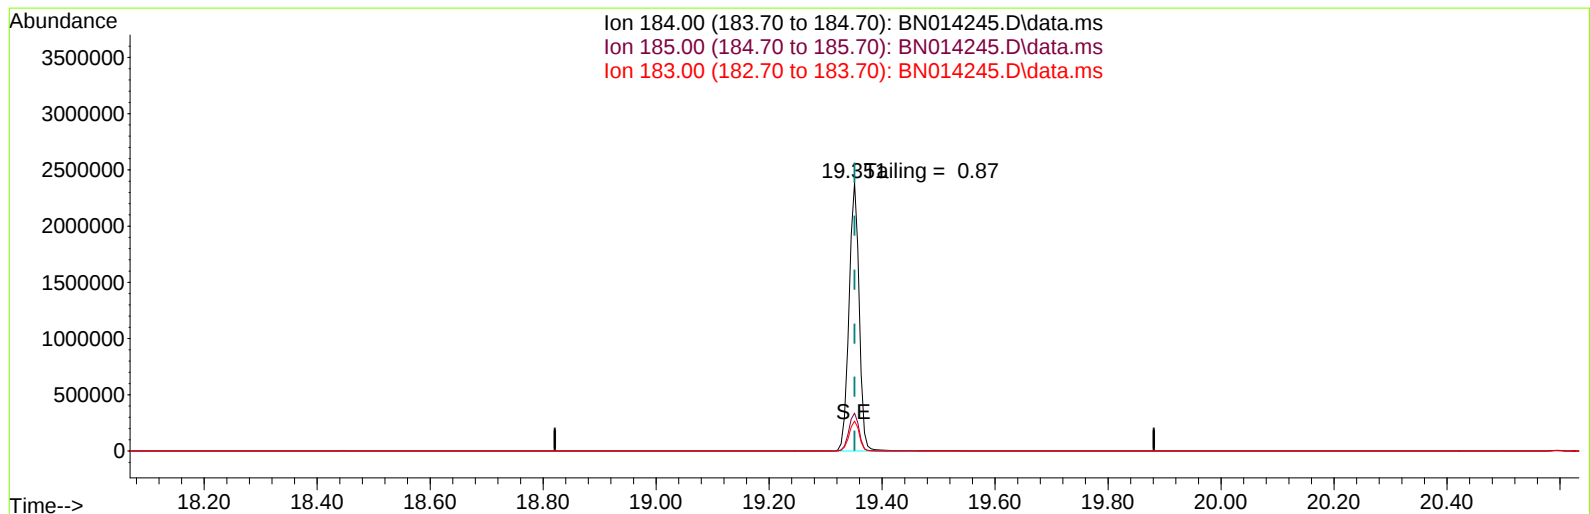

TIC: BN014245.D\data.ms

(77) Benzidine

19.351min (0.000) 0.00 ng

response 2985737

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.19
0.00	0.00	0.00