

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041023\
 Data File : BN024820.D
 Acq On : 10 Apr 2023 11:55
 Operator : CG/JU
 Sample : SSTD01090
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010212

Quant Time: Apr 11 02:39:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 10 15:00:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	390253	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	1745639	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.593	164	1088625	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.334	188	2277425	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	2124389	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	2310070	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	39867	3.912	ng/uL	0.00
4) Pyridine-d5	3.740	84	290114	9.449	ng/u1	0.00
7) Phenol-d5	7.099	99	352214	9.257	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	249920	9.821	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	269183	9.627	ng/u1	0.00
15) 4-Methylphenol-d8	8.658	113	279875	9.266	ng/u1	0.00
21) Nitrobenzene-d5	9.110	128	131603	9.311	ng/u1	0.00
24) 2-Nitrophenol-d4	9.840	143	142264	9.293	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	265269	9.694	ng/u1	0.00
31) 4-Chloroaniline-d4	10.899	131	395490	9.524	ng/u1	0.00
46) Dimethylphthalate-d6	13.998	166	827676	9.807	ng/u1	0.00
49) Acenaphthylene-d8	14.281	160	943486	9.756	ng/u1	0.00
54) 4-Nitrophenol-d4	14.781	143	151599	8.763	ng/u1	0.00
60) Fluorene-d10	15.581	176	712537	10.000	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	121515	8.199	ng/u1	0.00
73) Anthracene-d10	17.434	188	1067274	9.978	ng/u1	0.00
81) Pyrene-d10	19.728	212	1207324	9.787	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.810	264	1203862	9.967	ng/u1	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	43679	3.947	ng/uL	98
5) Pyridine	3.764	79	295836	9.326	ng/u1	94
6) Benzaldehyde	7.081	77	219682	11.796	ng/u1	98
8) Phenol	7.128	94	373855	9.435	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.364	93	303378	9.752	ng/u1	98
12) 2-Chlorophenol	7.505	128	282136	9.661	ng/u1	98
13) 2-Methylphenol	8.387	108	269807	9.274	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.469	45	609363	9.976	ng/u1	98
16) Acetophenone	8.775	105	472001	9.883	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.758	70	249350	9.679	ng/u1	99
18) 4-Methylphenol	8.716	108	304490	9.412	ng/u1	92
19) Hexachloroethane	9.028	117	112246	9.524	ng/u1	100
22) Nitrobenzene	9.158	77	370772	9.762	ng/u1	98
23) Isophorone	9.681	82	660661	9.476	ng/u1	100
25) 2-Nitrophenol	9.869	139	156447	9.473	ng/u1	97
26) 2,4-Dimethylphenol	9.928	107	337462	9.705	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.163	93	428129	9.868	ng/u1	99
29) 2,4-Dichlorophenol	10.405	162	266919	9.719	ng/u1	98
30) Naphthalene	10.810	128	964314	9.891	ng/u1	99
32) 4-Chloroaniline	10.922	127	407622	9.696	ng/u1	97
33) Hexachlorobutadiene	11.093	225	158399	9.895	ng/u1	95
34) Caprolactam	11.687	113	46314	4.815	ng/u1	97
35) 4-Chloro-3-methylphenol	12.040	107	309482	9.611	ng/u1	99
36) 2-Methylnaphthalene	12.416	142	633044	9.825	ng/u1	99


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041023\
 Data File : BN024820.D
 Acq On : 10 Apr 2023 11:55
 Operator : CG/JU
 Sample : SSTD01090
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD010212

Quant Time: Apr 11 02:39:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041023.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 10 15:00:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.634	142	638201	9.922	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.787	216	314069	9.891	ng/ul	96
40) Hexachlorocyclopentadiene	12.763	237	173643	8.968	ng/ul	96
41) 2,4,6-Trichlorophenol	13.022	196	209251	9.645	ng/ul	96
42) 2,4,5-Trichlorophenol	13.093	196	230242	9.697	ng/ul	98
43) 1,1'-Biphenyl	13.422	154	859910	9.914	ng/ul	97
44) 2-Chloronaphthalene	13.469	162	662035	9.830	ng/ul	98
45) 2-Nitroaniline	13.675	65	215232	9.152	ng/ul	100
47) Dimethylphthalate	14.046	163	837324	9.861	ng/ul	98
48) 2,6-Dinitrotoluene	14.169	165	150001	9.050	ng/ul	96
50) Acenaphthylene	14.310	152	1059350	9.973	ng/ul	99
51) 3-Nitroaniline	14.498	138	161159	9.253	ng/ul	98
52) Acenaphthene	14.651	153	727656	9.909	ng/ul	99
53) 2,4-Dinitrophenol	14.698	184	72678	6.820	ng/ul	90
55) 4-Nitrophenol	14.798	109	127886	9.083	ng/ul	97
56) Dibenzofuran	14.987	168	1002765	9.907	ng/ul	97
57) 2,4-Dinitrotoluene	14.951	165	224534	9.359	ng/ul#	99
58) 2,3,4,6-Tetrachlorophenol	15.210	232	193965	9.921	ng/ul	99
59) Diethylphthalate	15.404	149	835465	9.792	ng/ul	98
61) Fluorene	15.634	166	818365	10.052	ng/ul	96
62) 4-Chlorophenyl-phenyle...	15.628	204	385338	10.169	ng/ul	96
63) 4-Nitroaniline	15.657	138	157072	9.295	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.716	198	124163	8.552	ng/ul#	95
67) N-Nitrosodiphenylamine	15.845	169	695464	10.066	ng/ul	96
68) 4-Bromophenyl-phenylether	16.522	248	229464	10.024	ng/ul	94
69) Hexachlorobenzene	16.639	284	258070	9.957	ng/ul	97
70) Atrazine	16.792	200	222589	9.468	ng/ul	98
71) Pentachlorophenol	16.987	266	147228	9.139	ng/ul	91
72) Phenanthrene	17.381	178	1275576	9.925	ng/ul	99
74) Anthracene	17.469	178	1308060	10.101	ng/ul	98
75) 1,2,3,4-Tetrachloroben...	13.393	216	322728	9.963	ng/uL	98
76) Pentachlorobenzene	14.904	250	309314	9.981	ng/uL	97
77) Carbazole	17.739	167	1173547	10.036	ng/ul	100
78) Di-n-butylphthalate	18.298	149	1326064	9.554	ng/ul	99
80) Fluoranthene	19.392	202	1431076	9.679	ng/ul	99
82) Pyrene	19.757	202	1559321	10.020	ng/ul	98
83) Butylbenzylphthalate	20.657	149	589196	9.119	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.445	252	435617	8.937	ng/ul	99
85) Benzo(a)anthracene	21.516	228	1510368	9.899	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.433	149	905310	9.386	ng/ul	99
87) Chrysene	21.569	228	1434883	9.873	ng/ul	98
89) Di-n-octyl phthalate	22.374	149	1493729	9.409	ng/ul	100
90) Benzo(b)fluoranthene	23.227	252	1495026	9.868	ng/ul	95
91) Benzo(k)fluoranthene	23.274	252	1502941	10.082	ng/ul	99
93) Benzo(a)pyrene	23.863	252	1290801	9.732	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.504	276	1509721	9.566	ng/ul	99
95) Dibenzo(a,h)anthracene	26.527	278	1270054	9.726	ng/ul	99
96) Benzo(g,h,i)perylene	27.298	276	1210825	9.504	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed







#2
 1,4-Dioxane
 Concen: 3.947 ng/uL
 RT: 3.346 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55

Instrument :
 BNA_N
 ClientSampleId :
 SST010212

Tgt Ion: 88 Resp: 43679




Ion	Ratio	Lower	Upper
88	100		
43	40.8	33.0	49.4
58	88.1	72.3	108.5

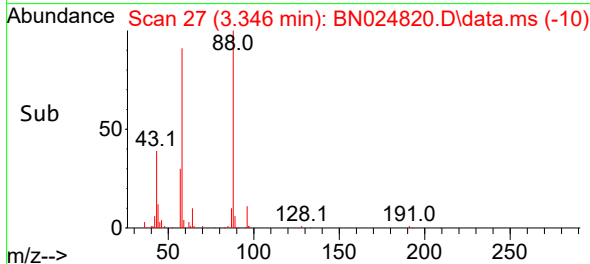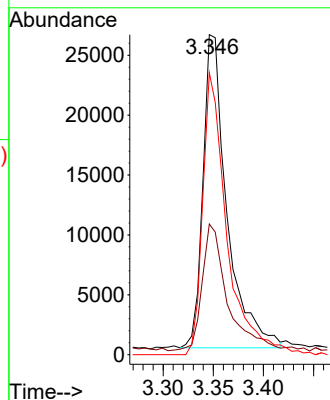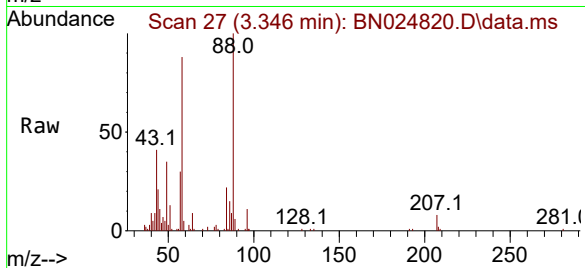


#5
 Pyridine
 Concen: 9.326 ng/uL
 RT: 3.764 min Scan# 98
 Delta R.T. 0.006 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55

Tgt Ion: 79 Resp: 295836

Ion	Ratio	Lower	Upper
79	100		
52	101.3	76.1	114.1
51	47.1	35.8	53.6


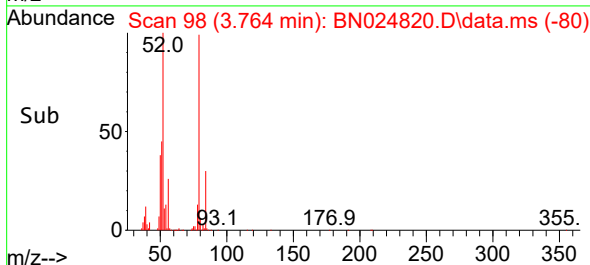
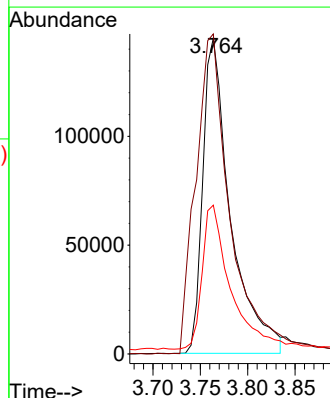
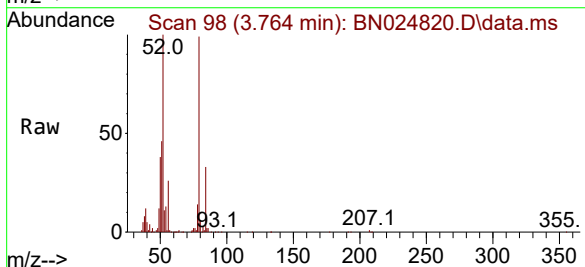




#6
Benzaldehyde
Concen: 11.796 ng/ul
RT: 7.081 min Scan# 662
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion: 77 Resp: 219682
Ion Ratio Lower Upper
77 100
105 93.4 74.3 111.5
106 87.8 73.3 109.9

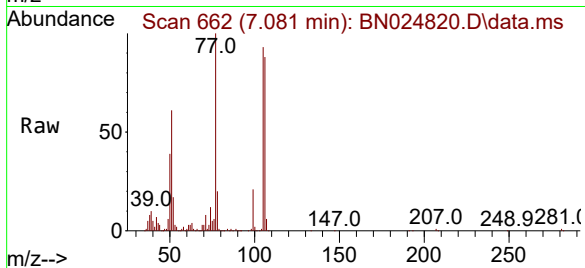

#8
Phenol
Concen: 9.435 ng/ul
RT: 7.128 min Scan# 670
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion: 94 Resp: 373855
Ion Ratio Lower Upper
94 100
65 32.1 25.1 37.7
66 40.9 31.9 47.9


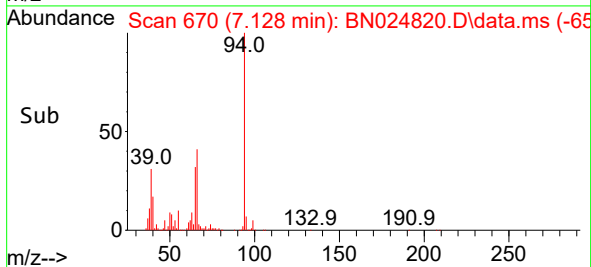

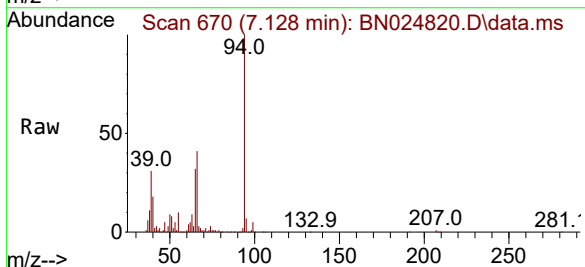




#10
Bis(2-Chloroethyl)ether
Concen: 9.752 ng/ul
RT: 7.364 min Scan# 710
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion: 93 Resp: 303378
Ion Ratio Lower Upper
93 100
63 90.4 70.9 106.3
95 33.1 26.0 39.0

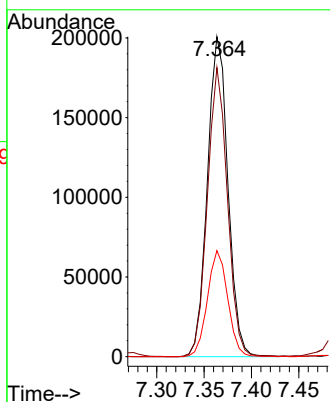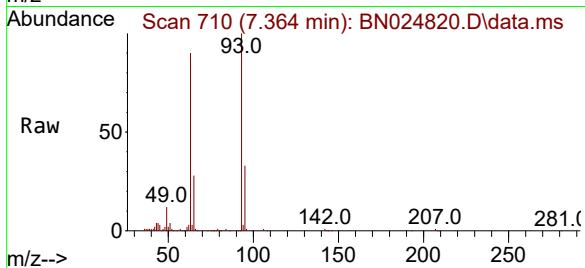

#12
2-Chlorophenol
Concen: 9.661 ng/ul
RT: 7.505 min Scan# 734
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:128 Resp: 282136
Ion Ratio Lower Upper
128 100
64 55.3 44.8 67.2
130 31.2 26.6 39.8

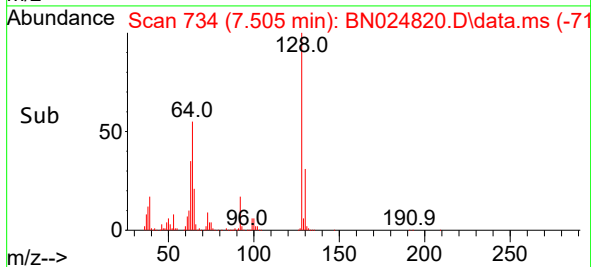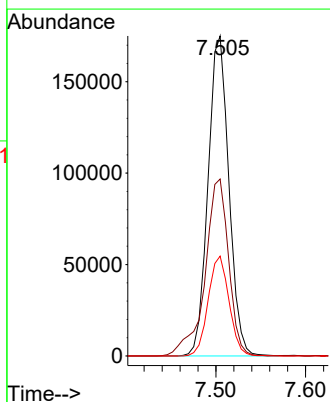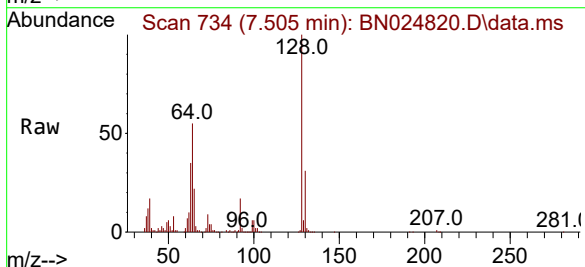



#13

2-Methylphenol

Concen: 9.274 ng/ul

RT: 8.387 min Scan# 884

Delta R.T. -0.006 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :





SSTD010212

Tgt Ion:108 Resp: 269807

Ion Ratio Lower Upper

108 100

107 92.6 71.5 107.3



#14

2,2'-oxybis(1-Chloropropane)

Concen: 9.976 ng/ul

RT: 8.469 min Scan# 898

Delta R.T. -0.012 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55




Tgt Ion: 45 Resp: 609363


Ion Ratio Lower Upper

45 100

77 9.9 8.4 12.6

79 7.4 6.6 9.8


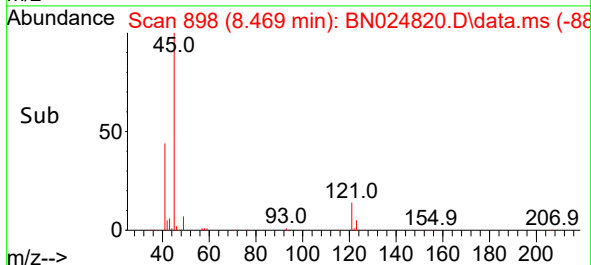
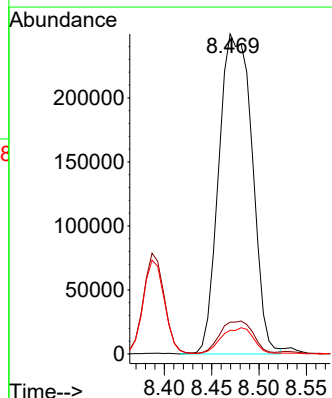
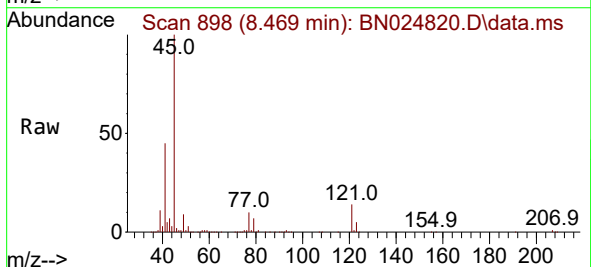




#16
 Acetophenone
 Concen: 9.883 ng/ul
 RT: 8.775 min Scan# 950
 Delta R.T. 0.000 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55




Instrument :
 BNA_N
 ClientSampleId :
 SSTD010212


Tgt Ion: 105 Resp: 472001
 Ion Ratio Lower Upper
 105 100
 77 83.0 64.8 97.2
 51 35.8 28.7 43.1



#17
 N-Nitroso-di-n-propylamine
 Concen: 9.679 ng/ul
 RT: 8.758 min Scan# 947
 Delta R.T. 0.000 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55

Tgt Ion: 70 Resp: 249350
 Ion Ratio Lower Upper
 70 100
 42 79.3 64.2 96.2
 101 8.8 7.3 10.9
 130 18.1 15.0 22.6









#18
4-Methylphenol
Concen: 9.412 ng/ul
RT: 8.716 min Scan# 941
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:108 Resp: 304490
Ion Ratio Lower Upper
108 100
107 115.5 85.8 128.6

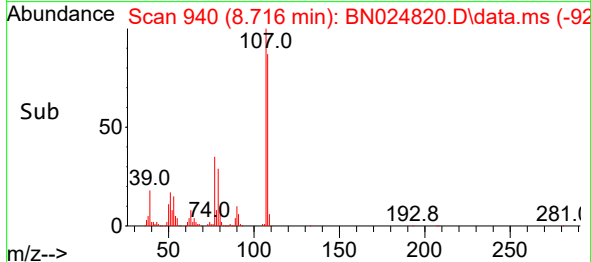

#19
Hexachloroethane
Concen: 9.524 ng/ul
RT: 9.028 min Scan# 993
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:117 Resp: 112246
Ion Ratio Lower Upper
117 100
201 90.9 72.2 108.4
199 57.8 46.2 69.4


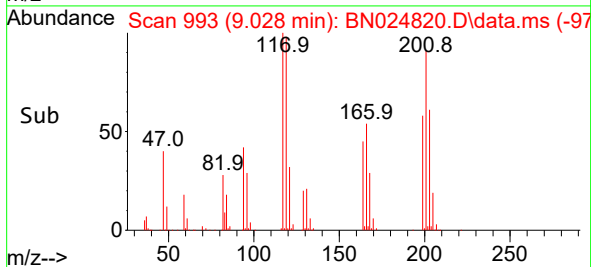

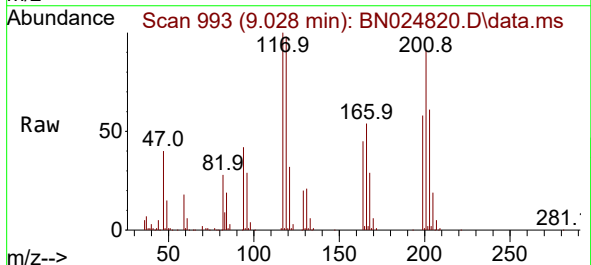




#22
Nitrobenzene
Concen: 9.762 ng/ul
RT: 9.158 min Scan# 1015
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion: 77 Resp: 370772
Ion Ratio Lower Upper
77 100
123 40.6 33.5 50.3
65 13.9 11.8 17.8

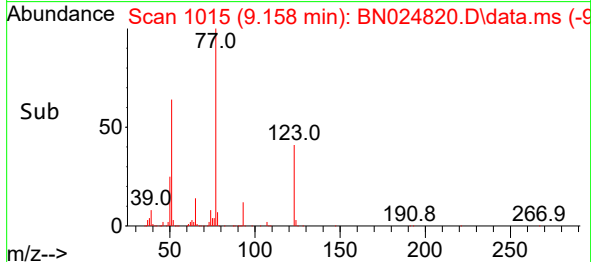

#23
Isophorone
Concen: 9.476 ng/ul
RT: 9.681 min Scan# 1104
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion: 82 Resp: 660661
Ion Ratio Lower Upper
82 100
95 6.9 5.4 8.0
138 15.9 12.8 19.2


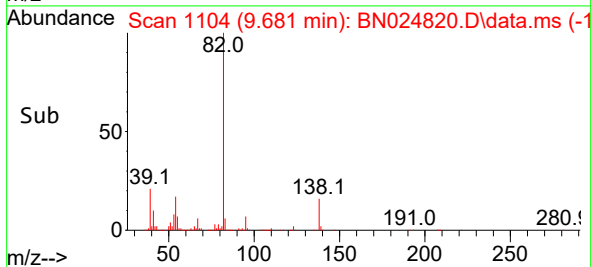

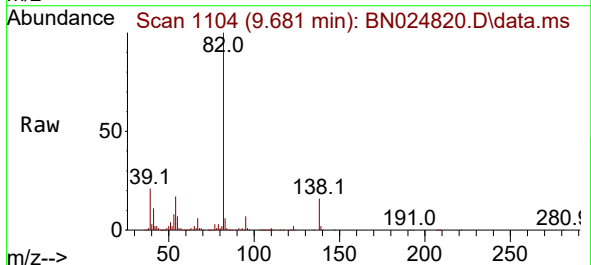




#25
2-Nitrophenol
Concen: 9.473 ng/ul
RT: 9.869 min Scan# 1136
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:139 Resp: 156447
Ion Ratio Lower Upper
139 100
65 60.4 49.8 74.8
109 29.7 26.2 39.2



#26
2,4-Dimethylphenol
Concen: 9.705 ng/ul
RT: 9.928 min Scan# 1146
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:107 Resp: 337462
Ion Ratio Lower Upper
107 100
121 50.7 39.7 59.5
122 82.7 66.1 99.1









#27
 Bis(2-Chloroethoxy)methane
 Concen: 9.868 ng/ul
 RT: 10.163 min Scan# 1187
 Delta R.T. -0.006 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55




Instrument :
 BNA_N
 ClientSampleId :
 SST010212


Tgt Ion: 93 Resp: 428129
 Ion Ratio Lower Upper
 93 100
 95 31.8 26.1 39.1
 123 10.5 8.5 12.7

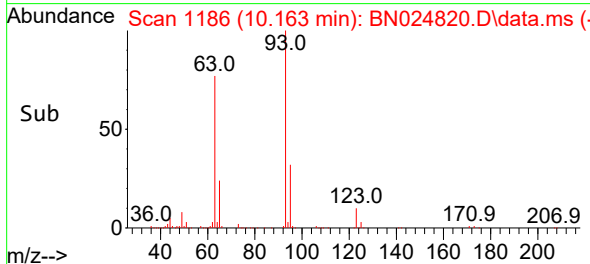

#29
 2,4-Dichlorophenol
 Concen: 9.719 ng/ul
 RT: 10.405 min Scan# 1227
 Delta R.T. 0.000 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55

Tgt Ion:162 Resp: 266919
 Ion Ratio Lower Upper
 162 100
 164 65.9 50.9 76.3
 98 38.2 31.0 46.4

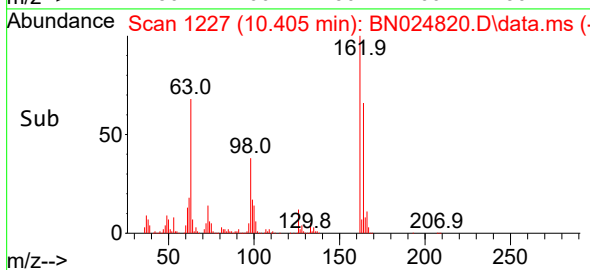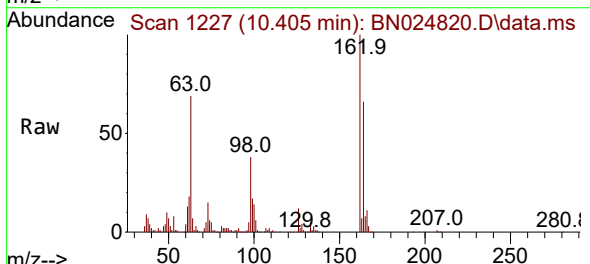



#30

Naphthalene

Concen: 9.891 ng/ul

RT: 10.810 min Scan# 1296

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:128 Resp: 964314

Ion Ratio Lower Upper

128 100

129 11.0 8.4 12.6

127 13.1 10.7 16.1



#32

4-Chloroaniline

Concen: 9.696 ng/ul

RT: 10.922 min Scan# 1315

Delta R.T. 0.000 min

Lab File: BN024820.D




Acq: 10 Apr 2023 11:55


Tgt Ion:127 Resp: 407622

Ion Ratio Lower Upper

127 100

129 33.3 25.5 38.3









#33
Hexachlorobutadiene
Concen: 9.895 ng/ul
RT: 11.093 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:225 Resp: 158399
Ion Ratio Lower Upper
225 100
223 62.7 45.9 68.9
227 62.3 51.2 76.8

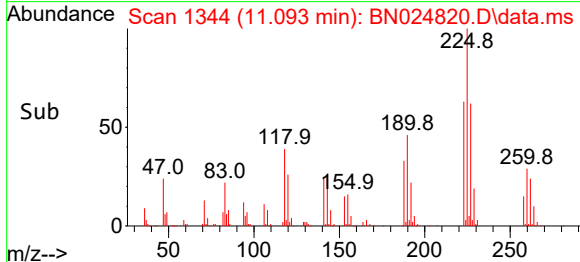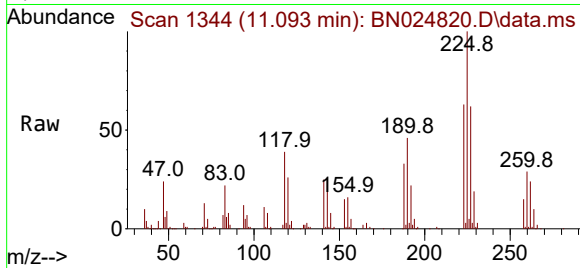

#34
Caprolactam
Concen: 4.815 ng/ul
RT: 11.687 min Scan# 1445
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:113 Resp: 46314
Ion Ratio Lower Upper
113 100
55 229.1 188.3 282.5
56 164.3 133.5 200.3

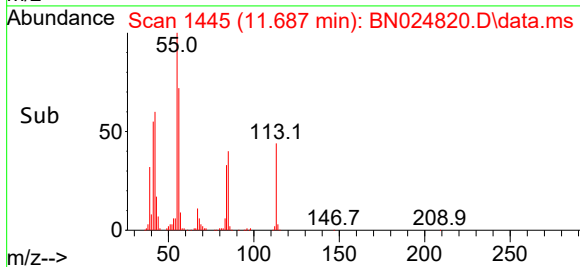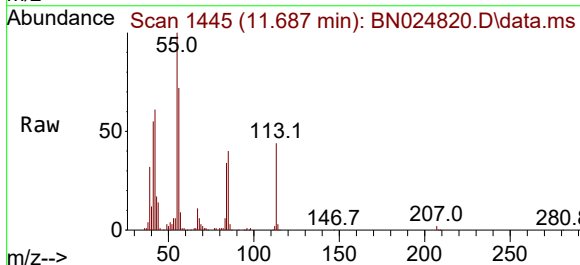



#35

4-Chloro-3-methylphenol

Concen: 9.611 ng/ul

RT: 12.040 min Scan# 1506

Delta R.T. -0.006 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:107 Resp: 309482

Ion Ratio Lower Upper

107 100

144 23.9 19.6 29.4

142 77.1 60.7 91.1

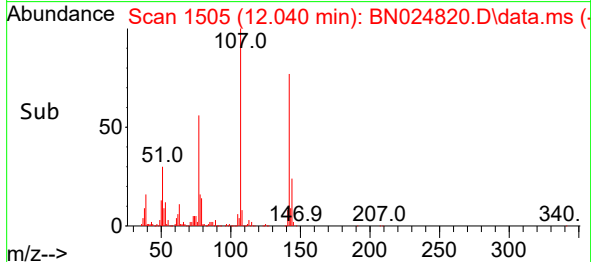

#36

2-Methylnaphthalene

Concen: 9.825 ng/ul

RT: 12.416 min Scan# 1569

Delta R.T. 0.000 min

Lab File: BN024820.D




Acq: 10 Apr 2023 11:55


Tgt Ion:142 Resp: 633044

Ion Ratio Lower Upper

142 100

141 88.4 71.4 107.2

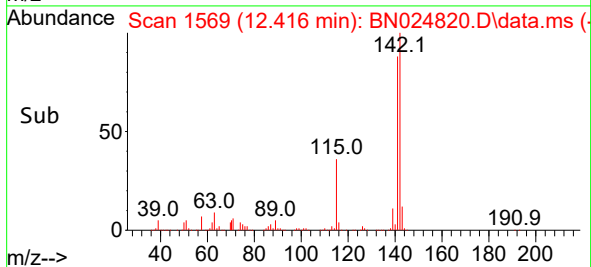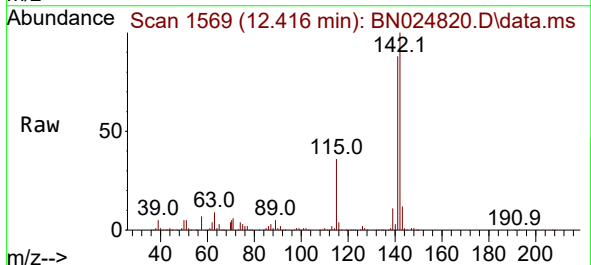



#37

1-Methylnaphthalene

Concen: 9.922 ng/ul

RT: 12.634 min Scan# 1606

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:142 Resp: 638201

Ion Ratio Lower Upper

142 100

141 92.2 73.5 110.3

116 3.8 3.1 4.7

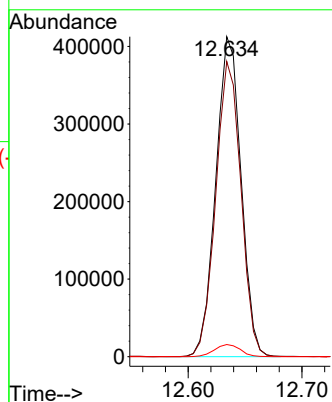

#39

1,2,4,5-Tetrachlorobenzene

Concen: 9.891 ng/ul

RT: 12.787 min Scan# 1632

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Tgt Ion:216 Resp: 314069




Ion Ratio Lower Upper


216 100

214 81.8 62.2 93.4

179 20.7 16.8 25.2

108 20.3 15.0 22.6


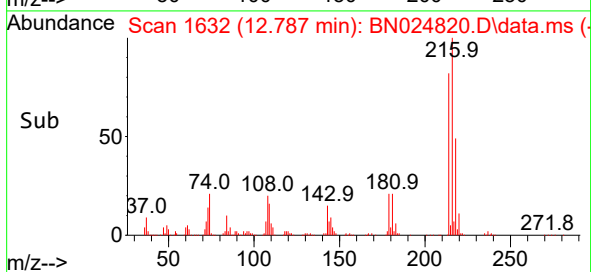






#40
Hexachlorocyclopentadiene
Concen: 8.968 ng/ul
RT: 12.763 min Scan# 1628
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:237 Resp: 173643
Ion Ratio Lower Upper
237 100
235 65.6 49.9 74.9
272 13.1 10.2 15.4

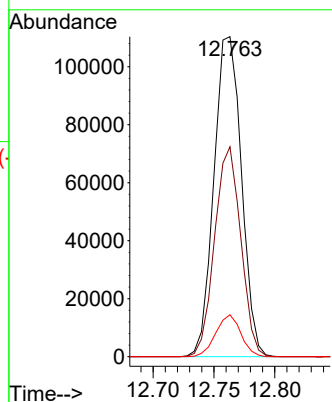

#41
2,4,6-Trichlorophenol
Concen: 9.645 ng/ul
RT: 13.022 min Scan# 1672
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:196 Resp: 209251
Ion Ratio Lower Upper
196 100
198 96.8 74.5 111.7
200 32.8 24.3 36.5

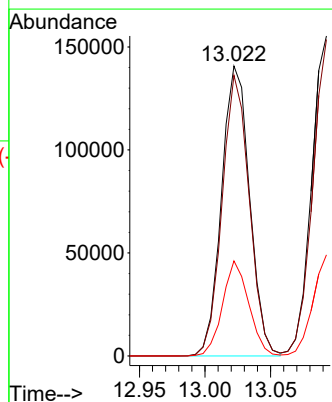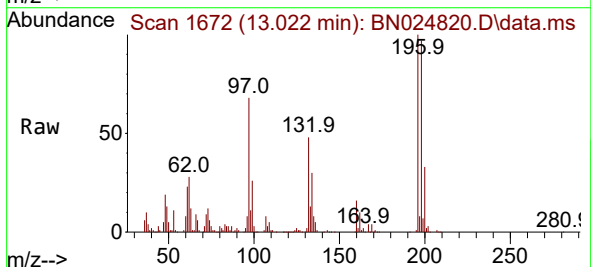



#42

2,4,5-Trichlorophenol

Concen: 9.697 ng/ul

RT: 13.093 min Scan# 1

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:196 Resp: 230242

Ion Ratio Lower Upper

196 100

198 98.9 78.2 117.2

200 31.6 24.0 36.0



#43

1,1'-Biphenyl

Concen: 9.914 ng/ul

RT: 13.422 min Scan# 1740

Delta R.T. -0.006 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55




Tgt Ion:154 Resp: 859910


Ion Ratio Lower Upper

154 100

153 38.1 32.2 48.2

76 15.1 12.4 18.6









#44
2-Chloronaphthalene
Concen: 9.830 ng/ul
RT: 13.469 min Scan# 1748
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:162 Resp: 662035
Ion Ratio Lower Upper
162 100
164 31.0 25.9 38.9
127 39.8 32.9 49.3

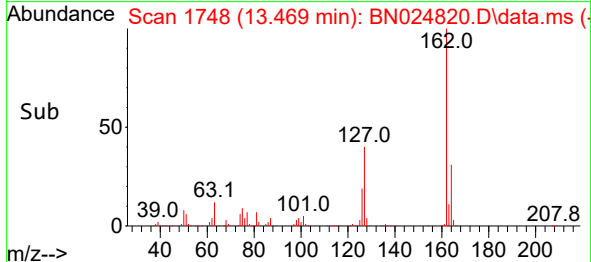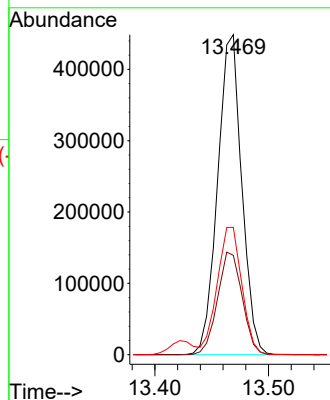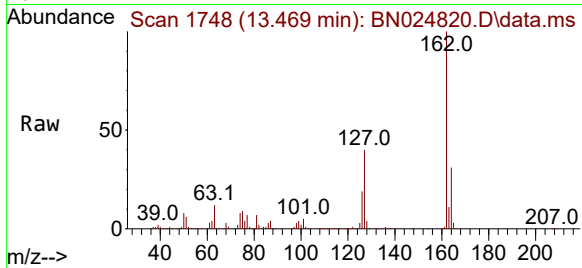

#45
2-Nitroaniline
Concen: 9.152 ng/ul
RT: 13.675 min Scan# 1783
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion: 65 Resp: 215232
Ion Ratio Lower Upper
65 100
92 63.1 50.7 76.1
138 89.2 71.4 107.2


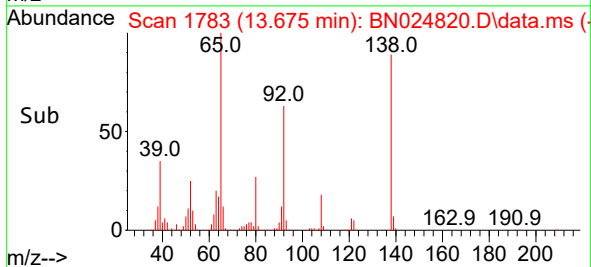
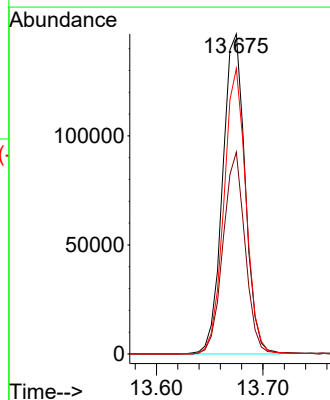
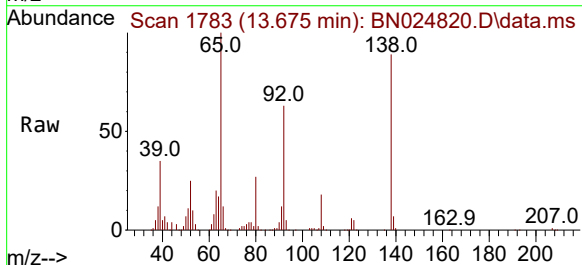




#47
Dimethylphthalate
Concen: 9.861 ng/ul
RT: 14.046 min Scan# 1846
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:163 Resp: 837324
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 9.3 8.2 12.2

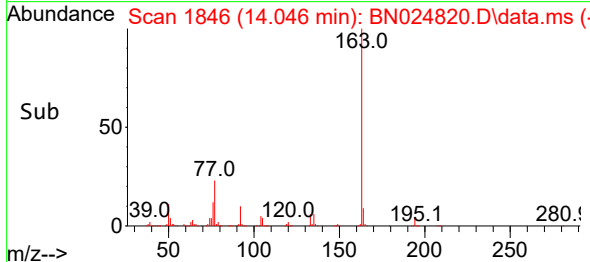

#48
2,6-Dinitrotoluene
Concen: 9.050 ng/ul
RT: 14.169 min Scan# 1867
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:165 Resp: 150001
Ion Ratio Lower Upper
165 100
89 64.4 49.8 74.8
121 24.5 17.2 25.8

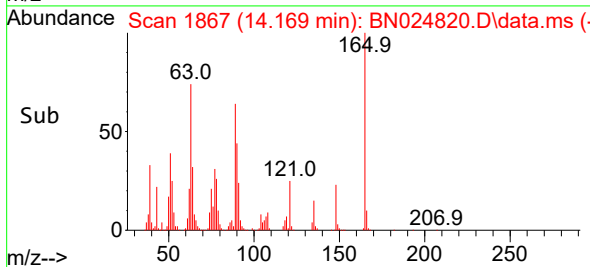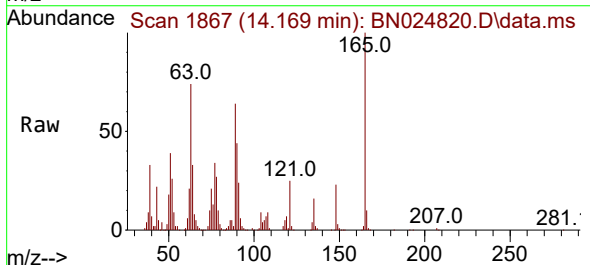



#50

Acenaphthylene

Concen: 9.973 ng/ul

RT: 14.310 min Scan# 1891

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:152 Resp: 1059350

Ion Ratio Lower Upper

152 100

151 19.6 16.2 24.4

153 13.1 10.6 16.0



#51

3-Nitroaniline

Concen: 9.253 ng/ul

RT: 14.498 min Scan# 1923

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55




Tgt Ion:138 Resp: 161159


Ion Ratio Lower Upper

138 100

108 11.8 8.6 12.8

92 121.8 99.5 149.3


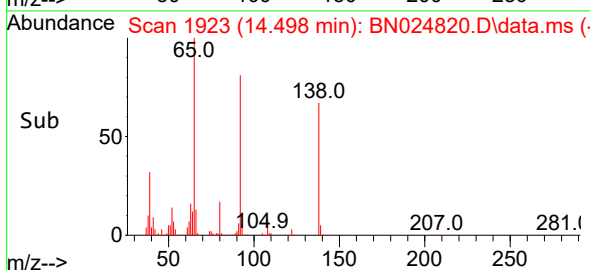




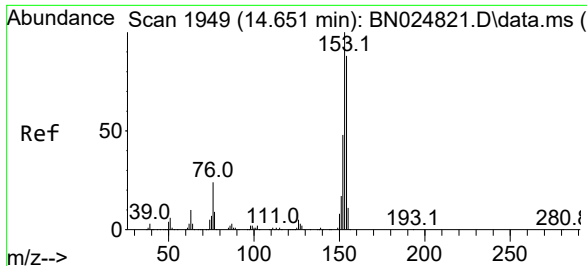

#52
Acenaphthene
Concen: 9.909 ng/ul
RT: 14.651 min Scan# 1949
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:153 Resp: 727656
Ion Ratio Lower Upper
153 100
152 48.6 38.8 58.2
154 86.3 70.3 105.5

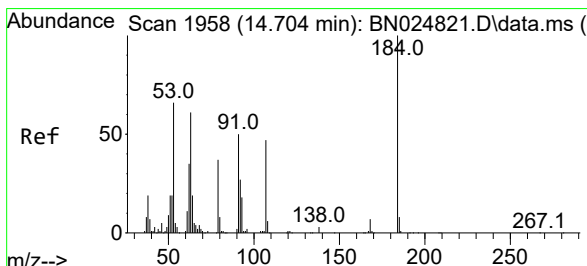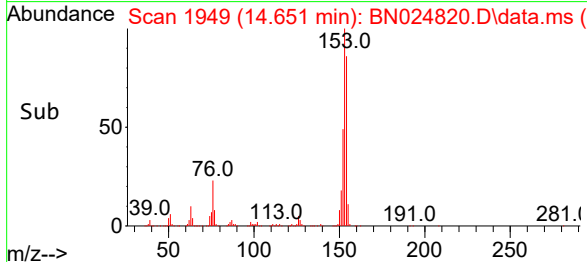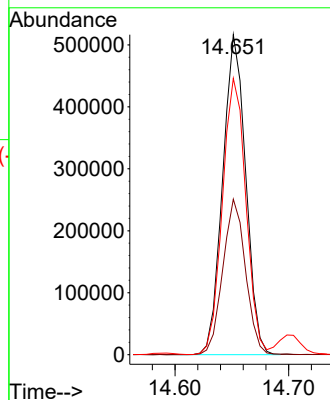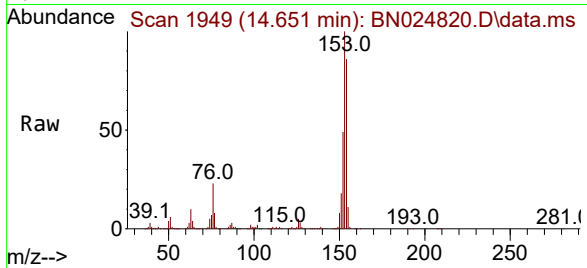

#53
2,4-Dinitrophenol
Concen: 6.820 ng/ul
RT: 14.698 min Scan# 1957
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:184 Resp: 72678
Ion Ratio Lower Upper
184 100
63 93.1 62.6 93.8
154 64.1 50.9 76.3


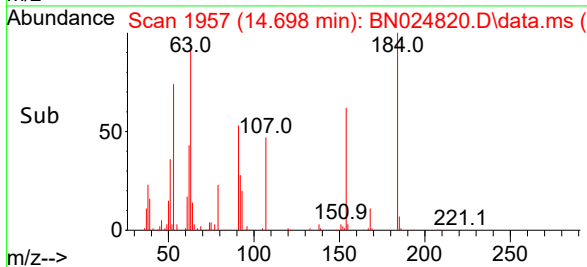
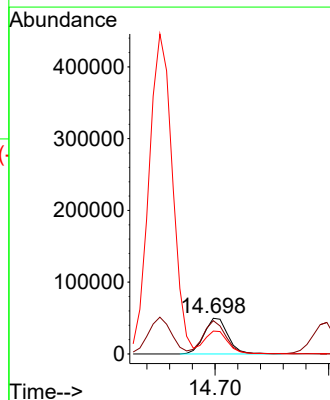
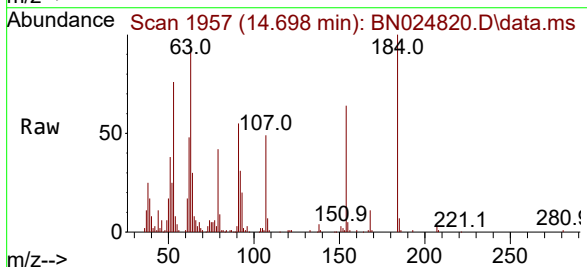




#55
4-Nitrophenol
Concen: 9.083 ng/ul
RT: 14.798 min Scan# 1974
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:109 Resp: 127886
Ion Ratio Lower Upper
109 100
139 129.6 104.3 156.5
65 148.4 124.3 186.5

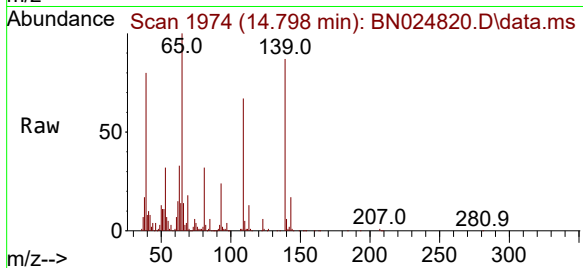

#56
Dibenzofuran
Concen: 9.907 ng/ul
RT: 14.987 min Scan# 2006
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:168 Resp: 1002765
Ion Ratio Lower Upper
168 100
139 38.0 32.1 48.1

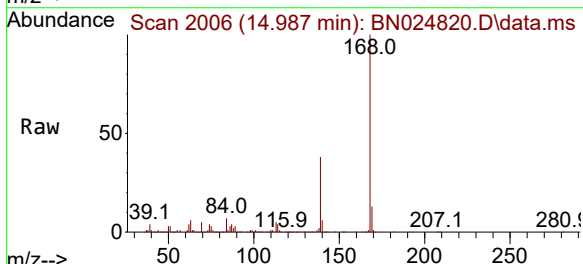



#57

2,4-Dinitrotoluene

Concen: 9.359 ng/ul

RT: 14.951 min Scan# 2000

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:165 Resp: 224534

Ion Ratio Lower Upper

165 100

63 56.0 45.4 68.0

182 2.1 2.2 3.2#

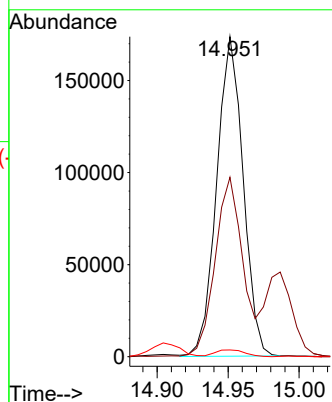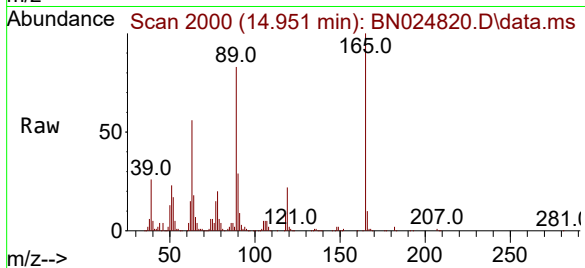

#58

2,3,4,6-Tetrachlorophenol

Concen: 9.921 ng/ul

RT: 15.210 min Scan# 2044

Delta R.T. -0.006 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Tgt Ion:232 Resp: 193965




Ion Ratio Lower Upper


232 100

131 49.5 40.6 61.0

130 2.7 2.2 3.2

166 34.0 27.0 40.4




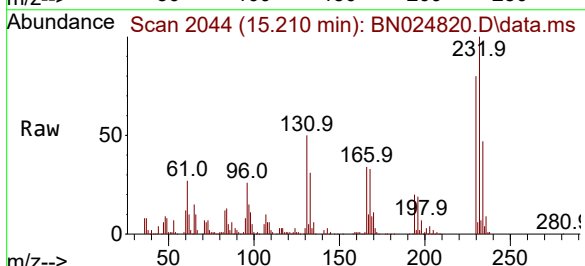




#59
Diethylphthalate
Concen: 9.792 ng/ul
RT: 15.404 min Scan# 2077
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:149 Resp: 835465
Ion Ratio Lower Upper
149 100
177 21.6 16.6 24.8
150 12.0 10.1 15.1

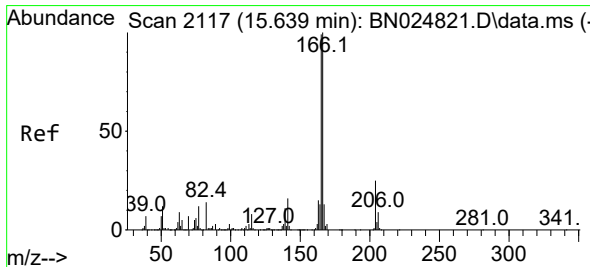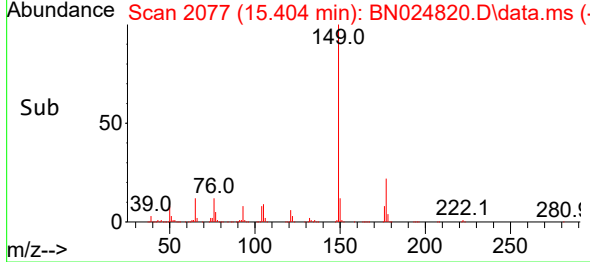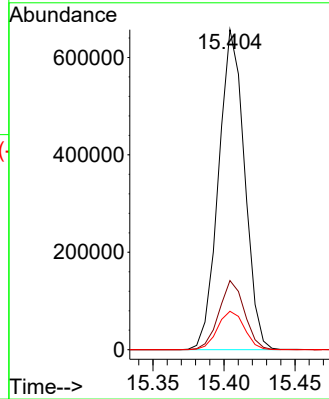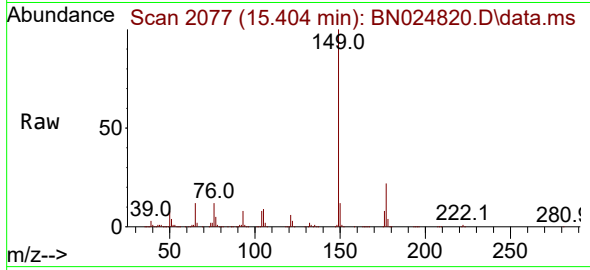

#61
Fluorene
Concen: 10.052 ng/ul
RT: 15.634 min Scan# 2116
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:166 Resp: 818365
Ion Ratio Lower Upper
166 100
165 93.9 79.1 118.7
167 13.5 10.8 16.2


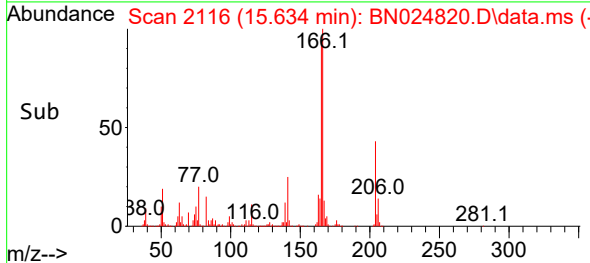
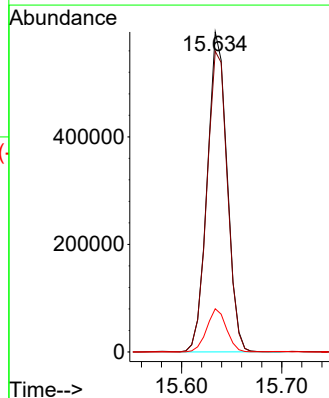
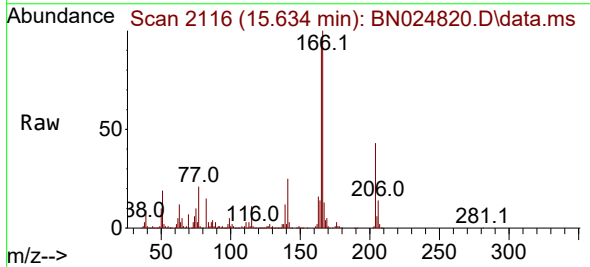




#62
4-Chlorophenyl-phenylether
Concen: 10.169 ng/ul
RT: 15.628 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:204 Resp: 385338
Ion Ratio Lower Upper
204 100
206 32.3 26.0 39.0
141 60.5 51.8 77.8

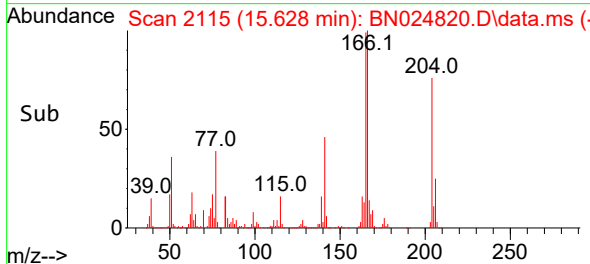

#63
4-Nitroaniline
Concen: 9.295 ng/ul
RT: 15.657 min Scan# 2120
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:138 Resp: 157072
Ion Ratio Lower Upper
138 100
92 57.3 43.3 64.9
108 80.4 64.2 96.4


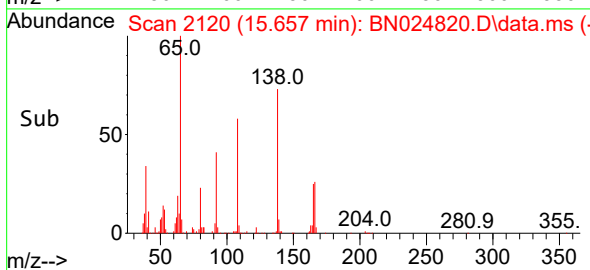

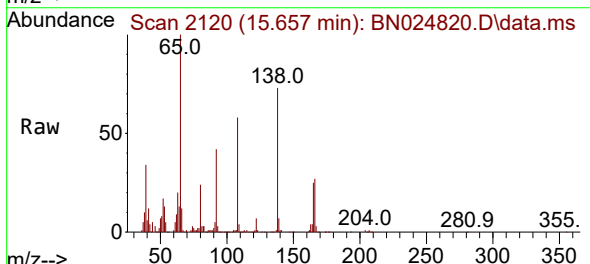




#66
4,6-Dinitro-2-methylphenol
Concen: 8.552 ng/ul
RT: 15.716 min Scan# 2130
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:198 Resp: 124163
Ion Ratio Lower Upper
198 100
182 5.5 3.4 5.0#
77 26.8 23.7 35.5

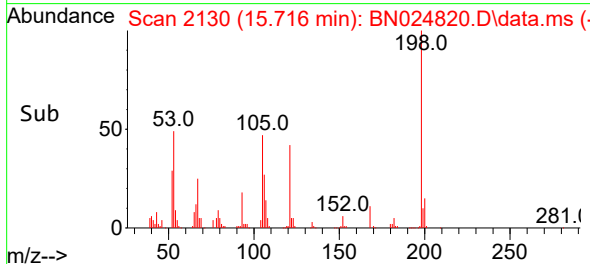

#67
N-Nitrosodiphenylamine
Concen: 10.066 ng/ul
RT: 15.845 min Scan# 2152
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:169 Resp: 695464
Ion Ratio Lower Upper
169 100
168 64.7 54.3 81.5
167 36.6 27.6 41.4


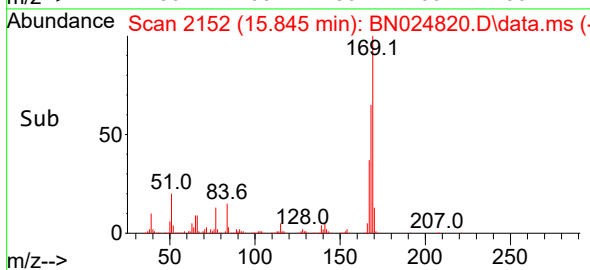

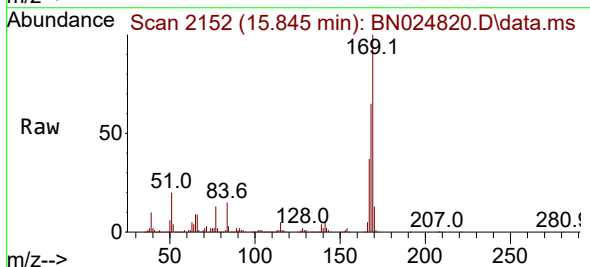




#68
4-Bromophenyl-phenylether
Concen: 10.024 ng/ul
RT: 16.522 min Scan# 211
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:248 Resp: 229464
Ion Ratio Lower Upper
248 100
250 101.4 77.1 115.7
141 84.3 62.3 93.5

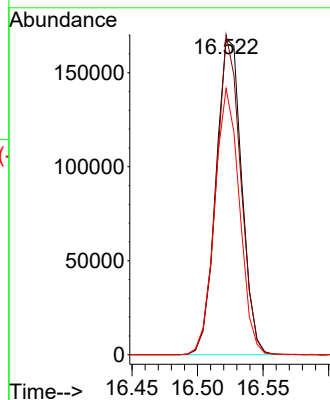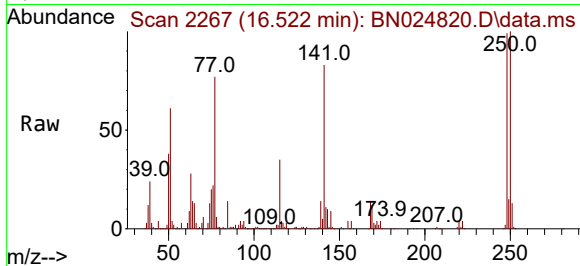

#69
Hexachlorobenzene
Concen: 9.957 ng/ul
RT: 16.639 min Scan# 2287
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:284 Resp: 258070
Ion Ratio Lower Upper
284 100
142 42.1 31.0 46.6
249 31.7 25.1 37.7

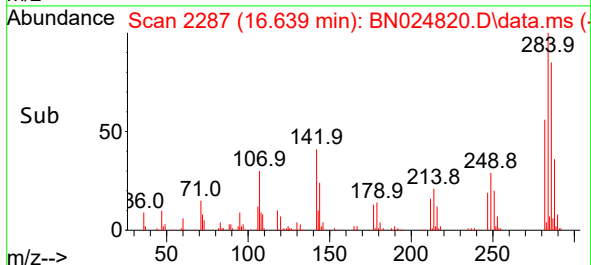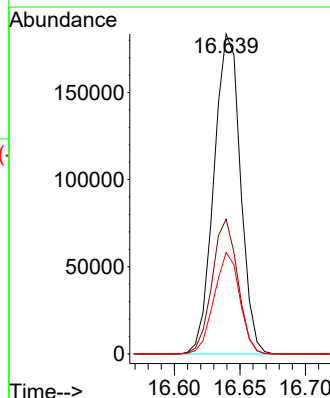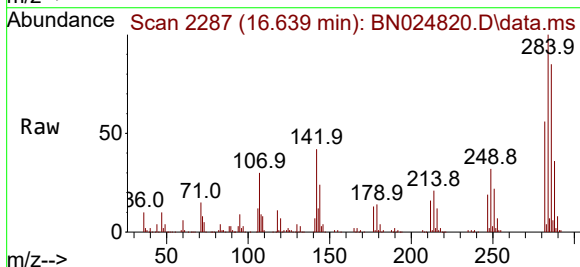



#70

Atrazine

Concen: 9.468 ng/ul

RT: 16.792 min Scan# 21

Delta R.T. -0.006 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:200 Resp: 222589

Ion Ratio Lower Upper

200 100

173 27.8 21.4 32.2

215 46.1 38.2 57.2

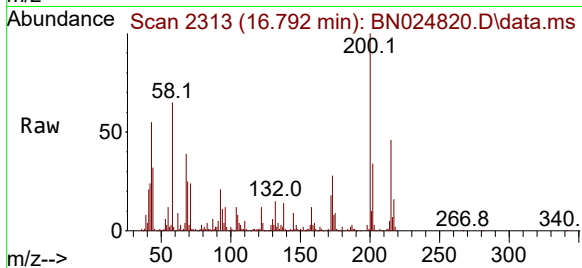

#71

Pentachlorophenol

Concen: 9.139 ng/ul

RT: 16.987 min Scan# 2346

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55




Tgt Ion:266 Resp: 147228


Ion Ratio Lower Upper

266 100

264 56.9 52.7 79.1

268 58.7 51.4 77.0




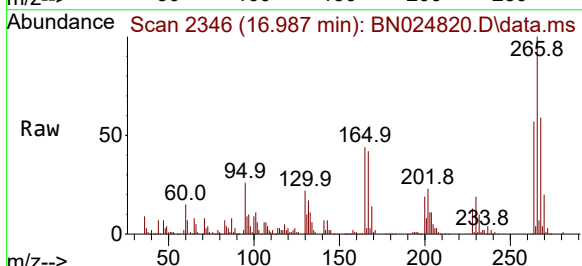




#72
Phenanthrene
Concen: 9.925 ng/ul
RT: 17.381 min Scan# 2413
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:178 Resp: 1275576
Ion Ratio Lower Upper
178 100
179 14.9 12.6 19.0
176 19.3 15.2 22.8

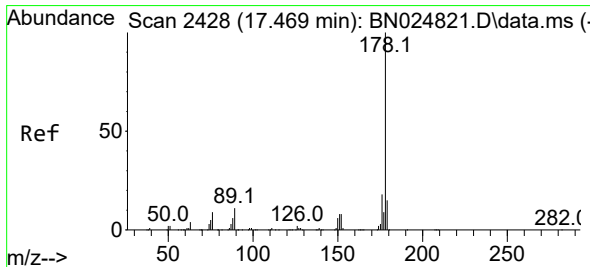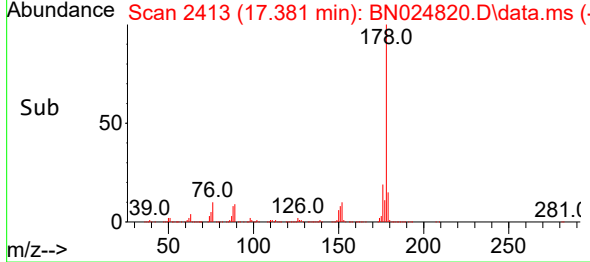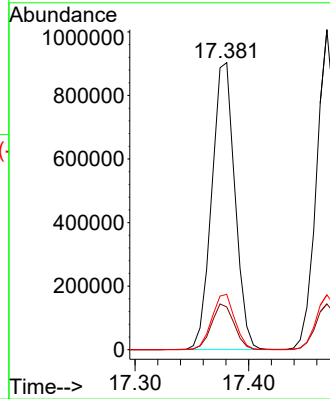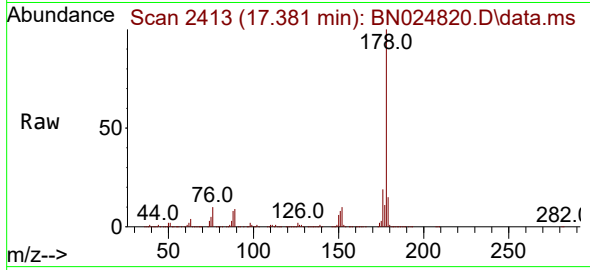

#74
Anthracene
Concen: 10.101 ng/ul
RT: 17.469 min Scan# 2428
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:178 Resp: 1308060
Ion Ratio Lower Upper
178 100
179 14.3 12.2 18.4
176 17.2 14.6 21.8


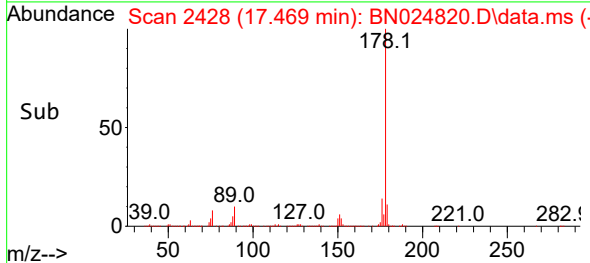
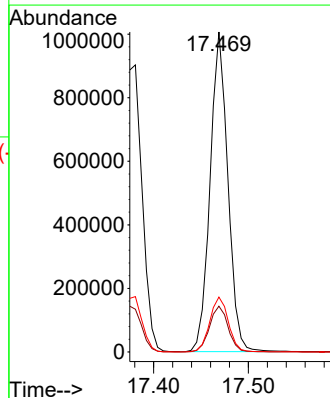
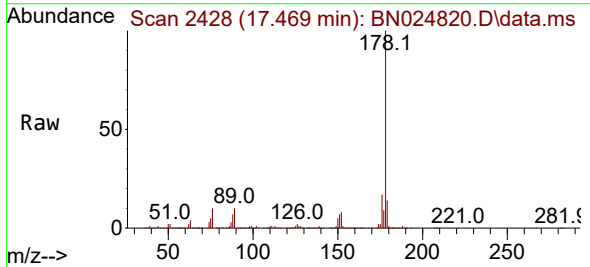


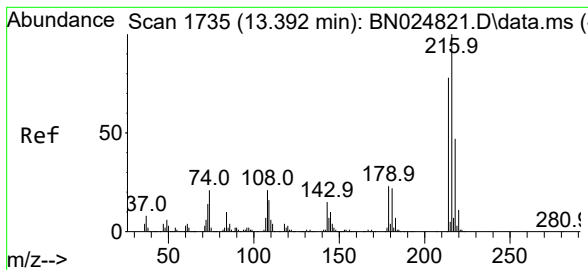

#75
1,2,3,4-Tetrachlorobenzene
Concen: 9.963 ng/uL
RT: 13.393 min Scan# 1735
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:216 Resp: 322728
Ion Ratio Lower Upper
216 100
214 79.1 62.5 93.7
218 48.8 37.7 56.5

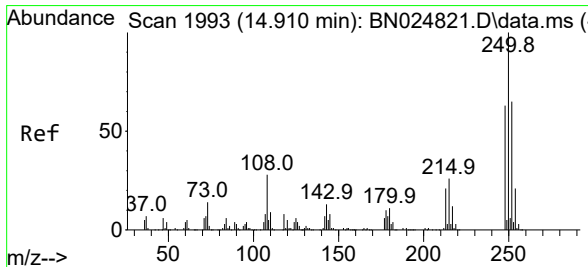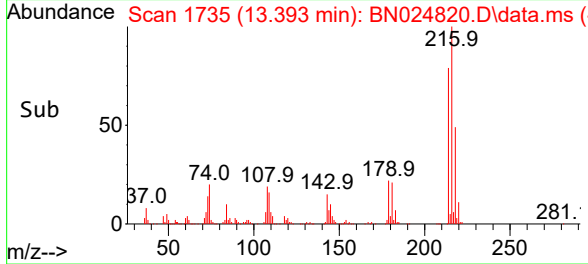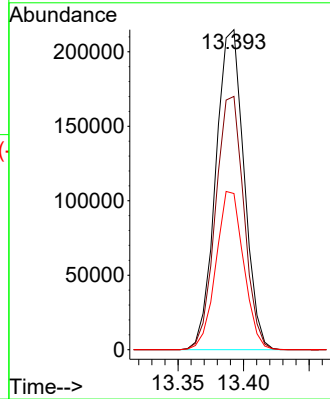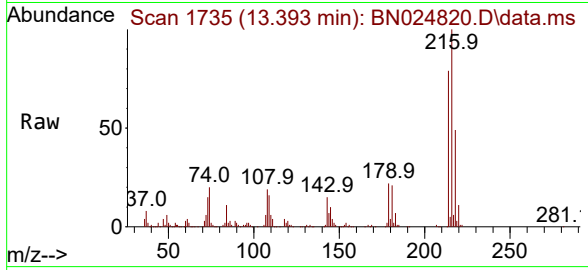

#76
Pentachlorobenzene
Concen: 9.981 ng/uL
RT: 14.904 min Scan# 1992
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:250 Resp: 309314
Ion Ratio Lower Upper
250 100
248 61.4 50.8 76.2
252 61.6 51.8 77.6


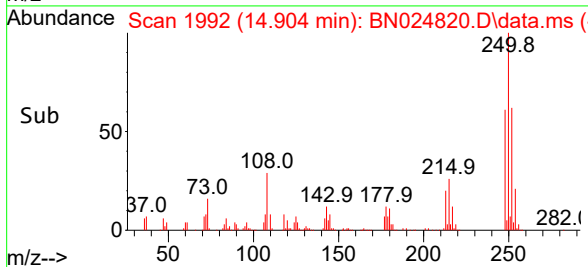
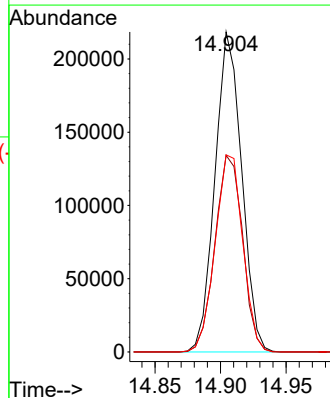
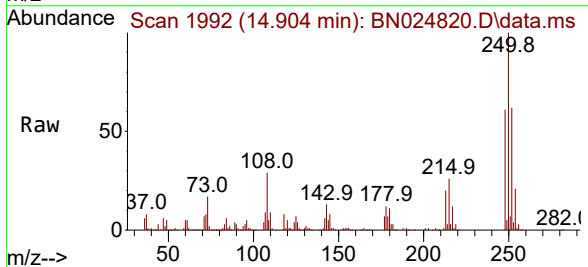




#77
 Carbazole
 Concen: 10.036 ng/ul
 RT: 17.739 min Scan# 2475
 Delta R.T. -0.006 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55




Instrument :
 BNA_N
 ClientSampleId :
 SST010212


Tgt Ion:167 Resp: 1173547
 Ion Ratio Lower Upper
 167 100
 166 20.6 16.6 24.8
 139 12.9 10.2 15.4

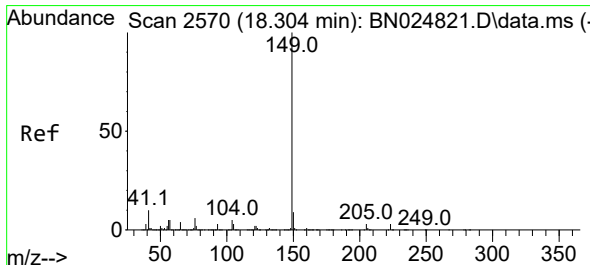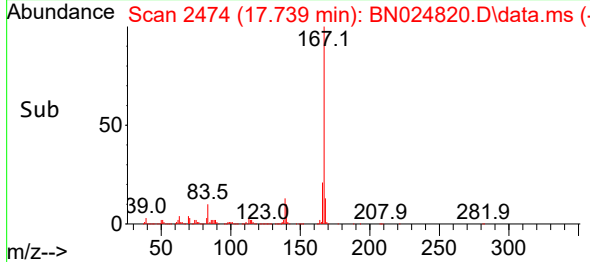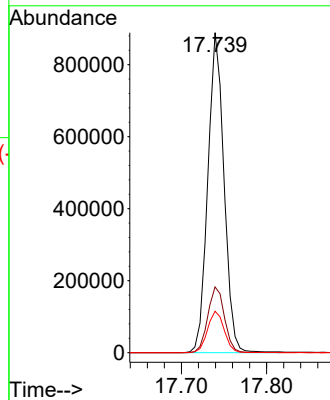

#78
 Di-n-butylphthalate
 Concen: 9.554 ng/ul
 RT: 18.298 min Scan# 2569
 Delta R.T. -0.006 min
 Lab File: BN024820.D
 Acq: 10 Apr 2023 11:55

Tgt Ion:149 Resp: 1326064
 Ion Ratio Lower Upper
 149 100
 150 9.3 7.4 11.2
 104 5.9 4.2 6.4


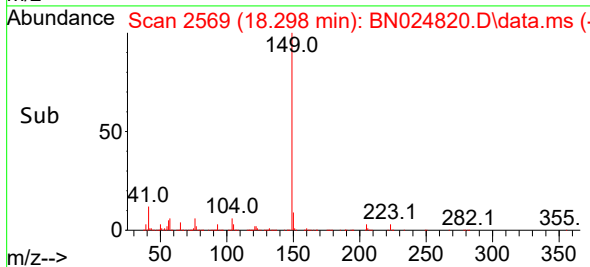
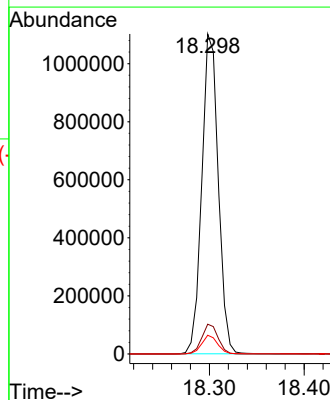
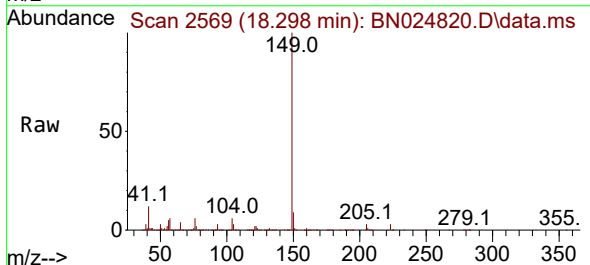




#80
Fluoranthene
Concen: 9.679 ng/ul
RT: 19.392 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:202 Resp: 1431076
Ion Ratio Lower Upper
202 100
101 13.7 10.7 16.1
100 10.6 7.9 11.9

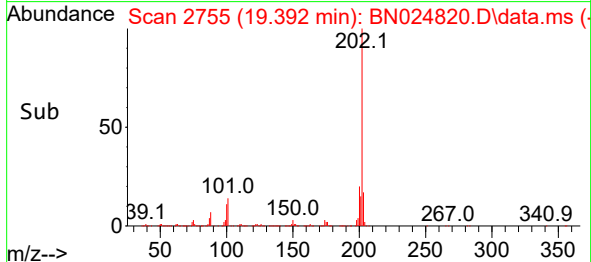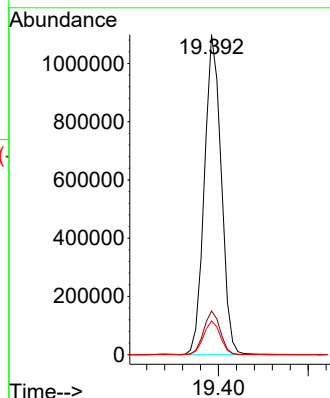

#82
Pyrene
Concen: 10.020 ng/ul
RT: 19.757 min Scan# 2817
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:202 Resp: 1559321
Ion Ratio Lower Upper
202 100
101 15.5 13.0 19.6
100 12.9 11.0 16.6

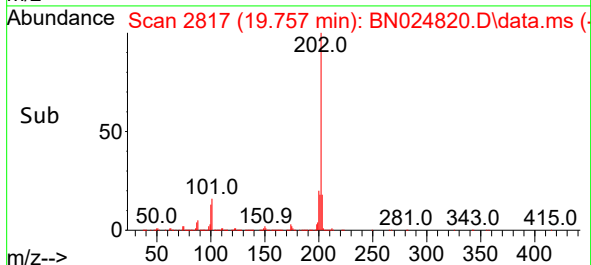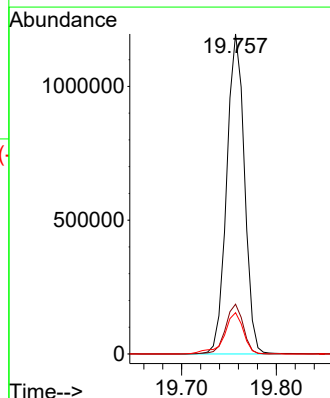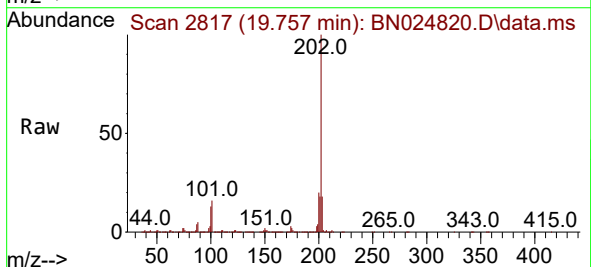



#83

Butylbenzylphthalate

Concen: 9.119 ng/ul

RT: 20.657 min Scan# 2970

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:149 Resp: 589196

Ion Ratio Lower Upper

149 100

91 79.7 62.6 93.8

206 20.3 16.2 24.2

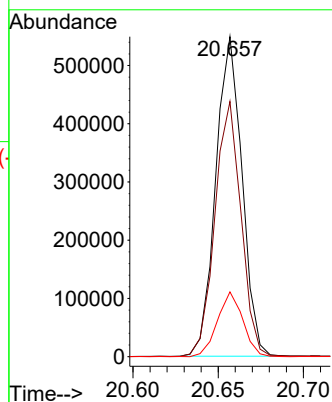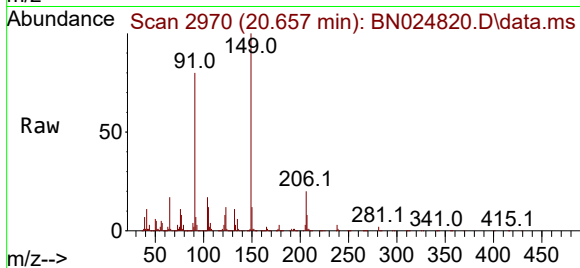

#84

3,3'-Dichlorobenzidine

Concen: 8.937 ng/ul

RT: 21.445 min Scan# 3104

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55




Tgt Ion:252 Resp: 435617


Ion Ratio Lower Upper

252 100

254 64.1 52.2 78.2

126 13.9 11.4 17.2




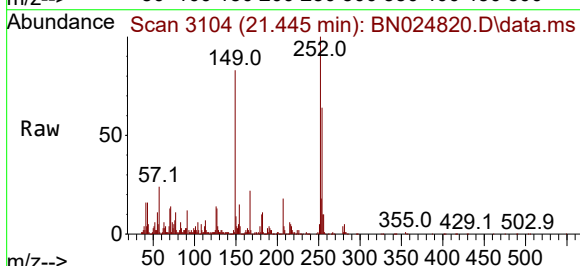




#85
Benzo(a)anthracene
Concen: 9.899 ng/ul
RT: 21.516 min Scan# 3116
Delta R.T. 0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:228 Resp: 1510368
Ion Ratio Lower Upper
228 100
229 20.1 16.2 24.2
226 26.6 20.7 31.1

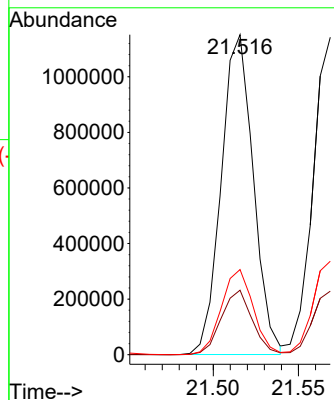

#86
Bis(2-ethylhexyl)phthalate
Concen: 9.386 ng/ul
RT: 21.433 min Scan# 3102
Delta R.T. 0.000 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:149 Resp: 905310
Ion Ratio Lower Upper
149 100
167 26.6 21.8 32.8
279 3.5 2.9 4.3

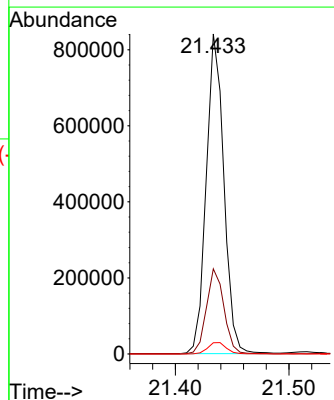



#87

Chrysene

Concen: 9.873 ng/ul

RT: 21.569 min Scan# 3125

Delta R.T. 0.000 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:228 Resp: 1434883

Ion Ratio Lower Upper

228 100

226 29.4 22.4 33.6

229 20.0 15.6 23.4



#89

Di-n-octyl phthalate

Concen: 9.409 ng/ul




RT: 22.374 min Scan# 3262


Delta R.T. -0.006 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Tgt Ion:149 Resp: 1493729









#90
Benzo(b)fluoranthene
Concen: 9.868 ng/ul
RT: 23.227 min Scan# 3410
Delta R.T. -0.006 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55




Instrument :
BNA_N
ClientSampleId :
SSTD010212


Tgt Ion:252 Resp: 1495026
Ion Ratio Lower Upper
252 100
253 20.7 19.2 28.8
125 12.3 10.4 15.6

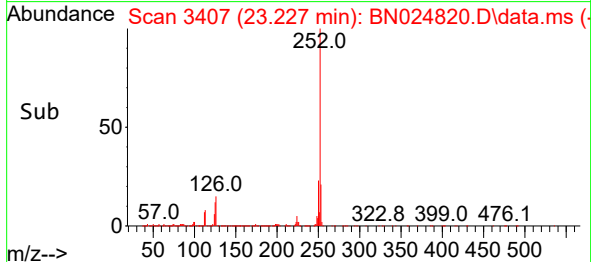

#91
Benzo(k)fluoranthene
Concen: 10.082 ng/ul
RT: 23.274 min Scan# 3415
Delta R.T. -0.012 min
Lab File: BN024820.D
Acq: 10 Apr 2023 11:55

Tgt Ion:252 Resp: 1502941
Ion Ratio Lower Upper
252 100
253 21.4 16.7 25.1
125 12.3 9.3 13.9





#93

Benzo(a)pyrene

Concen: 9.732 ng/ul

RT: 23.863 min Scan# 3

Delta R.T. -0.012 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:252 Resp: 1290801

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.0

125 13.4 10.8 16.2

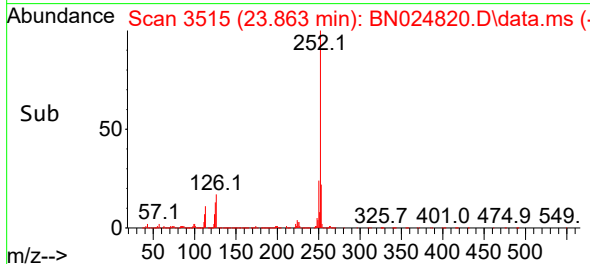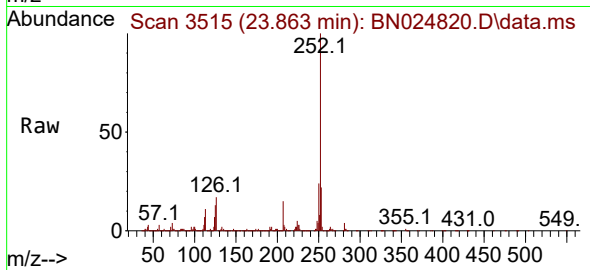

#94

Indeno(1,2,3-cd)pyrene

Concen: 9.566 ng/ul

RT: 26.504 min Scan# 3964

Delta R.T. -0.041 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55




Tgt Ion:276 Resp: 1509721


Ion Ratio Lower Upper

276 100

138 26.4 21.9 32.9

277 24.4 19.8 29.6

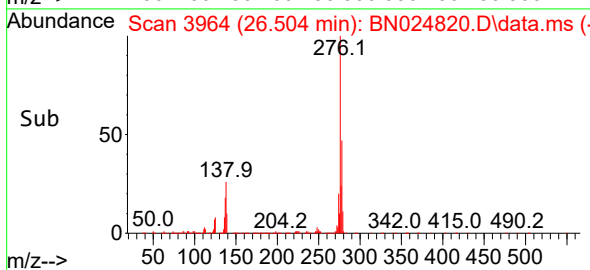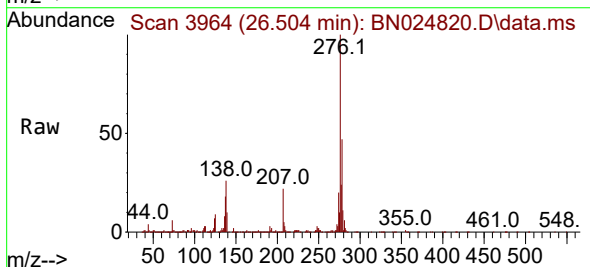



#95

Dibenzo(a,h)anthracene

Concen: 9.726 ng/ul

RT: 26.527 min Scan# 3974

Delta R.T. -0.035 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Instrument :

BNA_N

ClientSampleId :

SSTD010212





Tgt Ion:278 Resp: 1270054

Ion Ratio Lower Upper

278 100

139 17.8 14.6 21.8

279 22.2 18.2 27.4

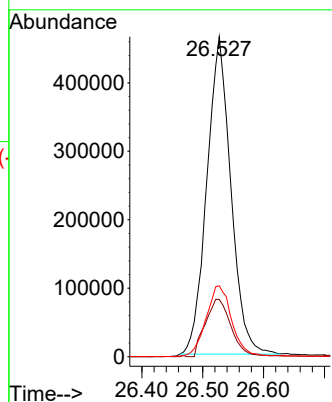

#96

Benzo(g,h,i)perylene

Concen: 9.504 ng/ul

RT: 27.298 min Scan# 4099

Delta R.T. -0.035 min

Lab File: BN024820.D

Acq: 10 Apr 2023 11:55

Tgt Ion:276 Resp: 1210825

Ion Ratio Lower Upper

276 100

138 23.5 19.8 29.8

277 23.1 17.6 26.4

