
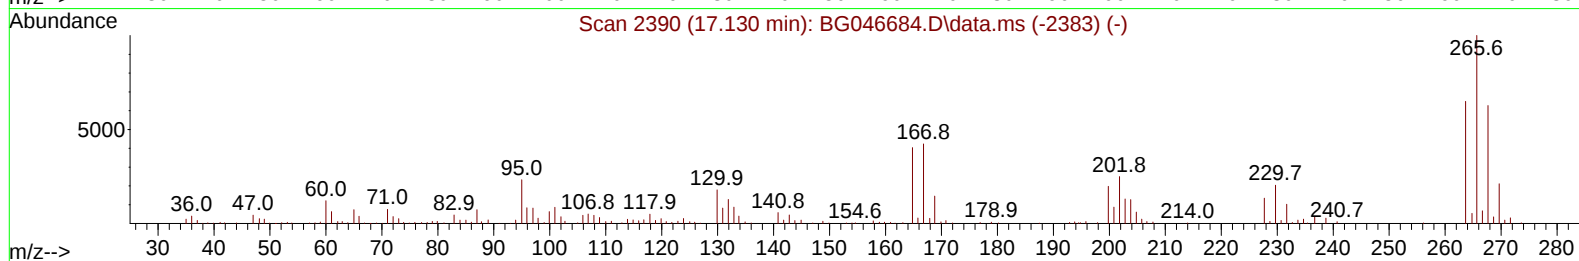
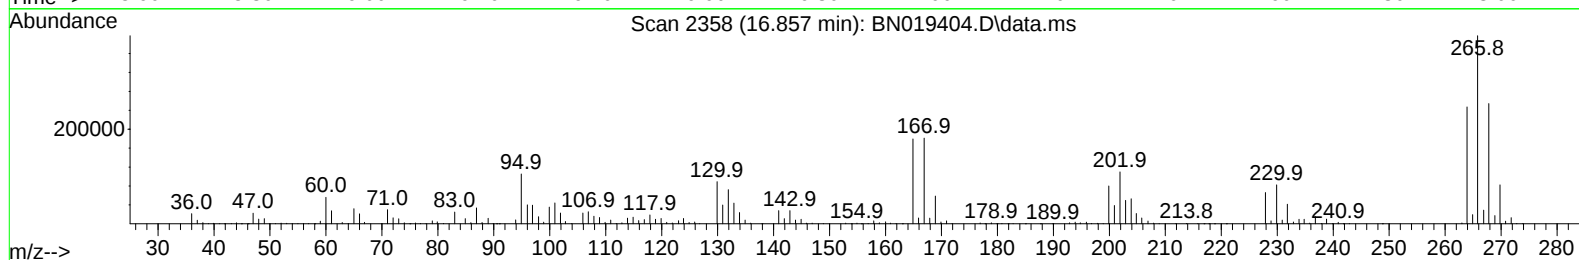


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041122\
Data File : BN019404.D
Acq On : 11 Apr 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:11:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

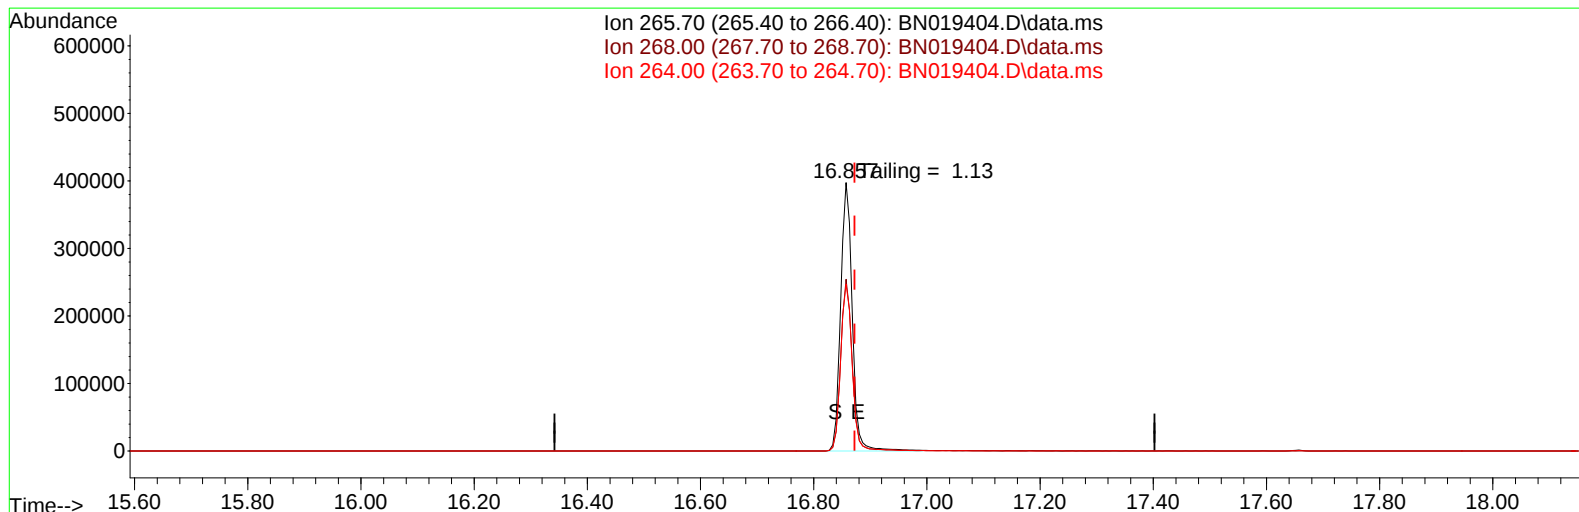

TIC: BN019404.D\data.ms

(70) Pentachlorophenol (C)




16.857min (-0.015) 22670.31 ng

response 568959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.97
264.00	61.60	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041122\
 Data File : BN019404.D
 Acq On : 11 Apr 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 12 08:11:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

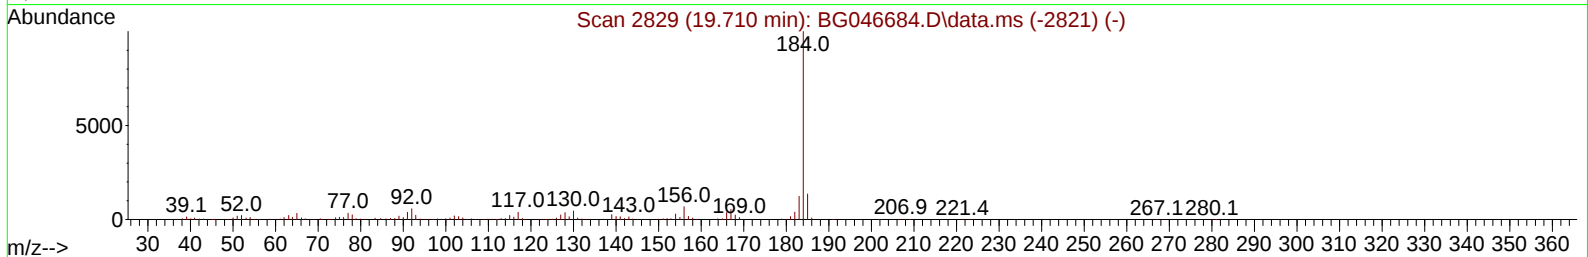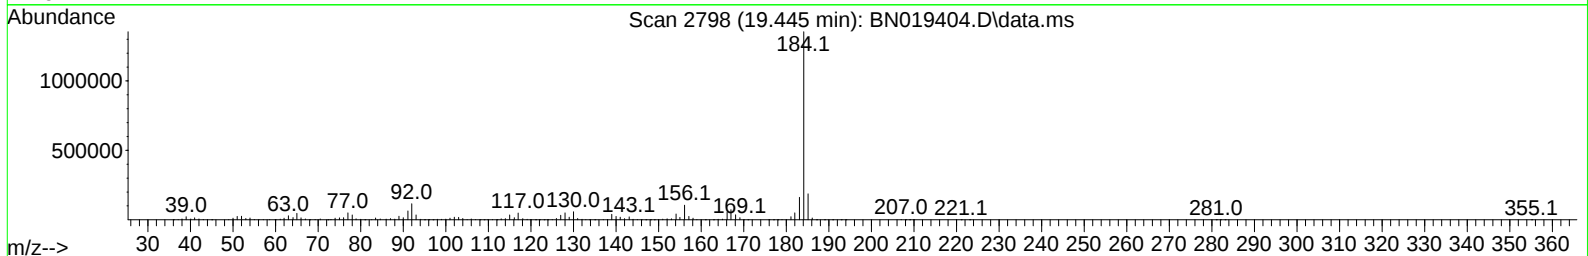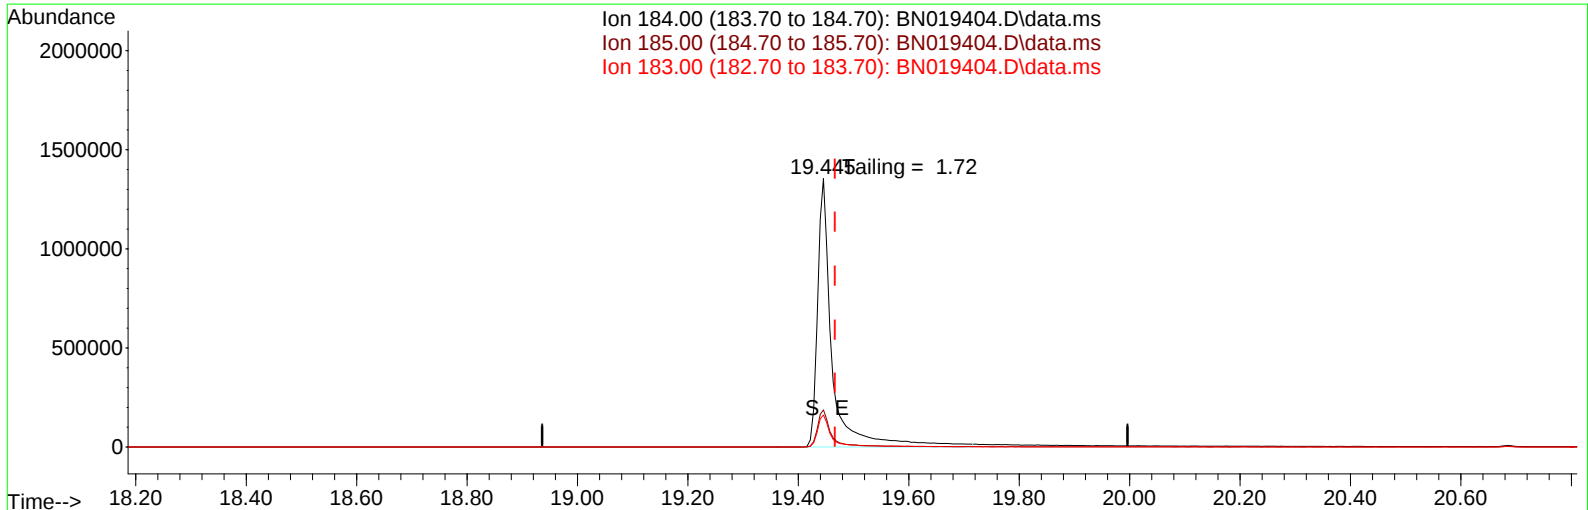

TIC: BN019404.D\data.ms

(77) Benzidine**19.445min (-0.021) 1234818.85 ng****response 2588335**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.95
0.00	0.00	0.00