


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041122\
 Data File : BN019404.D
 Acq On : 11 Apr 2022 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 04 17:40:00 2022

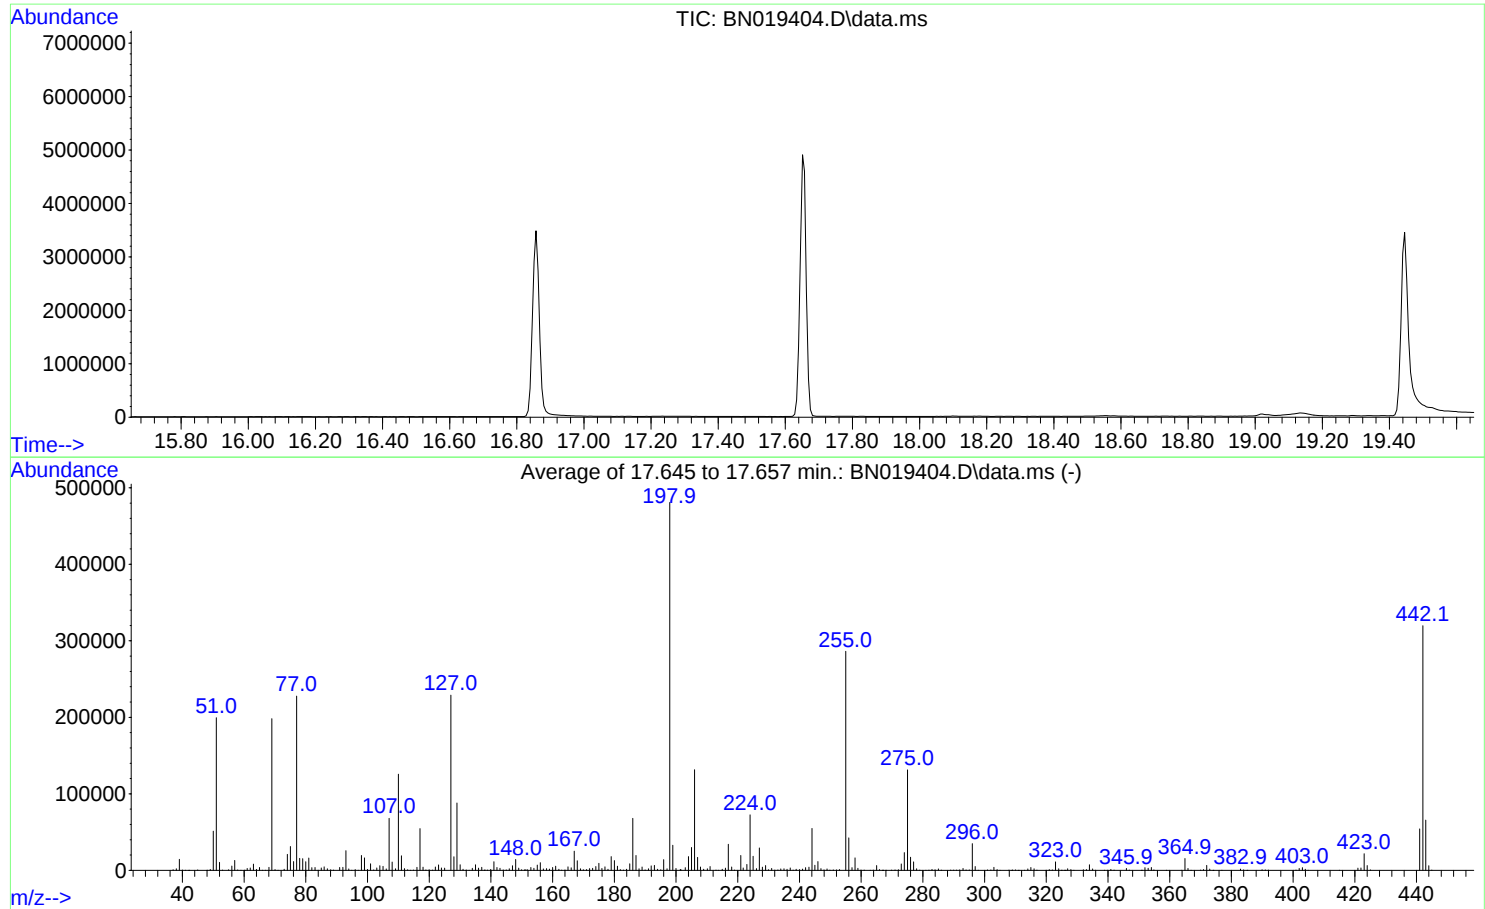




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	199504	PASS
68	69	0.00	2	2.0	3916	PASS
69	198	0.00	100	41.2	198221	PASS
70	69	0.00	2	0.6	1096	PASS
127	198	10	80	47.6	228907	PASS
197	198	0.00	2	0.5	2204	PASS
198	198	100	100	100.0	480747	PASS
199	198	5	9	6.8	32861	PASS
275	198	10	60	27.3	131288	PASS
365	198	1	100	3.2	15431	PASS
441	198	0.01	100	11.3	54149	PASS
442	442	50	100	100.0	319701	PASS
443	442	15	24	20.5	65621	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041122\
Data File : BN019404.D
Acq On : 11 Apr 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 12 08:11:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

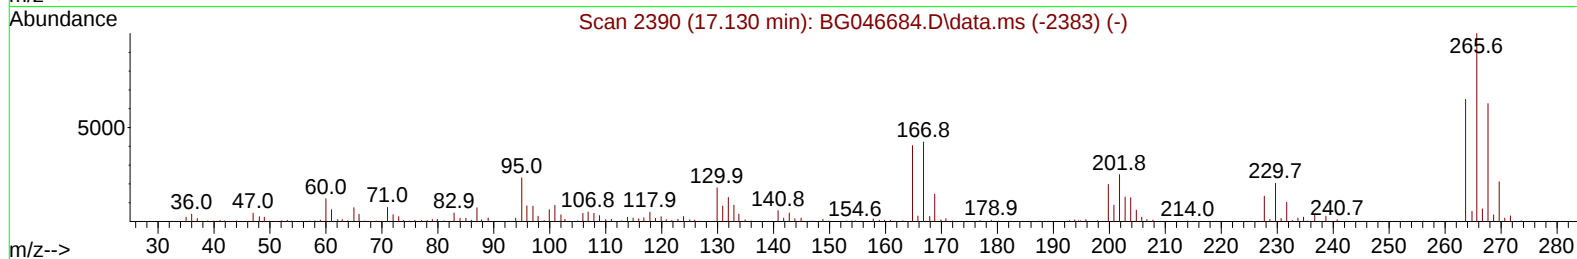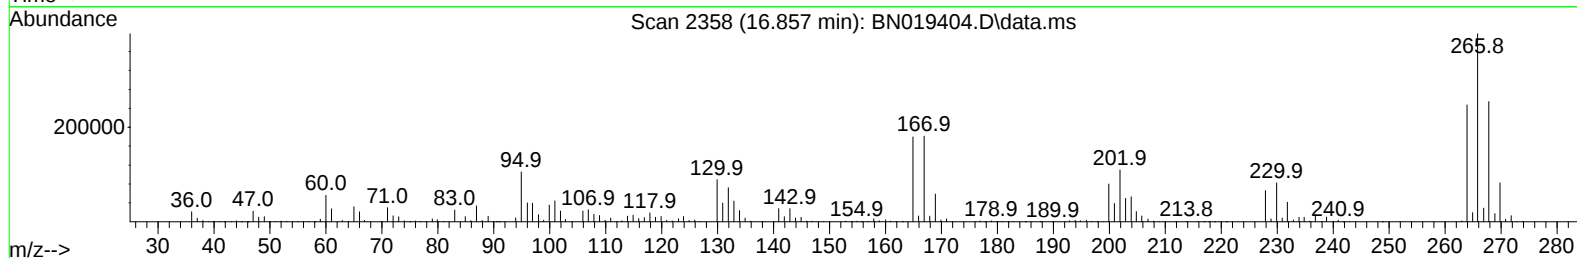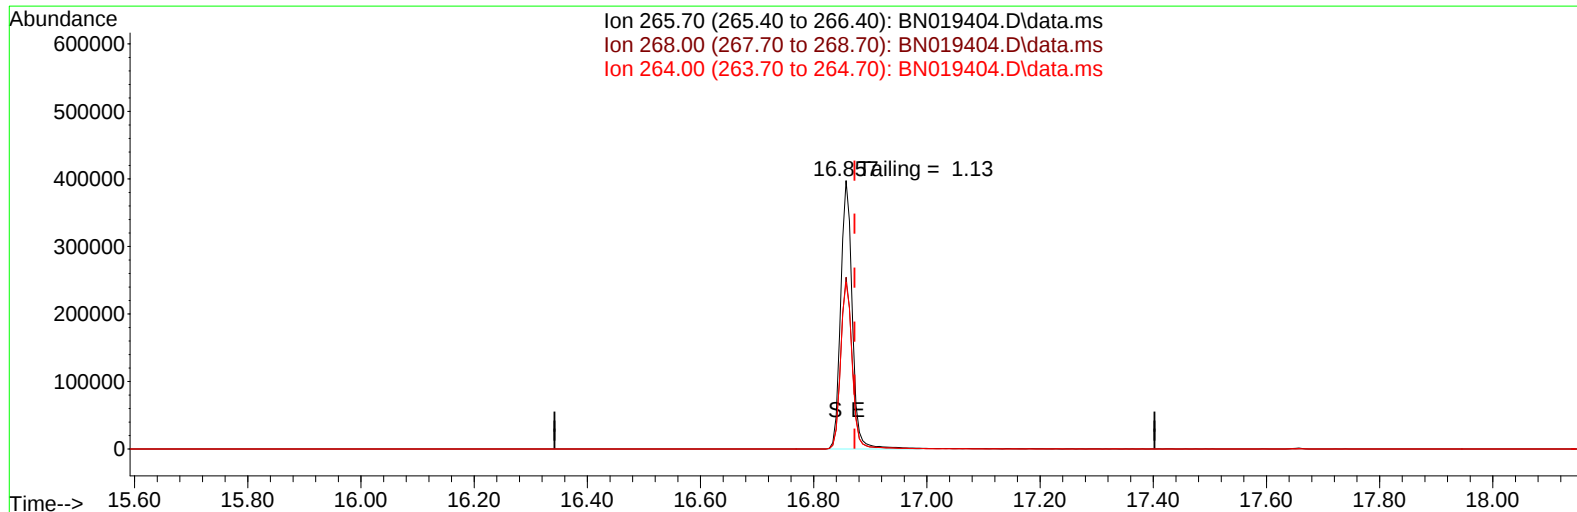

TIC: BN019404.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.015) 22670.31 ng




response 568959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.97
264.00	61.60	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041122\
Data File : BN019404.D
Acq On : 11 Apr 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 12 08:11:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

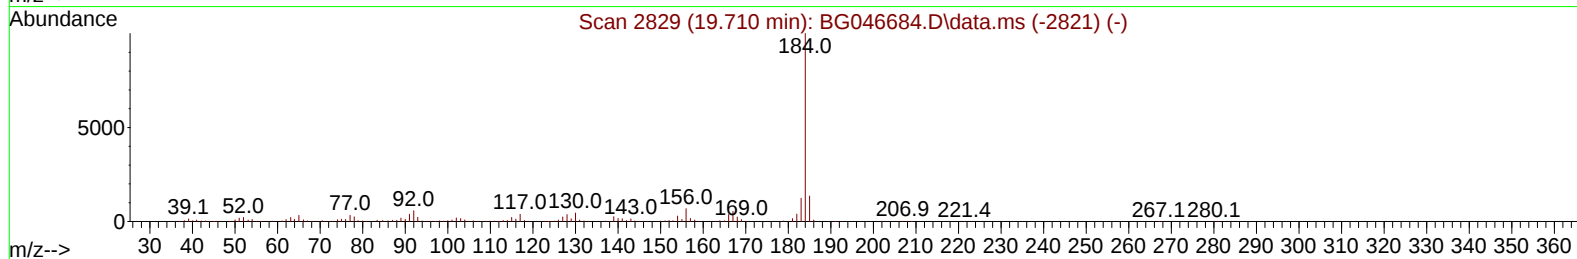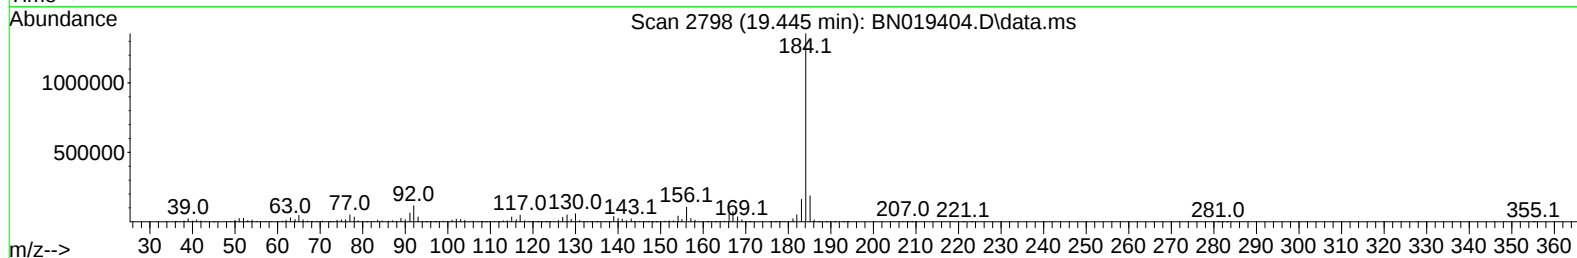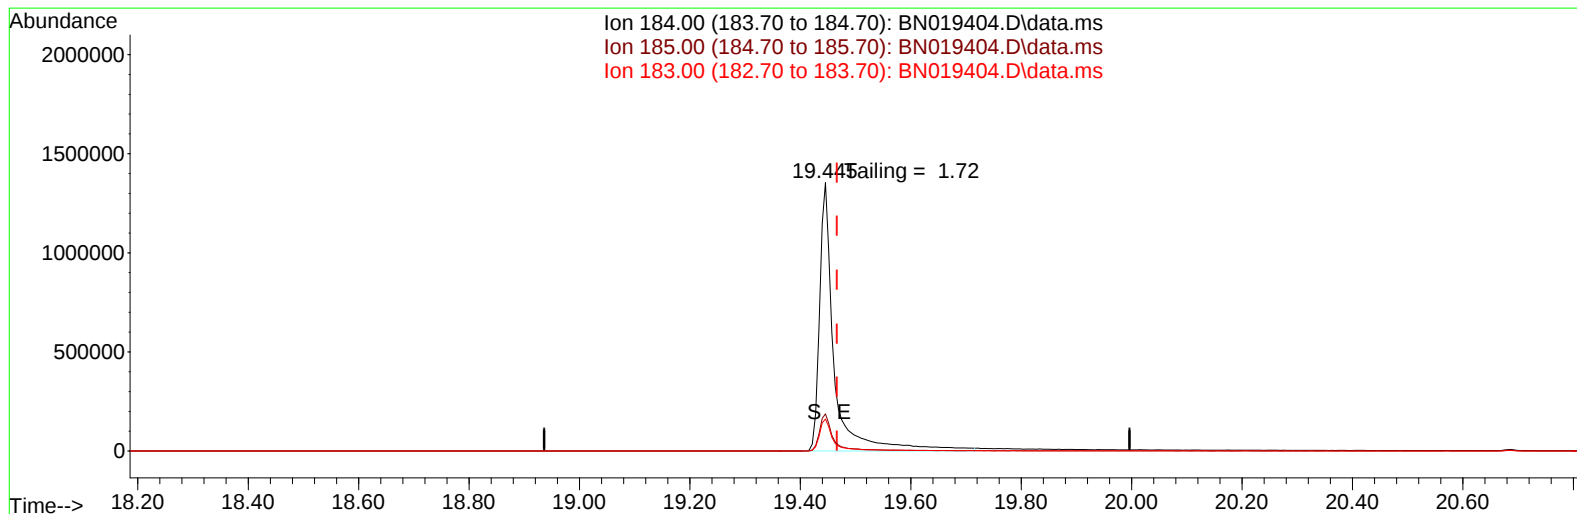

TIC: BN019404.D\data.ms

(77) Benzidine

19.445min (-0.021) 1234818.85 ng

response 2588335

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.82
183.00	13.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/11/2022	BNA_N	<u>BN019404.D</u>
Compound Name	Response	Retention Time
DDT	1630758	20.686
DDD	40691	20.245
DDE	2935	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43626	1674384	2.61

Instrument :
BNA_N
ClientSampleId :
DFTPP