

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041123\
 Data File : BN024828.D
 Acq On : 11 Apr 2023 10:13
 Operator : CG/JU
 Sample : PB152001BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 12 01:09:43 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 08 00:52:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	13215	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	40541	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.589	164	23468	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.338	188	48866	0.400	ng/ul	0.00
17) Chrysene-d12	21.535	240	38714	0.400	ng/ul	0.00
23) Perylene-d12	23.972	264	44824	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.322	96	81892	5.675	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	17974	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	38026	0.395	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.583	166	5957	0.070	ng/ul#	11
20) Pyrene	19.735	202	5425	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.823	252	13230	0.089	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041123\
Data File : BN024828.D
Acq On : 11 Apr 2023 10:13
Operator : CG/JU
Sample : PB152001BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 12 01:09:43 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 00:52:14 2023
Response via : Initial Calibration




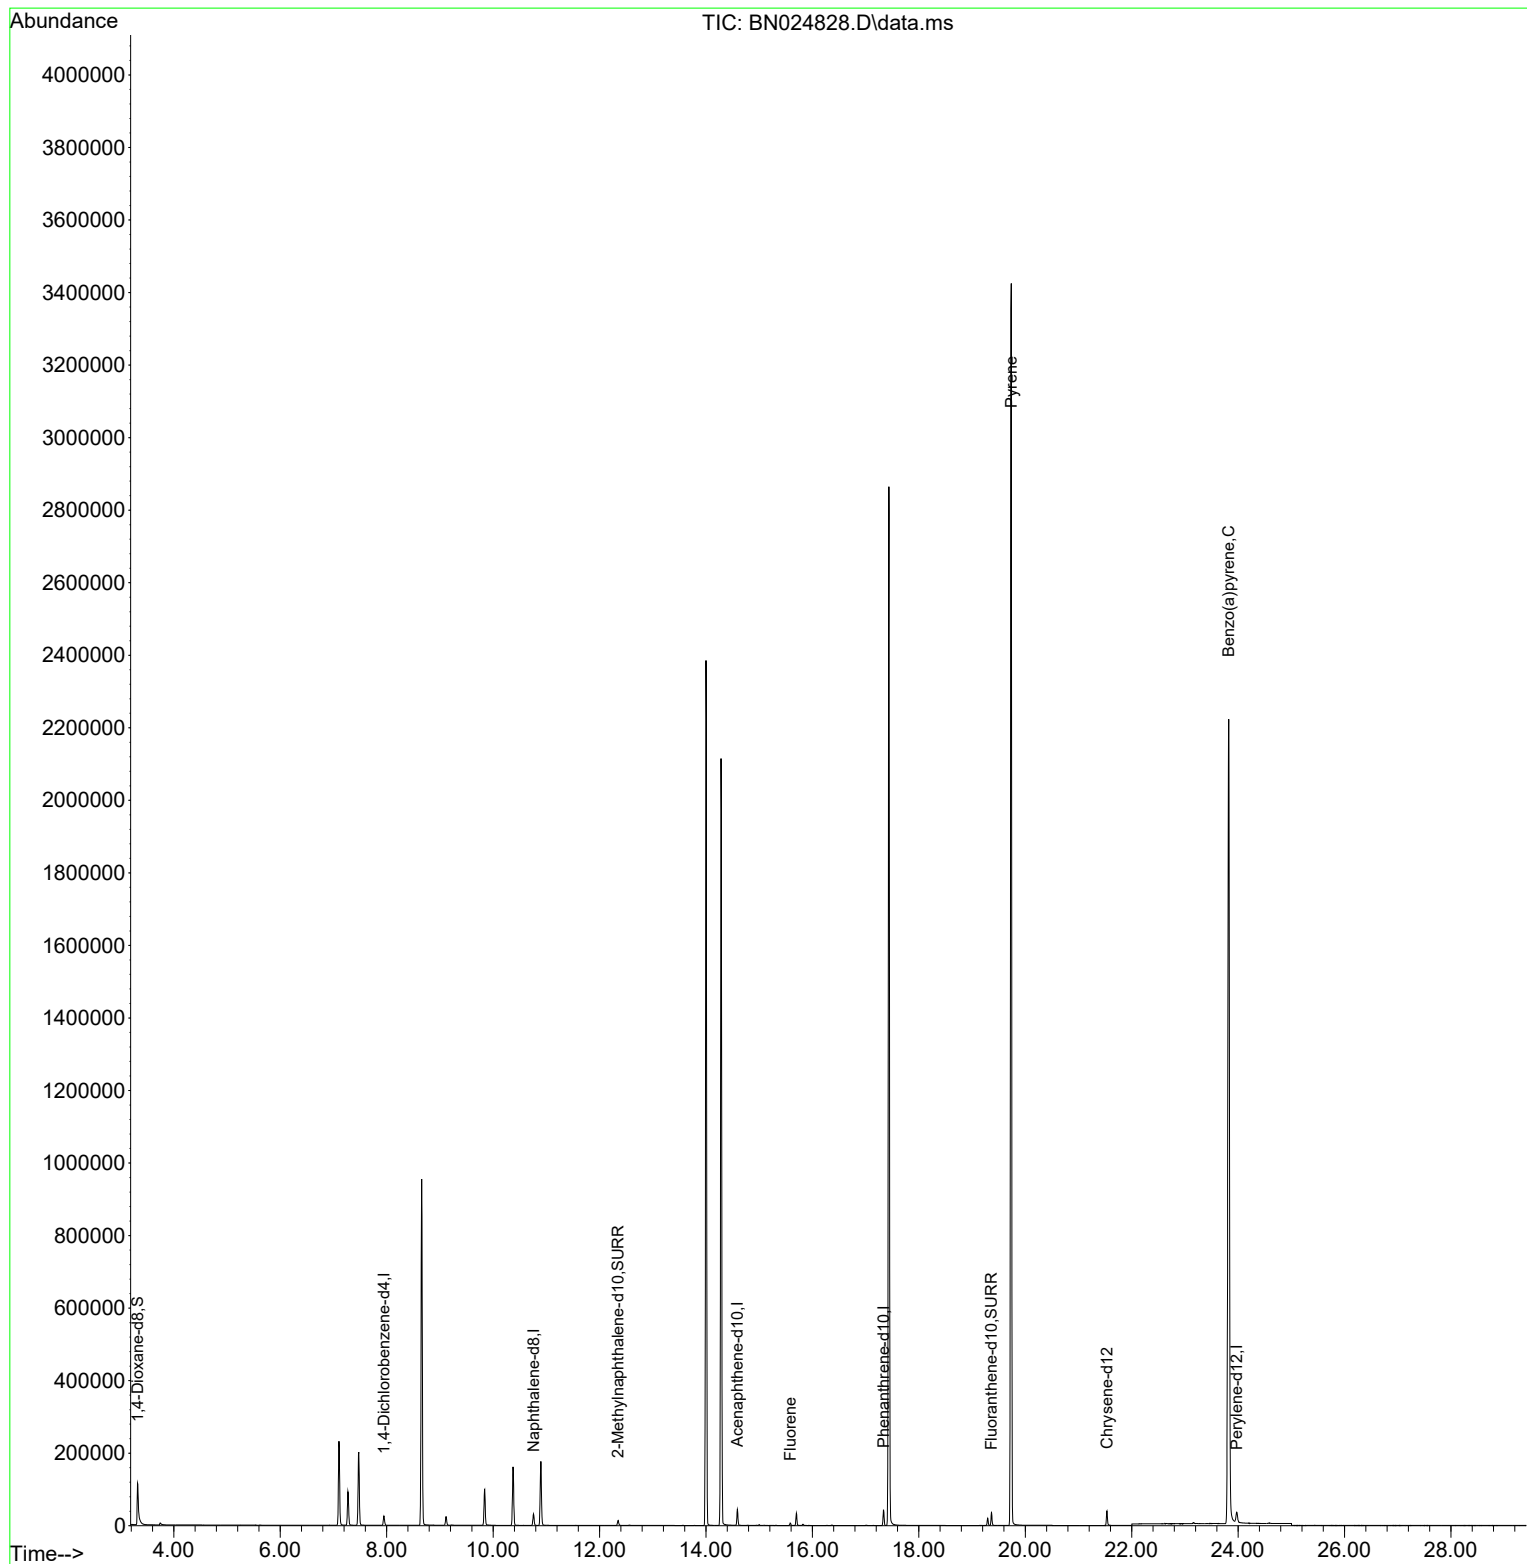


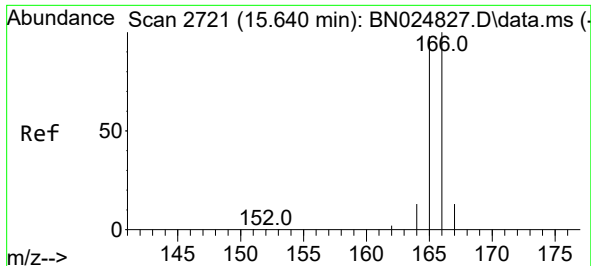

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.583 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN024828.D
Acq: 11 Apr 2023 10:13




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:166 Resp: 5957
Ion Ratio Lower Upper
166 100
165 5.2 80.1 120.1#
167 32.0 10.7 16.1#

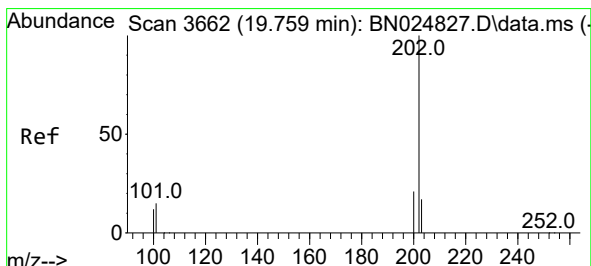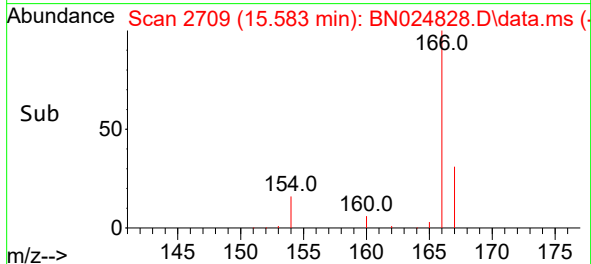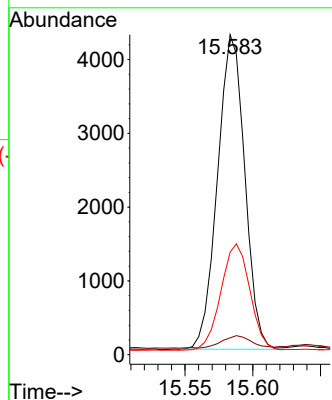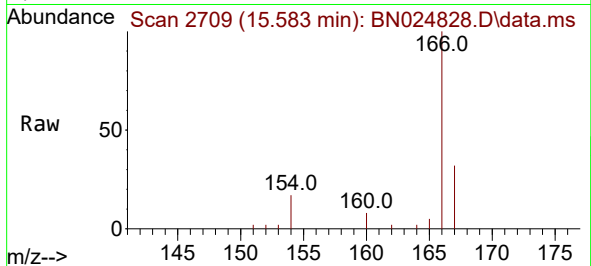

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.735 min Scan# 3657
Delta R.T. -0.024 min
Lab File: BN024828.D
Acq: 11 Apr 2023 10:13


Tgt Ion:202 Resp: 5425
Ion Ratio Lower Upper
202 100
101 174.1 11.8 17.8#
100 1246.6 9.5 14.3#

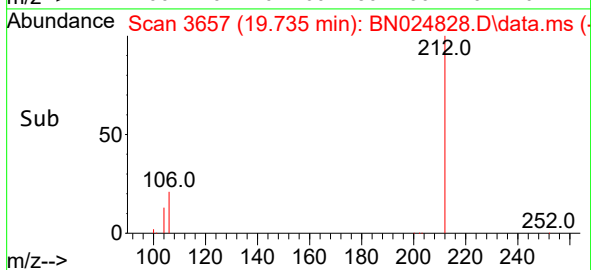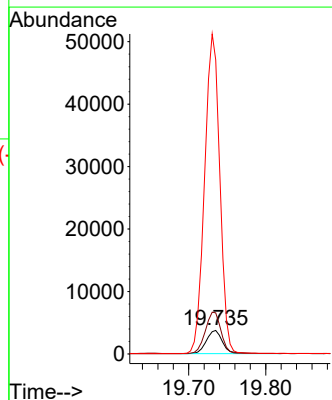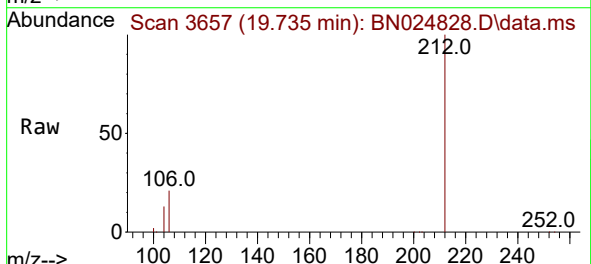

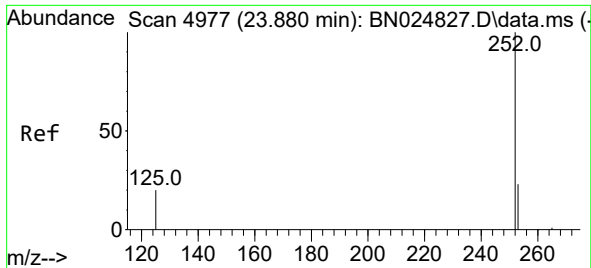

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.823 min Scan# 4958
Delta R.T. -0.045 min
Lab File: BN024828.D
Acq: 11 Apr 2023 10:13

Instrument :
BNA_N
ClientSampleId :

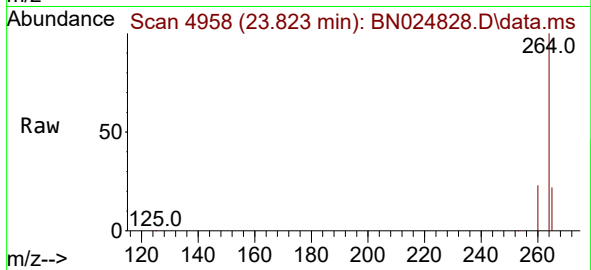

Tgt Ion:252 Resp: 13230
Ion Ratio Lower Upper
252 100
253 40.8 20.7 31.1#
125 35.8 15.9 23.9#

