

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041123\
 Data File : BN024831.D
 Acq On : 11 Apr 2023 12:03
 Operator : CG/JU
 Sample : 02250-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHD3

Quant Time: Apr 12 01:10:04 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 08 00:52:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7220	0.400	ng/u1	0.00
4) Naphthalene-d8	10.759	136	23267	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.594	164	12695	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.339	188	28737	0.400	ng/u1	0.00
17) Chrysene-d12	21.533	240	22662	0.400	ng/u1	0.00
23) Perylene-d12	23.988	264	23711	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	36127	4.582	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	9755	0.327	ng/u1	0.00
18) Fluoranthene-d10	19.369	212	28772	0.511	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.352	88	3676	0.423	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041123\
Data File : BN024831.D
Acq On : 11 Apr 2023 12:03
Operator : CG/JU
Sample : 02250-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHD3


Quant Time: Apr 12 01:10:04 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 00:52:14 2023
Response via : Initial Calibration

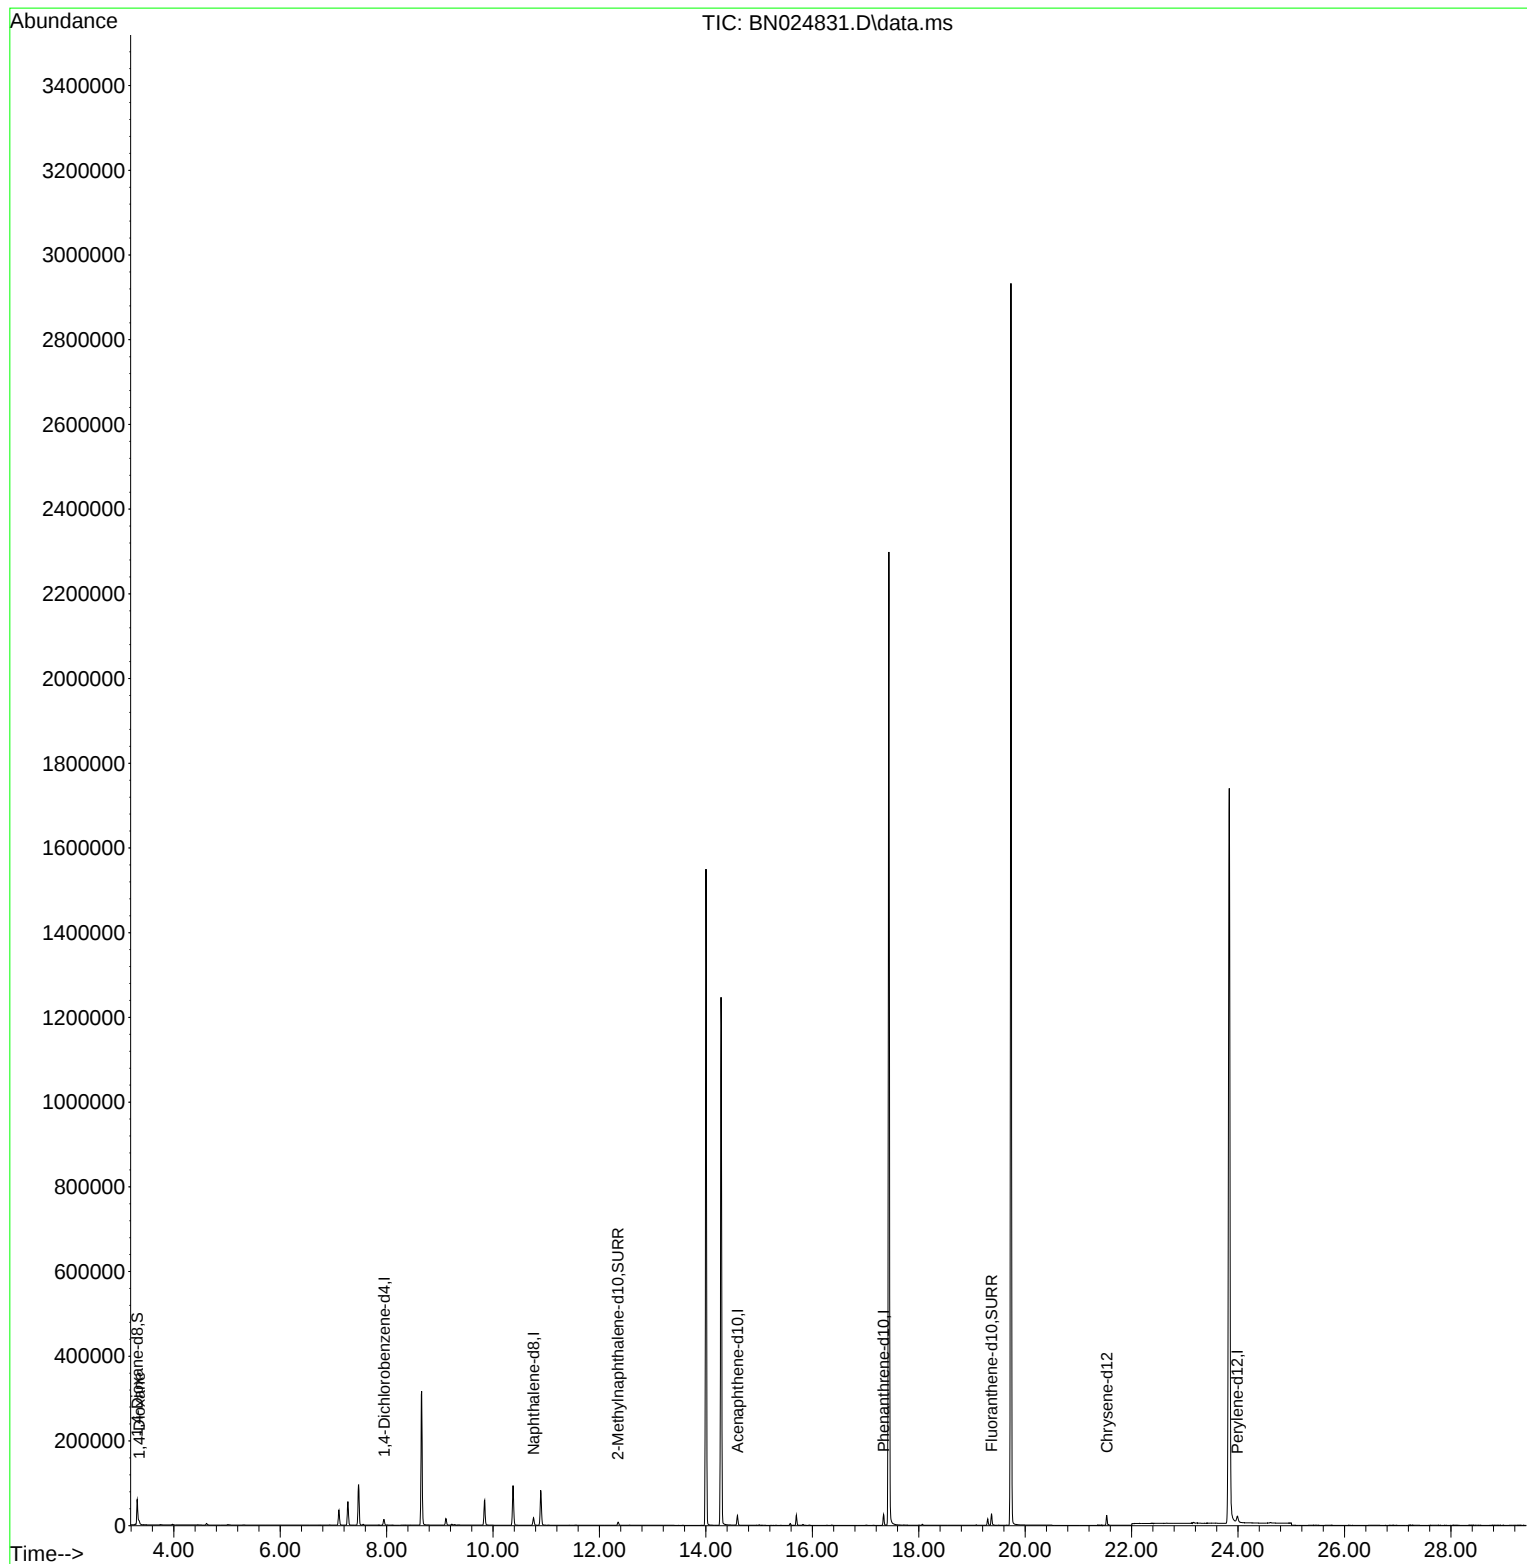

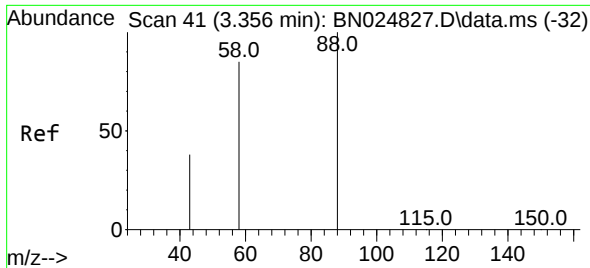

#2
 1,4-Dioxane
 Concen: 0.423 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. -0.000 min
 Lab File: BN024831.D
 Acq: 11 Apr 2023 12:03

Instrument :
 BNA_N
 ClientSampleId :
 BHD3

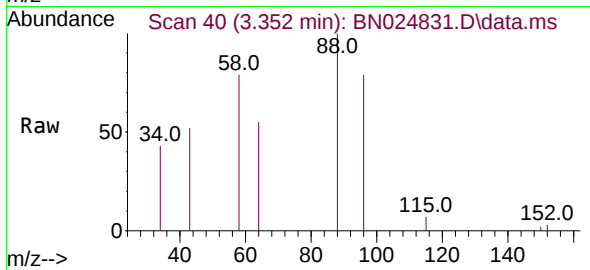

Tgt Ion: 88	Resp: 3676
Ion Ratio	Lower Upper
88 100	
43 51.9	39.1 58.7
58 79.0	65.7 98.5

