

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041123\
 Data File : BN024834.D
 Acq On : 11 Apr 2023 14:06
 Operator : CG/JU
 Sample : 02194-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDx2

Quant Time: Apr 12 01:10:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 08 00:52:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	6336	0.400	ng/u1	0.00
4) Naphthalene-d8	10.759	136	19467	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.593	164	11741	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.338	188	26847	0.400	ng/u1	0.00
17) Chrysene-d12	21.535	240	22956	0.400	ng/u1	0.00
23) Perylene-d12	23.978	264	24761	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	40966	5.921	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	8780	0.351	ng/u1	0.00
18) Fluoranthene-d10	19.368	212	25118	0.441	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.348	88	2718	0.357	ng/u1#	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041123\
Data File : BN024834.D
Acq On : 11 Apr 2023 14:06
Operator : CG/JU
Sample : 02194-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDx2


Quant Time: Apr 12 01:10:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 08 00:52:14 2023
Response via : Initial Calibration

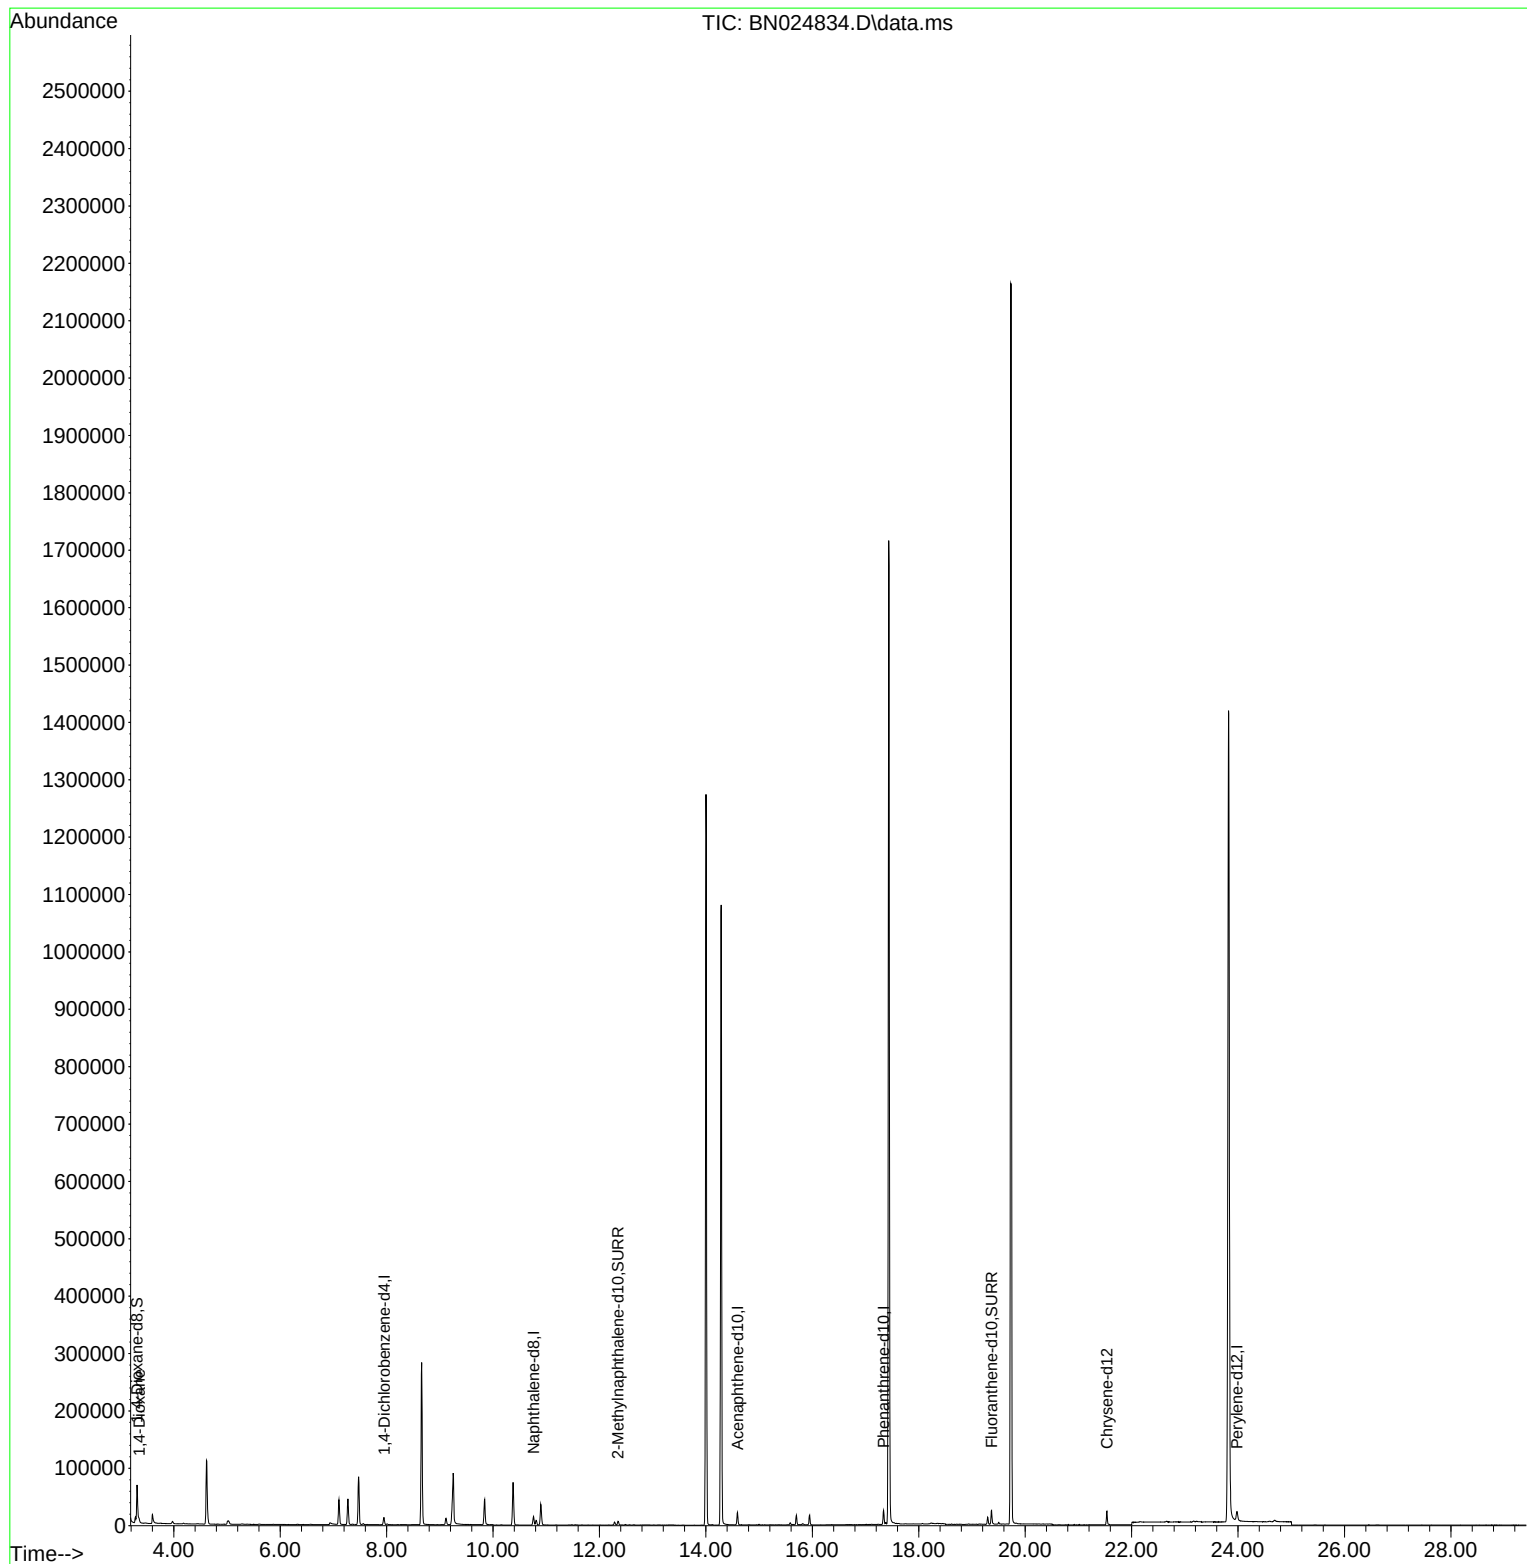

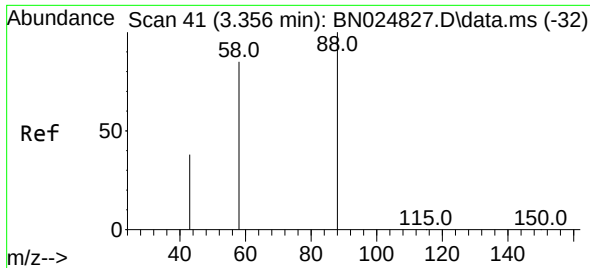

#2
 1,4-Dioxane
 Concen: 0.357 ng/ul
 RT: 3.348 min Scan# 39
 Delta R.T. -0.004 min
 Lab File: BN024834.D
 Acq: 11 Apr 2023 14:06

Instrument :
 BNA_N
 ClientSampleId :
 BHDx2

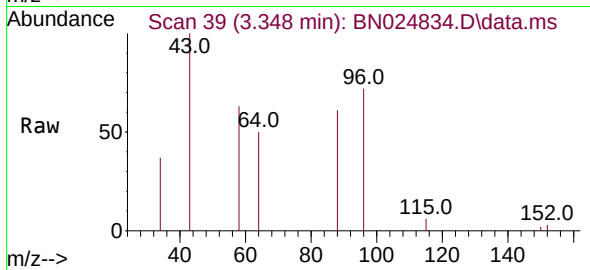

Tgt Ion:	88	Resp:	2718
Ion	Ratio	Lower	Upper
88	100		
43	163.9	39.1	58.7#
58	103.6	65.7	98.5#

