
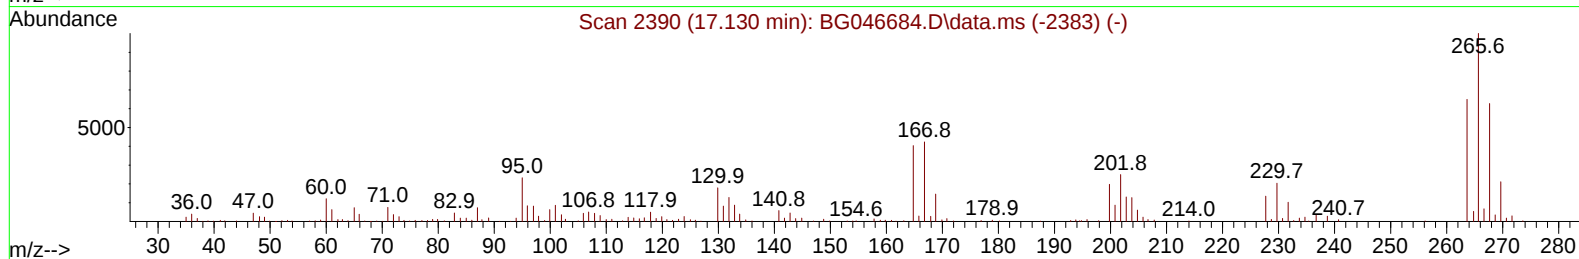
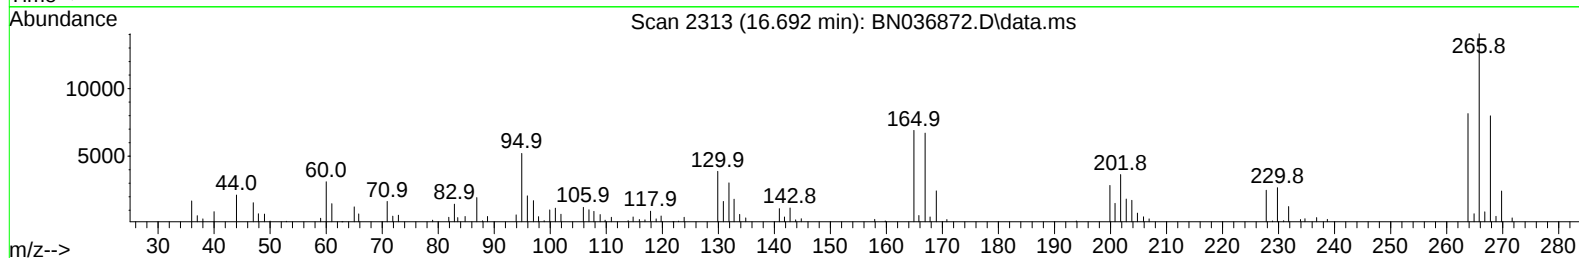


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036872.D
Acq On : 11 Apr 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 16:50:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

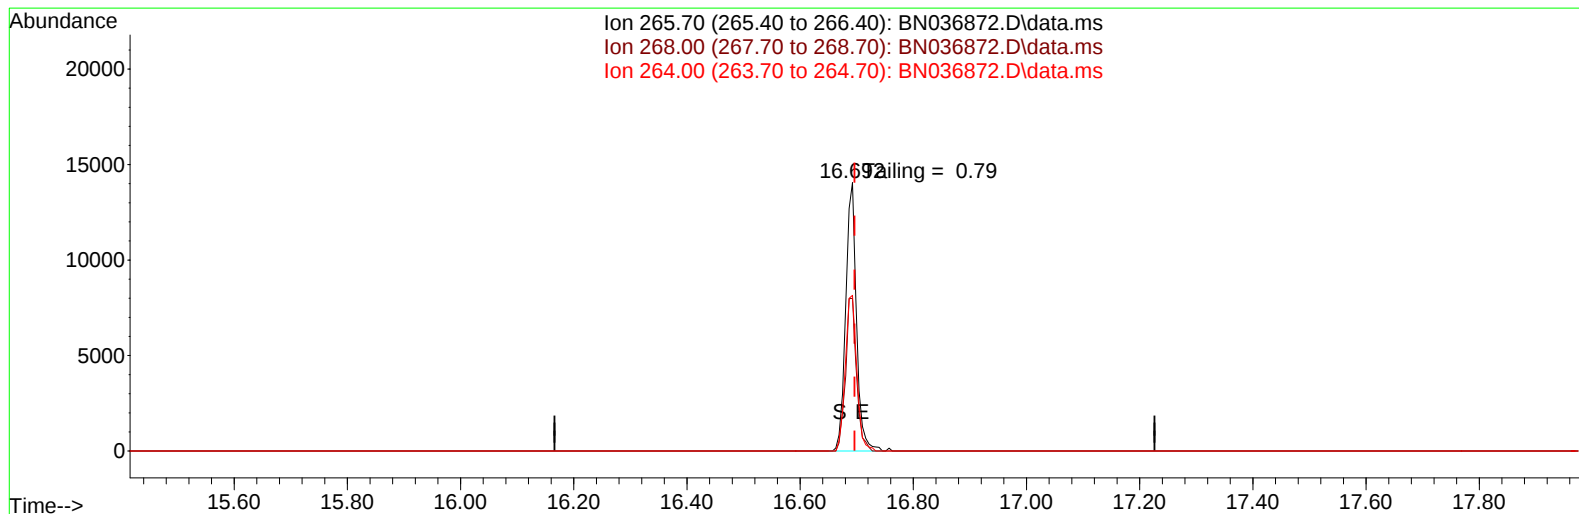

TIC: BN036872.D\data.ms

(70) Pentachlorophenol (C)




16.692min (-0.004) 36331.83 ng

response 18533

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.86
264.00	61.60	58.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041125\
Data File : BN036872.D
Acq On : 11 Apr 2025 11:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 11 16:50:38 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 01 00:16:52 2025
Response via : Initial Calibration

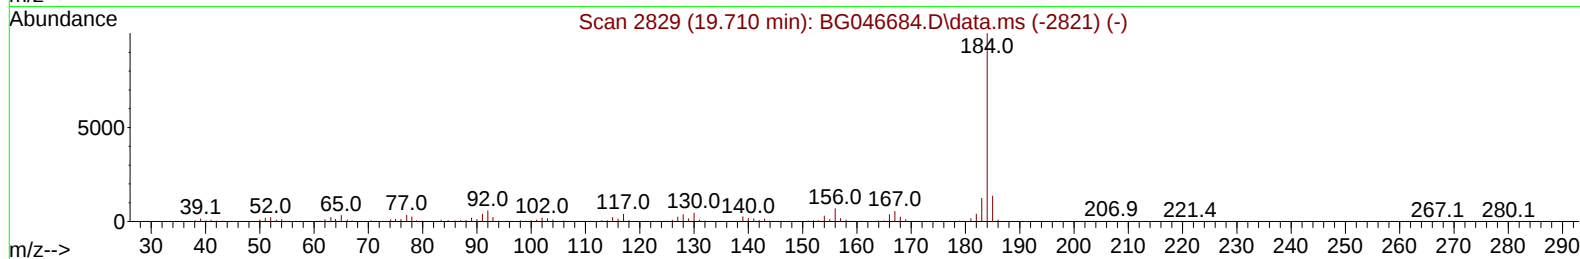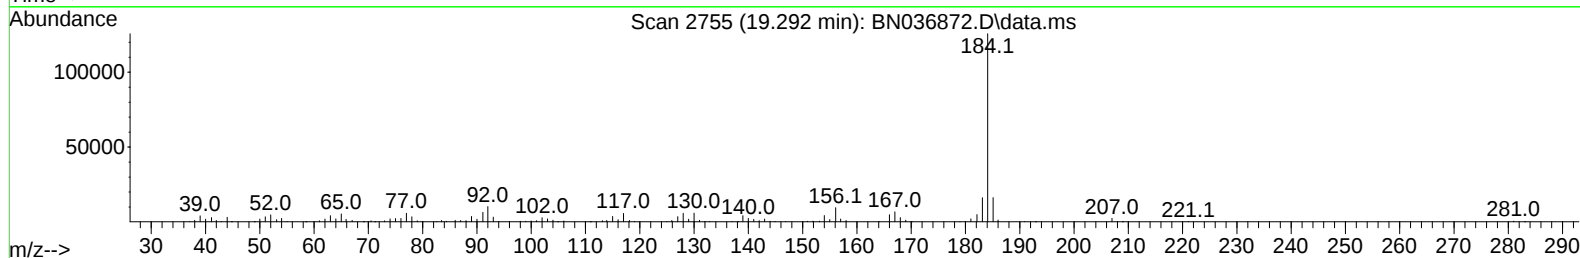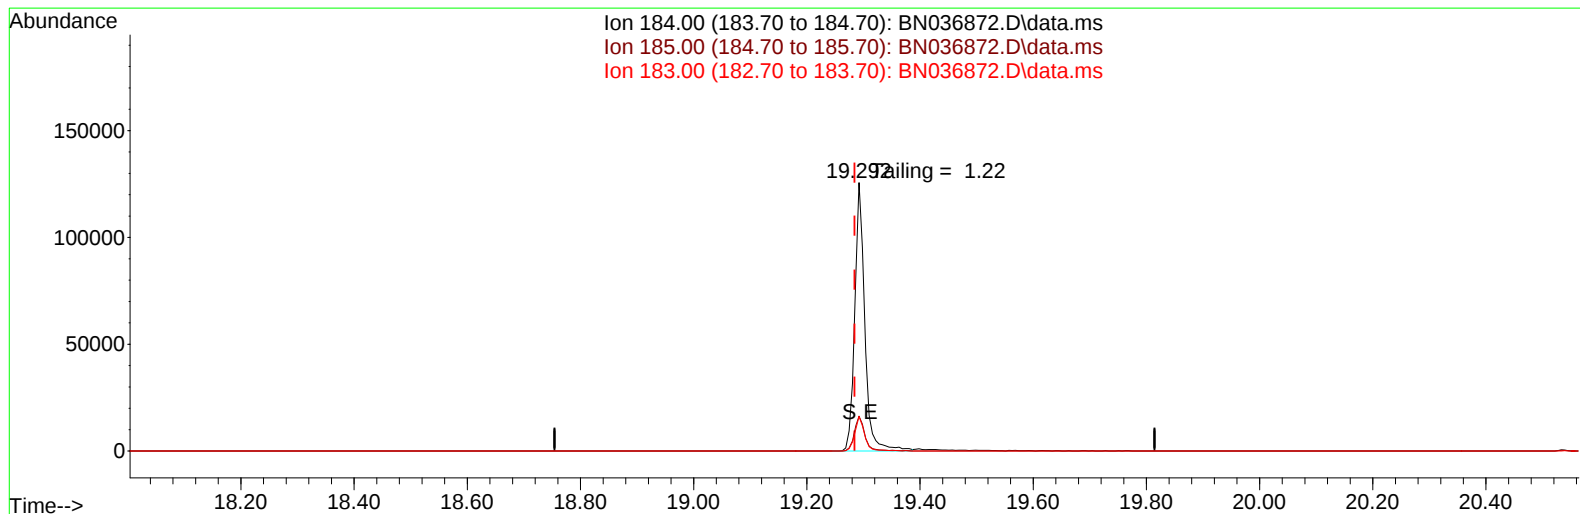

TIC: BN036872.D\data.ms

(77) Benzidine**19.292min (+ 0.008) 0.00 ng****response 156190**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.01
183.00	13.20	12.90
0.00	0.00	0.00