

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024842.D
 Acq On : 12 Apr 2023 11:24
 Operator : CG/JU
 Sample : PB152043BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK043

Quant Time: Apr 13 02:47:27 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	9742	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	30437	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.589	164	17177	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.339	188	35739	0.400	ng/ul	0.00
17) Chrysene-d12	21.533	240	27539	0.400	ng/ul	0.00
23) Perylene-d12	23.985	264	28981	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	65860	6.191	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	13599	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.364	212	27942	0.409	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.584	166	4725	0.076	ng/ul#	11
20) Pyrene	19.731	202	4341	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.836	252	10326	0.107	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024842.D
Acq On : 12 Apr 2023 11:24
Operator : CG/JU
Sample : PB152043BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK043

Quant Time: Apr 13 02:47:27 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration




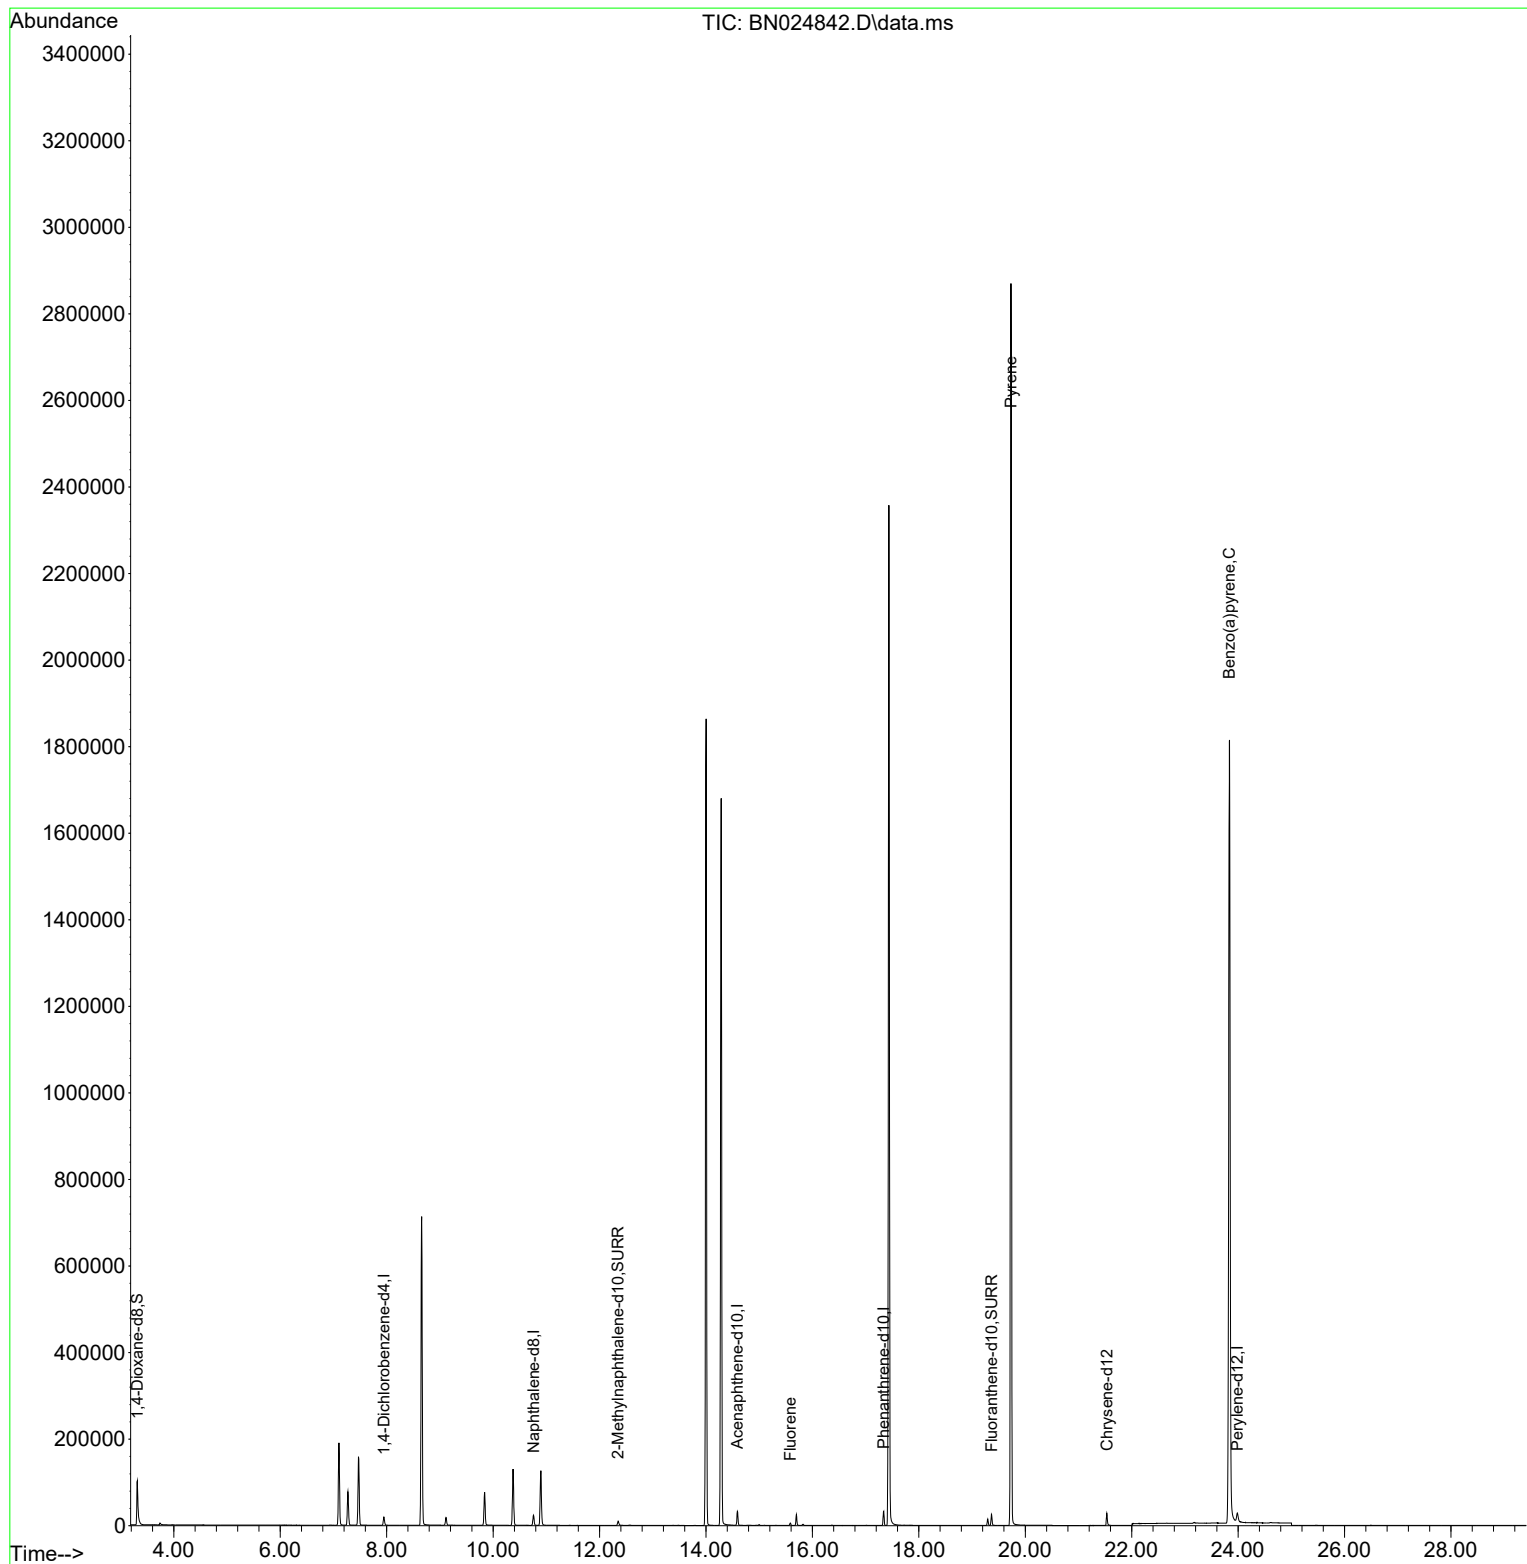


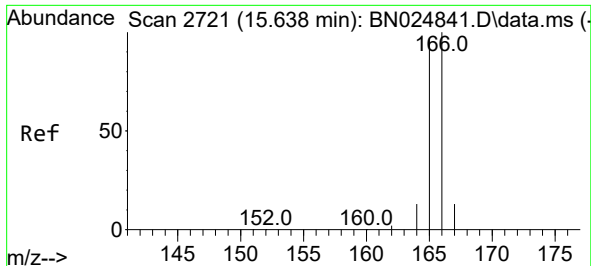

#12
Fluorene
Concen: 0.076 ng/ul
RT: 15.584 min Scan# 21
Delta R.T. -0.054 min
Lab File: BN024842.D
Acq: 12 Apr 2023 11:24




Instrument :
BNA_N
ClientSampleId :
SBLK043


Tgt Ion:166 Resp: 4725
Ion Ratio Lower Upper
166 100
165 5.8 80.1 120.1#
167 34.2 10.7 16.1#

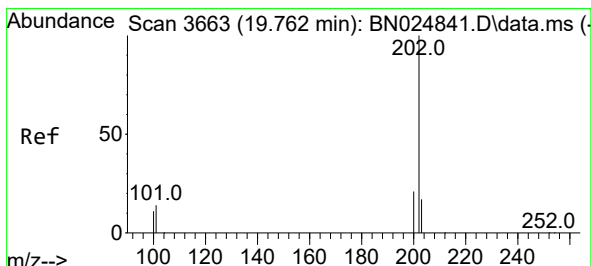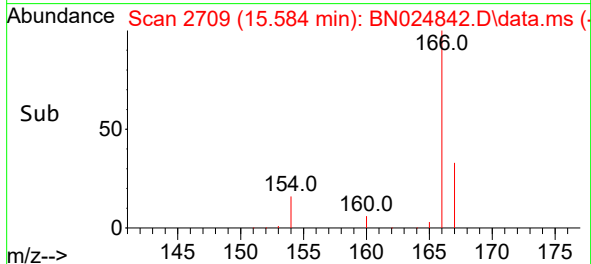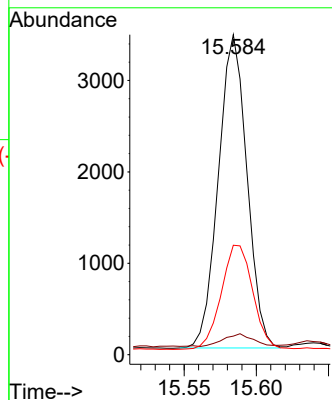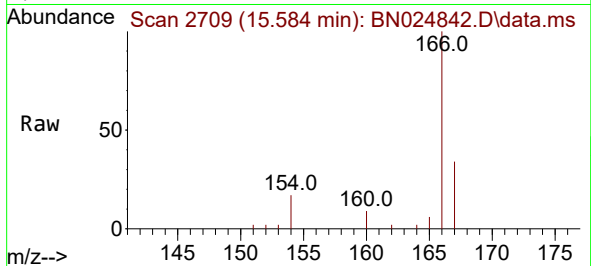

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.731 min Scan# 3656
Delta R.T. -0.031 min
Lab File: BN024842.D
Acq: 12 Apr 2023 11:24


Tgt Ion:202 Resp: 4341
Ion Ratio Lower Upper
202 100
101 177.3 11.8 17.8#
100 1351.4 9.5 14.3#

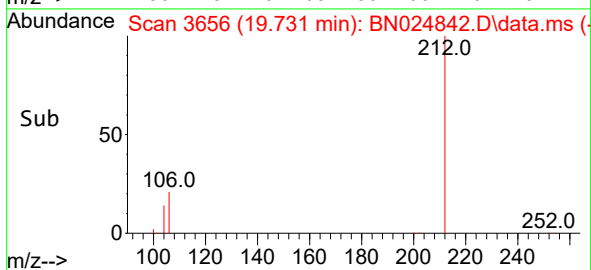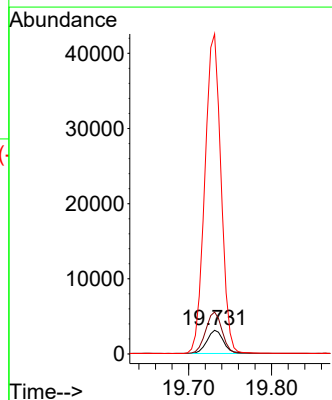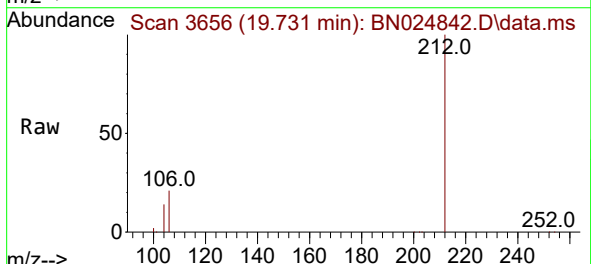

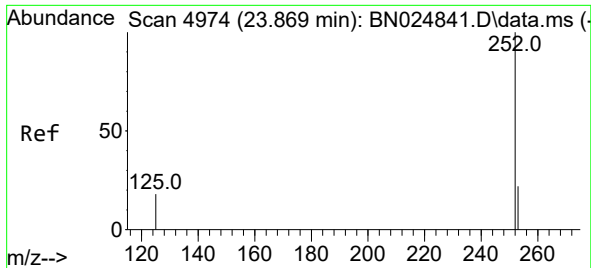

#26
Benzo(a)pyrene
Concen: 0.107 ng/ul
RT: 23.836 min Scan# 4962
Delta R.T. -0.033 min
Lab File: BN024842.D
Acq: 12 Apr 2023 11:24

Instrument :
BNA_N
ClientSampleId :
SBLK043

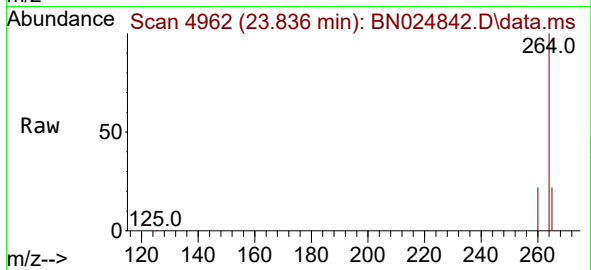

Tgt Ion:252 Resp: 10326
Ion Ratio Lower Upper
252 100
253 43.1 20.7 31.1#
125 38.4 15.9 23.9#

