

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024843.D
 Acq On : 12 Apr 2023 12:01
 Operator : CG/JU
 Sample : PB152056BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK056

Quant Time: Apr 13 02:47:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	11891	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	36258	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.593	164	20802	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.338	188	42782	0.400	ng/ul	0.00
17) Chrysene-d12	21.538	240	33265	0.400	ng/ul	0.00
23) Perylene-d12	23.978	264	37332	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.318	96	87913	6.770	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	17361	0.373	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	37825	0.458	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.735	202	5721	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.826	252	13180	0.106	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024843.D
Acq On : 12 Apr 2023 12:01
Operator : CG/JU
Sample : PB152056BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK056

Quant Time: Apr 13 02:47:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration




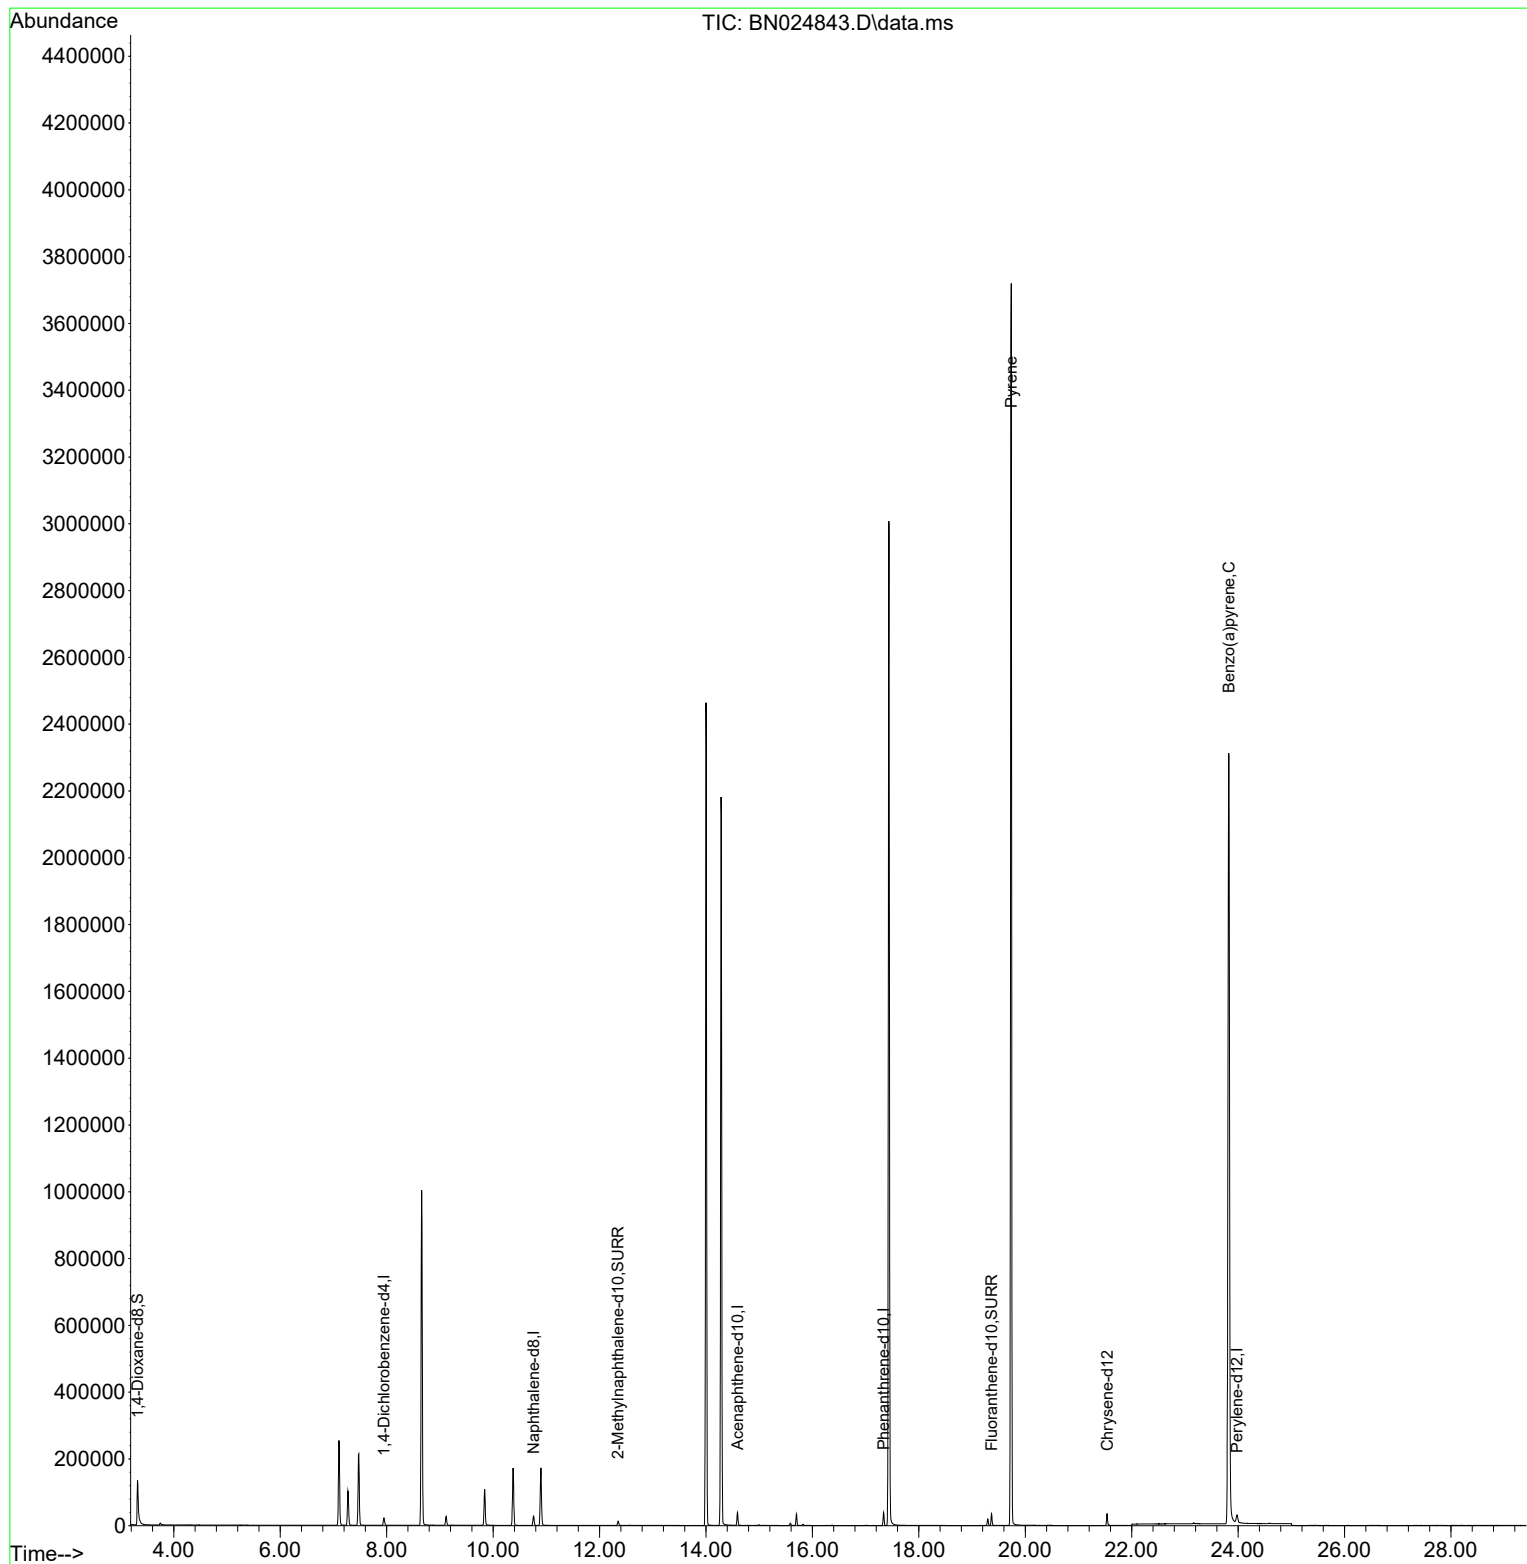


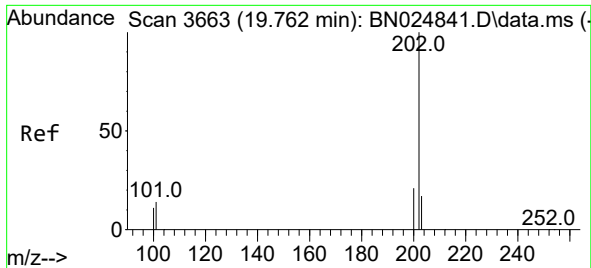

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.735 min Scan# 3657
Delta R.T. -0.027 min
Lab File: BN024843.D
Acq: 12 Apr 2023 12:01

Instrument :
BNA_N
ClientSampleId :
SBLK056

Tgt Ion:202 Resp: 5721
Ion Ratio Lower Upper
202 100
101 177.7 11.8 17.8#
100 1282.9 9.5 14.3#

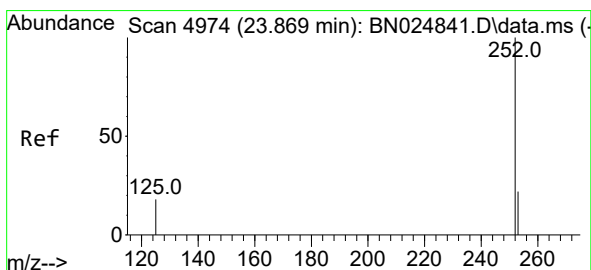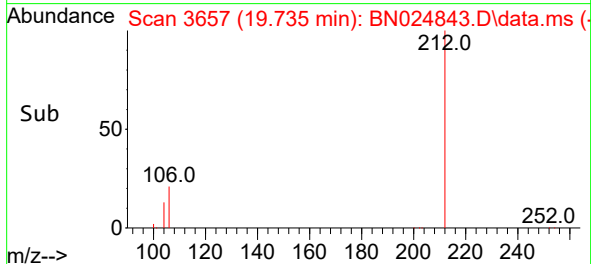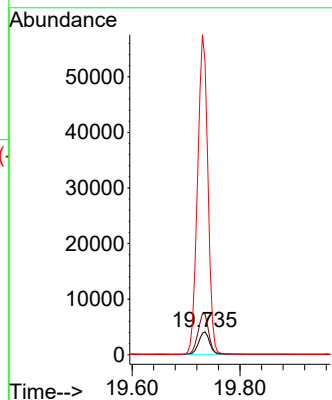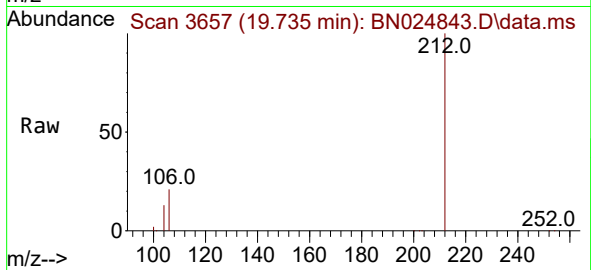

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.826 min Scan# 4959
Delta R.T. -0.043 min
Lab File: BN024843.D
Acq: 12 Apr 2023 12:01

Tgt Ion:252 Resp: 13180
Ion Ratio Lower Upper
252 100
253 40.0 20.7 31.1#
125 36.4 15.9 23.9#

