

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024844.D
 Acq On : 12 Apr 2023 12:38
 Operator : CG/JU
 Sample : 02250-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDW1

Quant Time: Apr 13 02:47:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	9866	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	30158	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.593	164	17847	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.338	188	37224	0.400	ng/ul	0.00
17) Chrysene-d12	21.535	240	29147	0.400	ng/ul	0.00
23) Perylene-d12	23.978	264	29841	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	51237	4.756	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	12545	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	31255	0.432	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	10502	0.885	ng/ul	96
20) Pyrene	19.735	202	4916	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.821	252	9897	0.100	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024844.D
Acq On : 12 Apr 2023 12:38
Operator : CG/JU
Sample : 02250-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDW1

Quant Time: Apr 13 02:47:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration




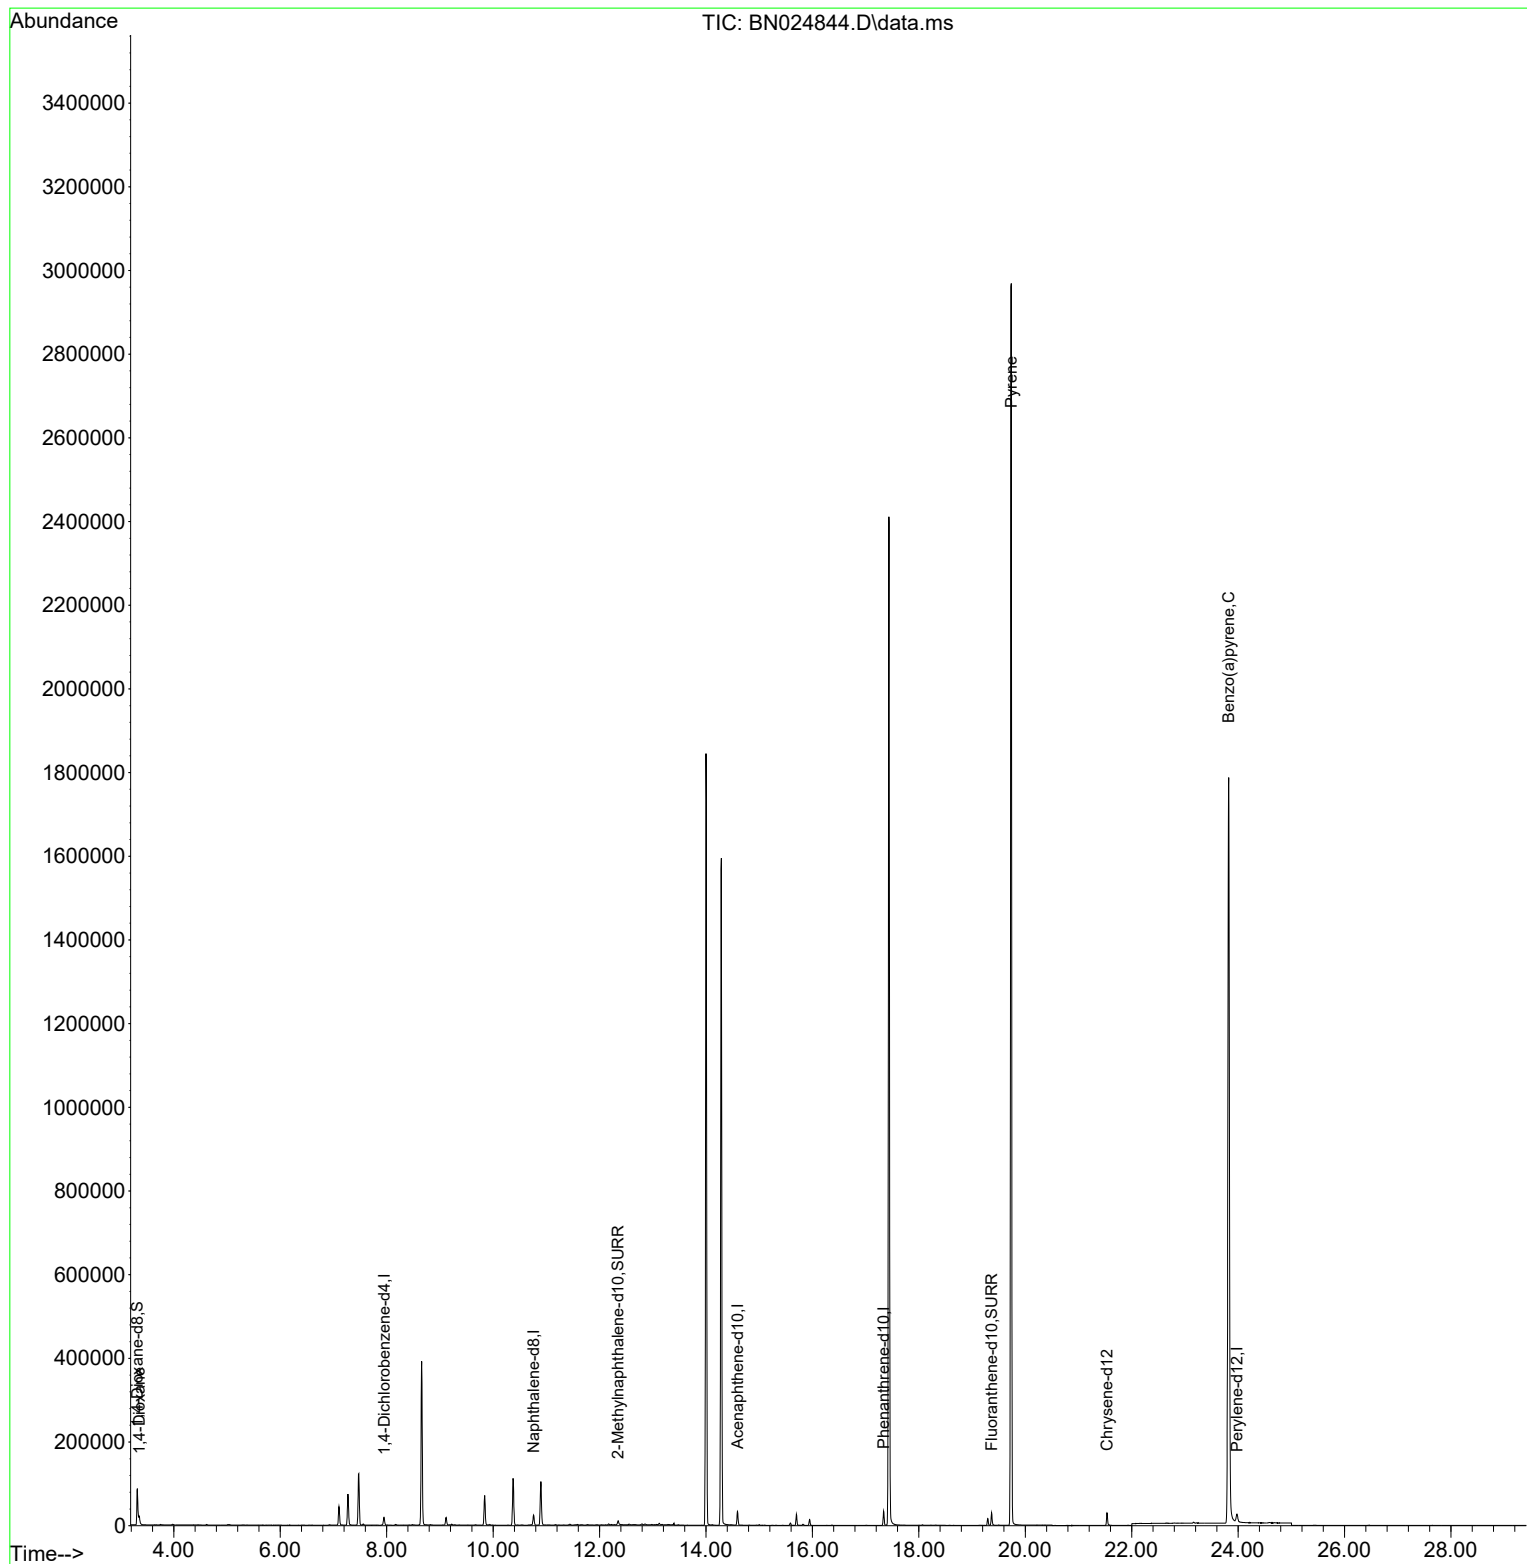


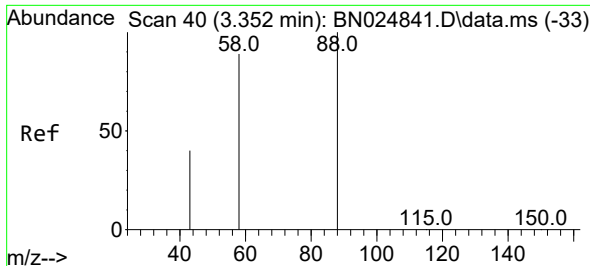

#2
 1,4-Dioxane
 Concen: 0.885 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN024844.D
 Acq: 12 Apr 2023 12:38




Instrument :
 BNA_N
 ClientSampleId :
 BHDW1


Tgt Ion: 88 Resp: 10502
 Ion Ratio Lower Upper
 88 100
 43 45.8 39.1 58.7
 58 84.8 65.7 98.5

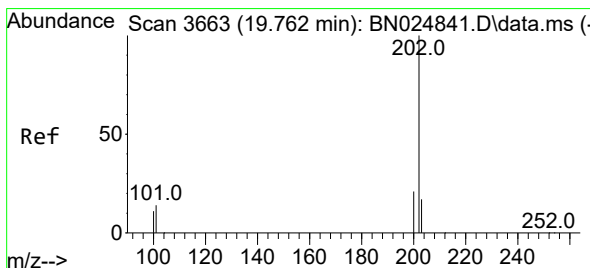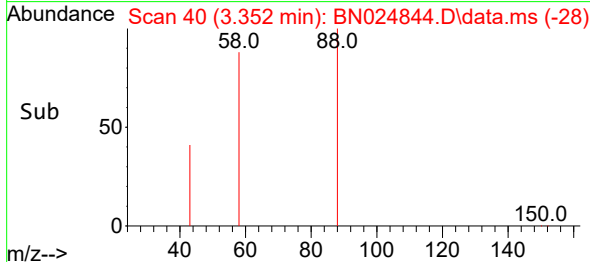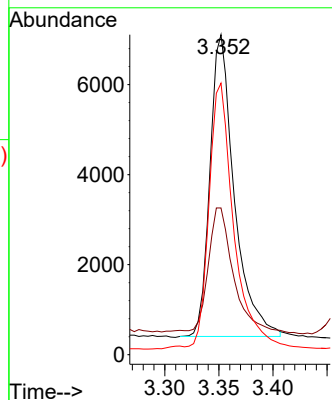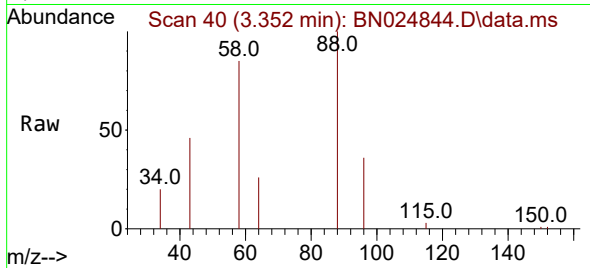

#20
 Pyrene
 Concen: 0.048 ng/ul
 RT: 19.735 min Scan# 3657
 Delta R.T. -0.027 min
 Lab File: BN024844.D
 Acq: 12 Apr 2023 12:38

Tgt Ion: 202 Resp: 4916
 Ion Ratio Lower Upper
 202 100
 101 171.3 11.8 17.8#
 100 1225.5 9.5 14.3#

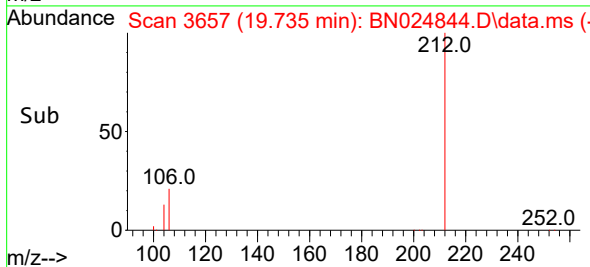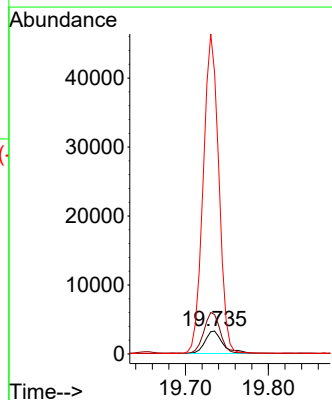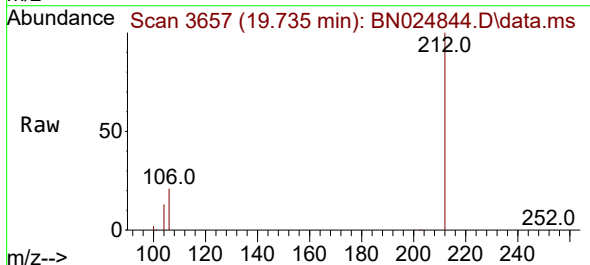

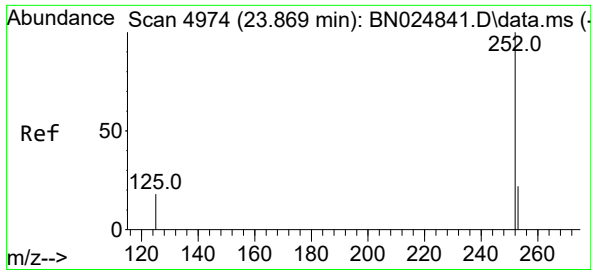

#26

Benzo(a)pyrene

Concen: 0.100 ng/ul

RT: 23.821 min Scan# 49

Delta R.T. -0.049 min

Lab File: BN024844.D


Acq: 12 Apr 2023 12:38

Instrument :

BNA_N

ClientSampleId :

BHDW1

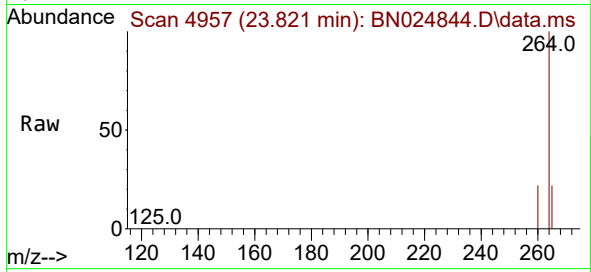

Tgt Ion:252 Resp: 9897

Ion Ratio Lower Upper

252 100

253 42.8 20.7 31.1#

125 40.1 15.9 23.9#

