

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024849.D
 Acq On : 12 Apr 2023 15:46
 Operator : CG/JU
 Sample : 02250-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDY5

Quant Time: Apr 13 02:48:09 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7965	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	24716	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.594	164	14760	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.339	188	31550	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	26634	0.400	ng/ul	0.00
23) Perylene-d12	23.994	264	26275	0.400	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	45256	5.203	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	12641	0.398	ng/ul	0.00
18) Fluoranthene-d10	19.369	212	32091	0.485	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	755	0.079	ng/ul#	63
20) Pyrene	19.736	202	5028	0.054	ng/ul#	1
26) Benzo(a)pyrene	23.845	252	10403	0.119	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024849.D
Acq On : 12 Apr 2023 15:46
Operator : CG/JU
Sample : 02250-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDY5

Quant Time: Apr 13 02:48:09 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration




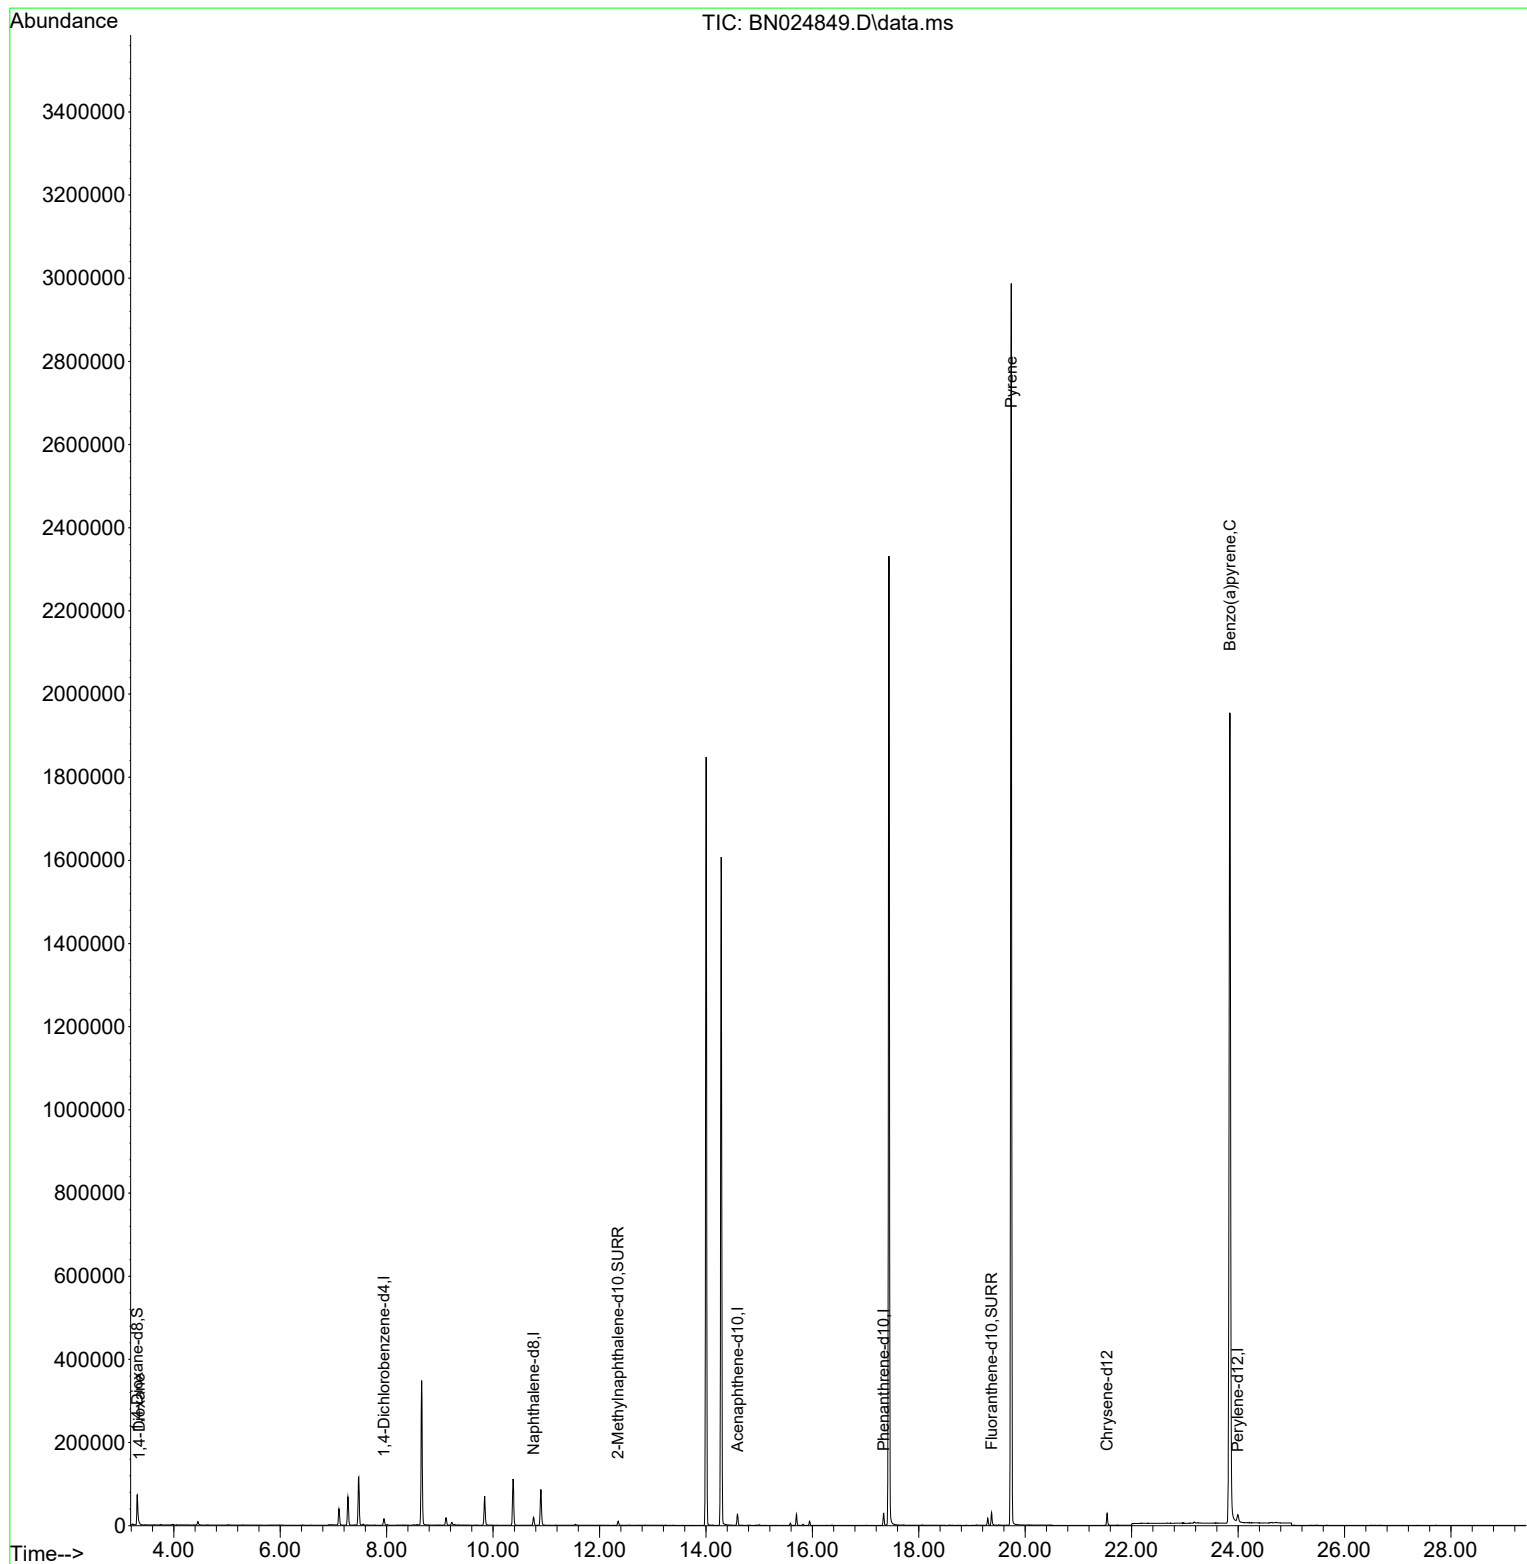


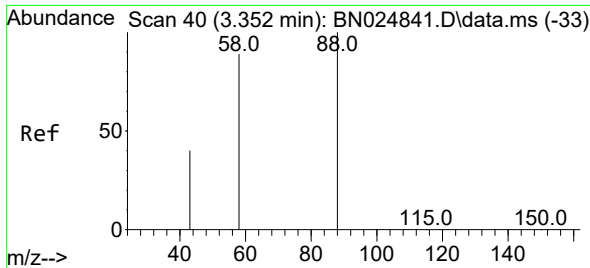

#2
 1,4-Dioxane
 Concen: 0.079 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN024849.D
 Acq: 12 Apr 2023 15:46




Instrument :
 BNA_N
 ClientSampleId :
 BHDY5


Tgt Ion: 88 Resp: 755
 Ion Ratio Lower Upper
 88 100
 43 93.6 39.1 58.7#
 58 64.7 65.7 98.5#

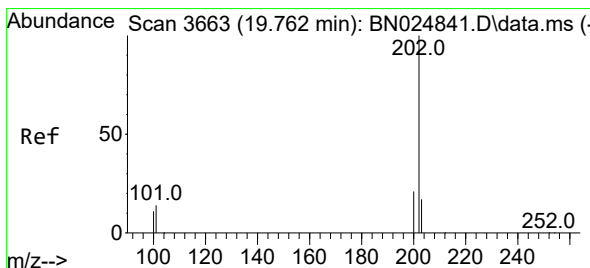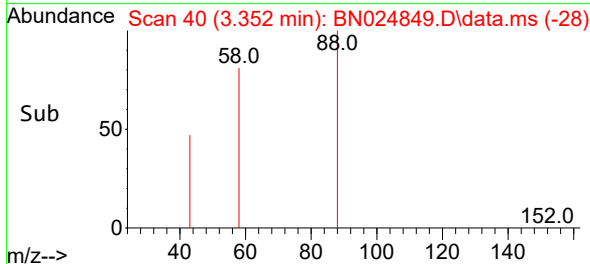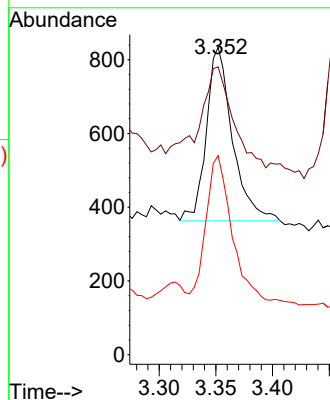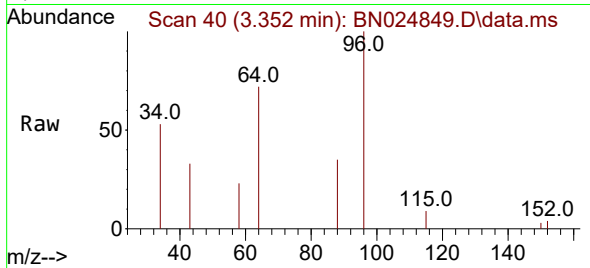

#20
 Pyrene
 Concen: 0.054 ng/ul
 RT: 19.736 min Scan# 3657
 Delta R.T. -0.026 min
 Lab File: BN024849.D
 Acq: 12 Apr 2023 15:46


Tgt Ion: 202 Resp: 5028
 Ion Ratio Lower Upper
 202 100
 101 176.1 11.8 17.8#
 100 1291.6 9.5 14.3#

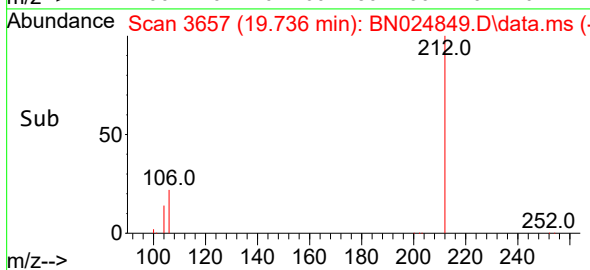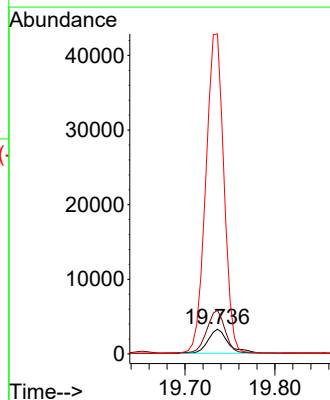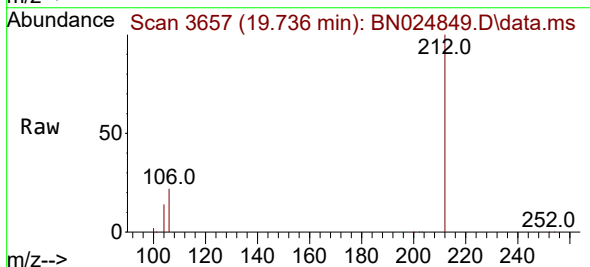

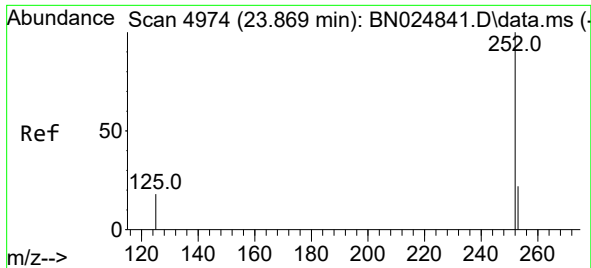

#26
 Benzo(a)pyrene
 Concen: 0.119 ng/ul
 RT: 23.845 min Scan# 4965
 Delta R.T. -0.024 min
 Lab File: BN024849.D
 Acq: 12 Apr 2023 15:46

Instrument :
 BNA_N
 ClientSampleId :
 BHDY5

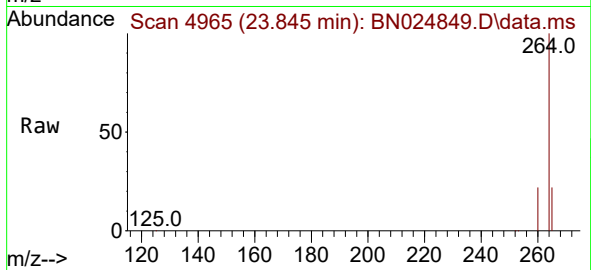

Tgt Ion:252 Resp: 10403
 Ion Ratio Lower Upper
 252 100
 253 42.8 20.7 31.1#
 125 38.1 15.9 23.9#

