

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024844.D
 Acq On : 12 Apr 2023 12:38
 Operator : CG/JU
 Sample : 02250-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDW1

Quant Time: Apr 13 02:47:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	9866	0.400	ng/u1	0.00
4) Naphthalene-d8	10.759	136	30158	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.593	164	17847	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.338	188	37224	0.400	ng/u1	0.00
17) Chrysene-d12	21.535	240	29147	0.400	ng/u1	0.00
23) Perylene-d12	23.978	264	29841	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	51237	4.756	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	12545	0.324	ng/u1	0.00
18) Fluoranthene-d10	19.368	212	31255	0.432	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.352	88	10502	0.885	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024844.D
Acq On : 12 Apr 2023 12:38
Operator : CG/JU
Sample : 02250-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDW1

Quant Time: Apr 13 02:47:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

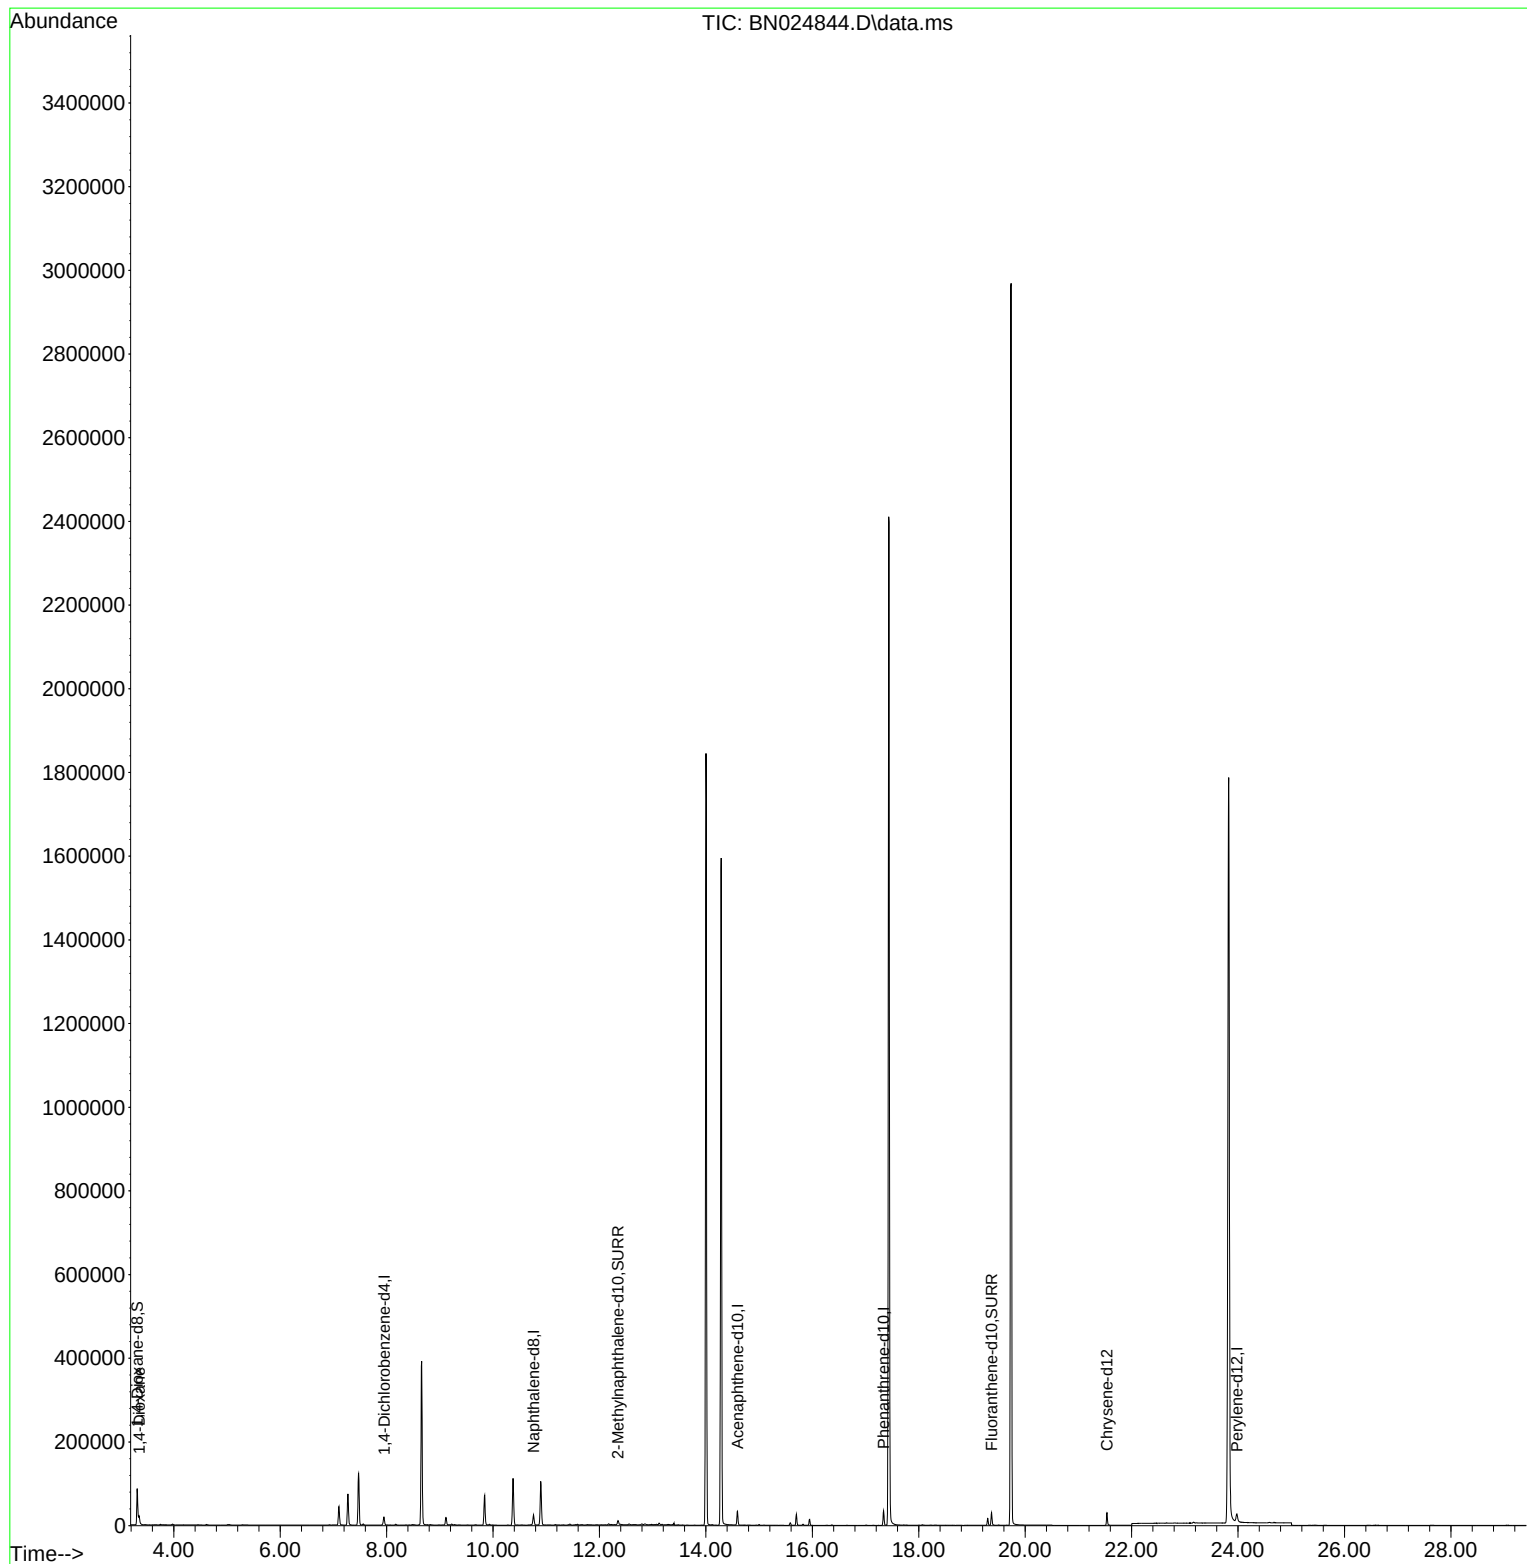

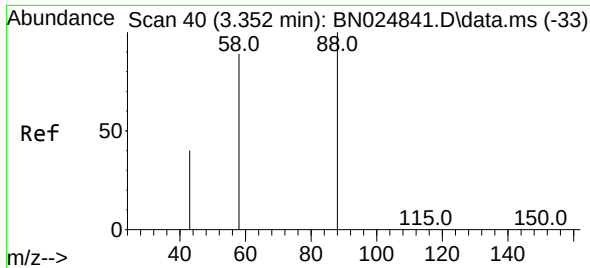

#2

1,4-Dioxane

Concen: 0.885 ng/ul

RT: 3.352 min Scan# 40

Delta R.T. 0.000 min

Lab File: BN024844.D


Acq: 12 Apr 2023 12:38

Instrument :

BNA_N

ClientSampleId :

BHDW1

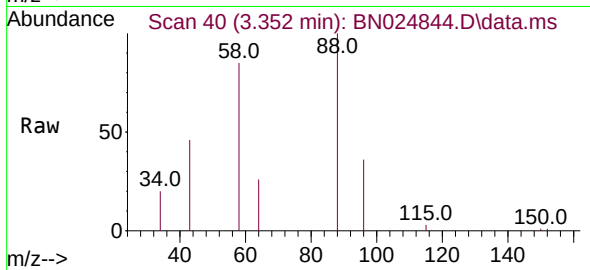

Tgt Ion: 88 Resp: 10502

Ion Ratio Lower Upper

88 100

43 45.8 39.1 58.7

58 84.8 65.7 98.5

