

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024848.D
 Acq On : 12 Apr 2023 15:08
 Operator : CG/JU
 Sample : 02250-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDY4

Quant Time: Apr 13 02:48:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	8349	0.400	ng/u1	0.00
4) Naphthalene-d8	10.759	136	25417	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.593	164	14973	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.338	188	32598	0.400	ng/u1	0.00
17) Chrysene-d12	21.531	240	27539	0.400	ng/u1	0.00
23) Perylene-d12	23.987	264	28246	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	49684	5.450	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	12414	0.380	ng/u1	0.00
18) Fluoranthene-d10	19.368	212	35540	0.520	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.352	88	13433	1.337	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024848.D
Acq On : 12 Apr 2023 15:08
Operator : CG/JU
Sample : 02250-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDY4


Quant Time: Apr 13 02:48:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

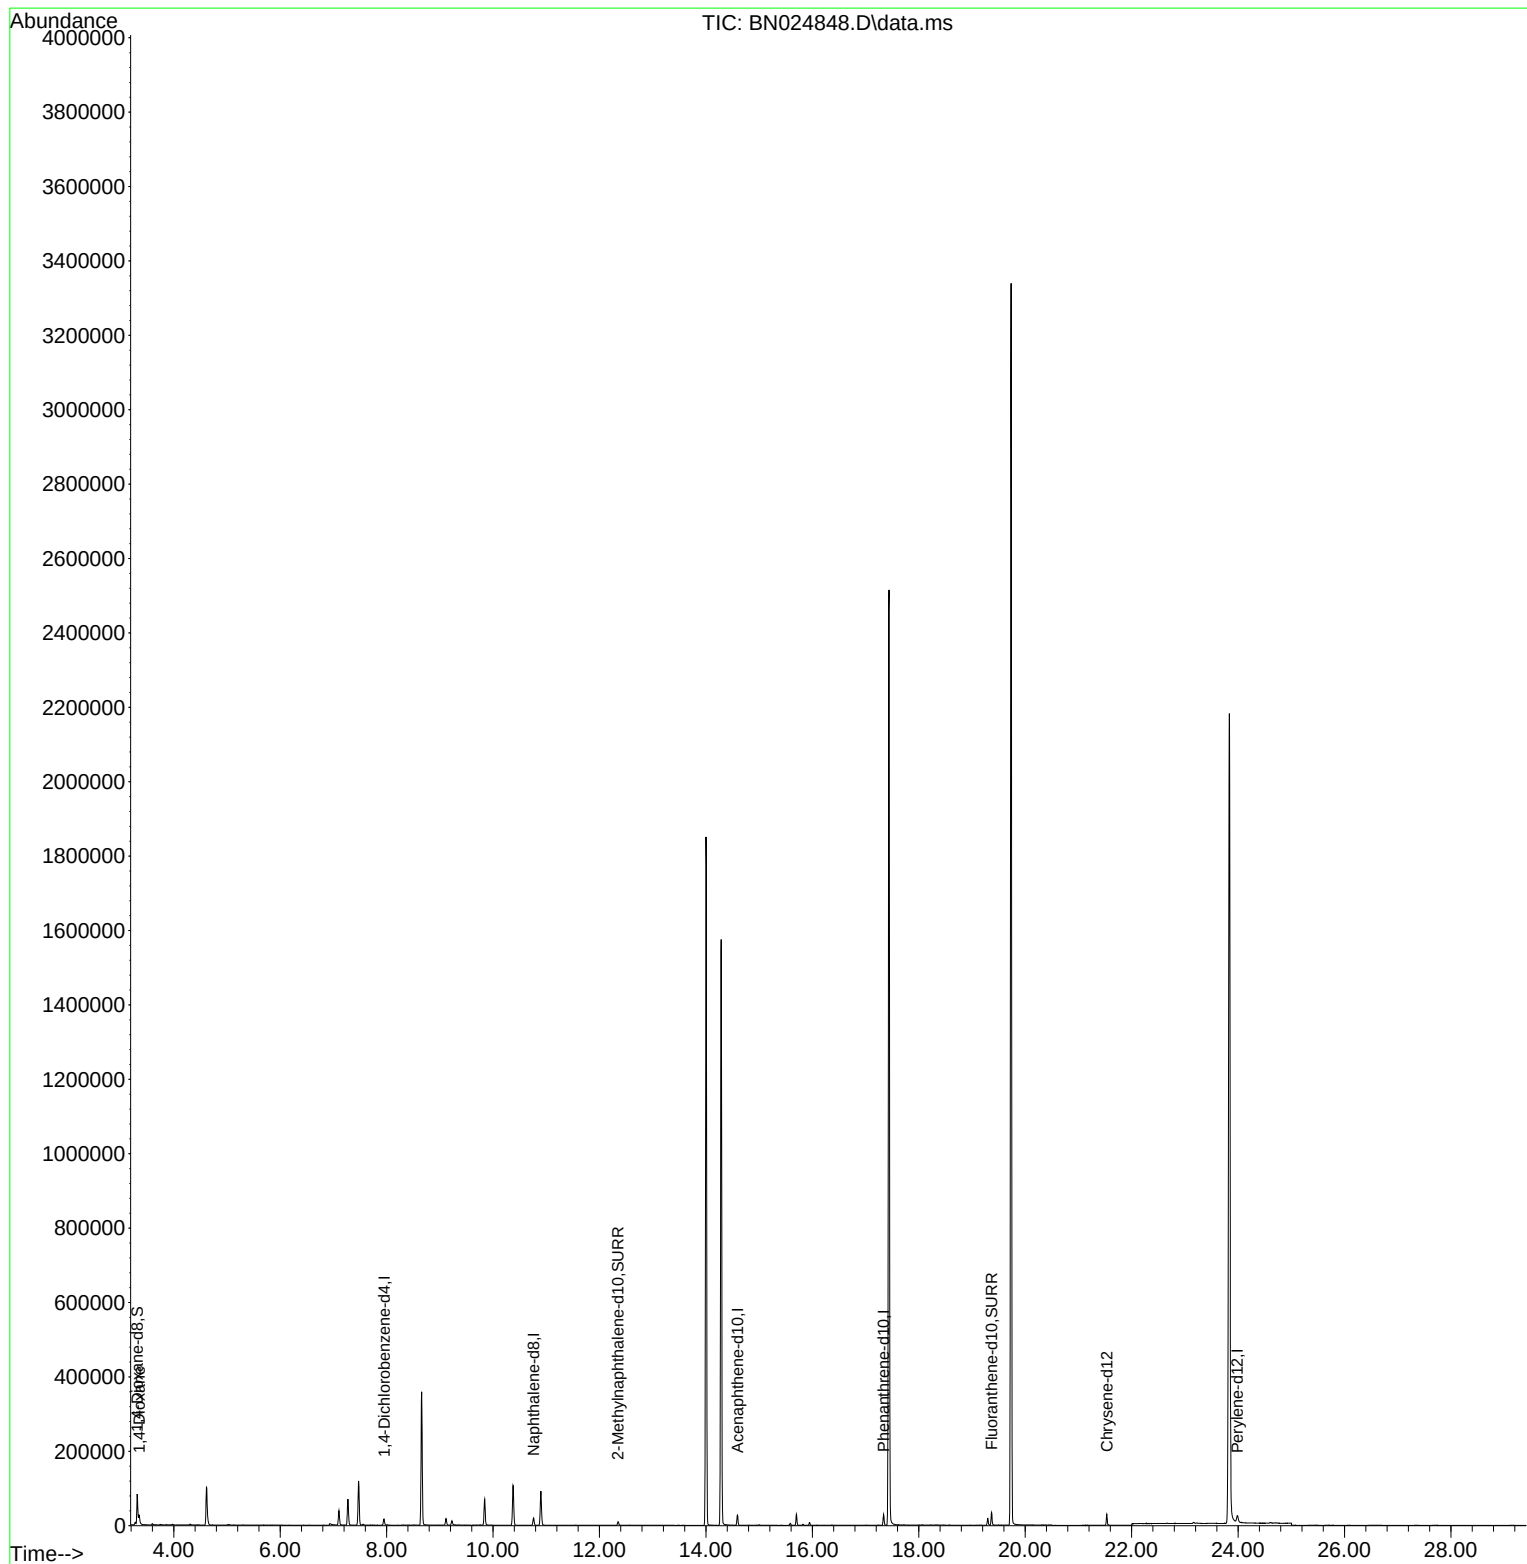

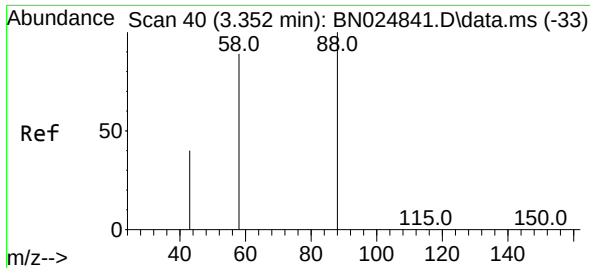

#2
 1,4-Dioxane
 Concen: 1.337 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN024848.D
 Acq: 12 Apr 2023 15:08

Instrument :
 BNA_N
 ClientSampleId :
 BHDY4

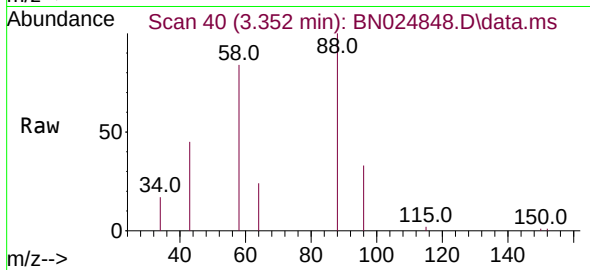

Tgt Ion:	88	Resp:	13433
Ion	Ratio	Lower	Upper
88	100		
43	44.6	39.1	58.7
58	83.7	65.7	98.5

