

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
 Data File : BN024850.D
 Acq On : 12 Apr 2023 16:24
 Operator : CG/JU
 Sample : 02250-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDY6

Quant Time: Apr 13 02:48:15 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	8051	0.400	ng/u1	0.00
4) Naphthalene-d8	10.759	136	23561	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.593	164	14485	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.338	188	31303	0.400	ng/u1	0.00
17) Chrysene-d12	21.535	240	25452	0.400	ng/u1	0.00
23) Perylene-d12	23.993	264	26394	0.400	ng/u1	# 0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	53271	6.059	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	13159	0.435	ng/u1	0.00
18) Fluoranthene-d10	19.368	212	34823	0.551	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.352	88	6403	0.661	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041223\
Data File : BN024850.D
Acq On : 12 Apr 2023 16:24
Operator : CG/JU
Sample : 02250-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDY6

Quant Time: Apr 13 02:48:15 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

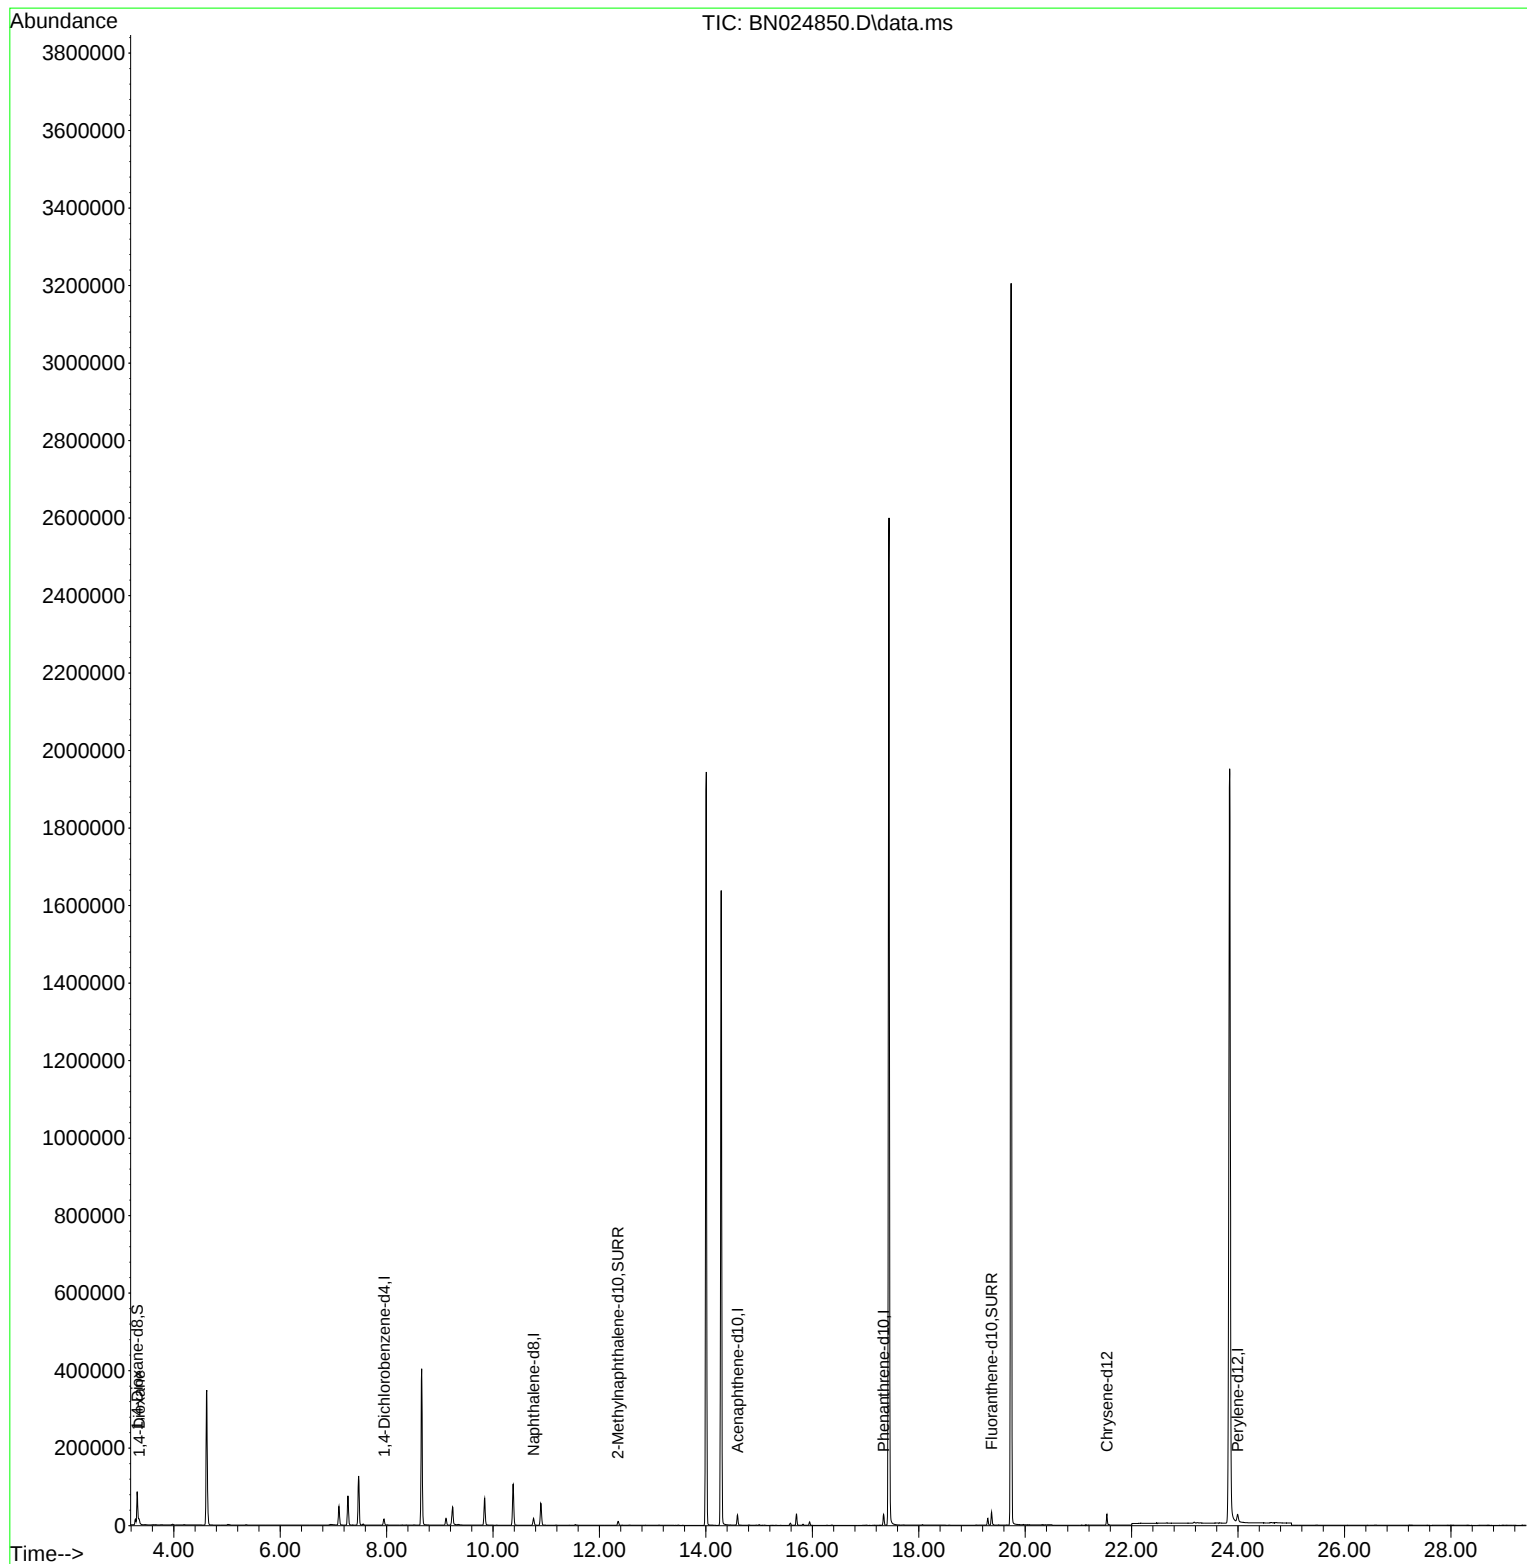

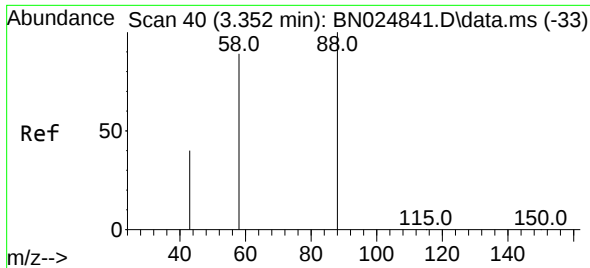

#2

1,4-Dioxane

Concen: 0.661 ng/ul

RT: 3.352 min Scan# 40

Delta R.T. 0.000 min

Lab File: BN024850.D


Acq: 12 Apr 2023 16:24

Instrument :

BNA_N

ClientSampleId :

BHDY6

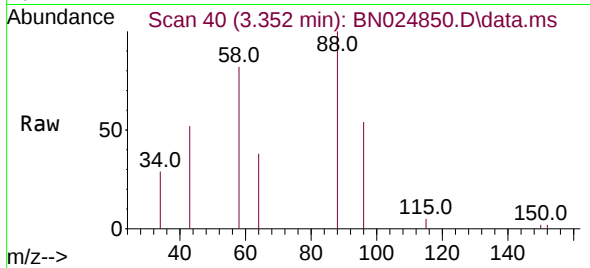

Tgt Ion: 88 Resp: 6403

Ion Ratio Lower Upper

88 100

43 52.1 39.1 58.7

58 82.3 65.7 98.5

