
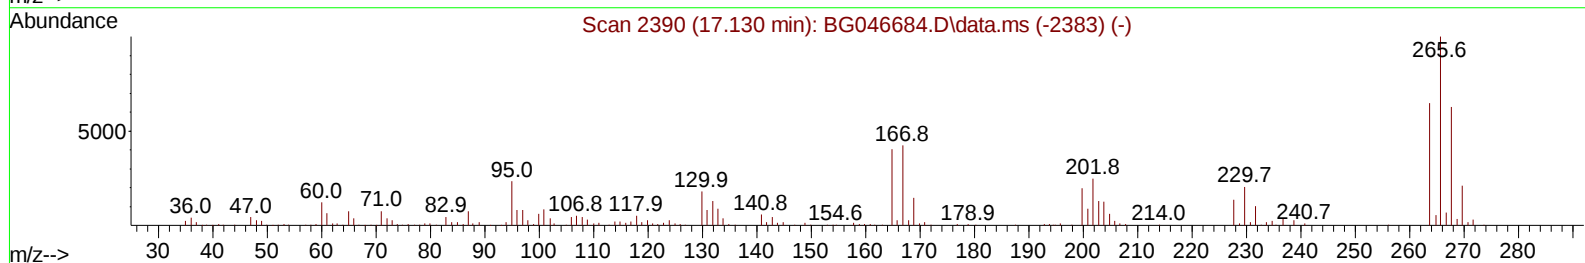
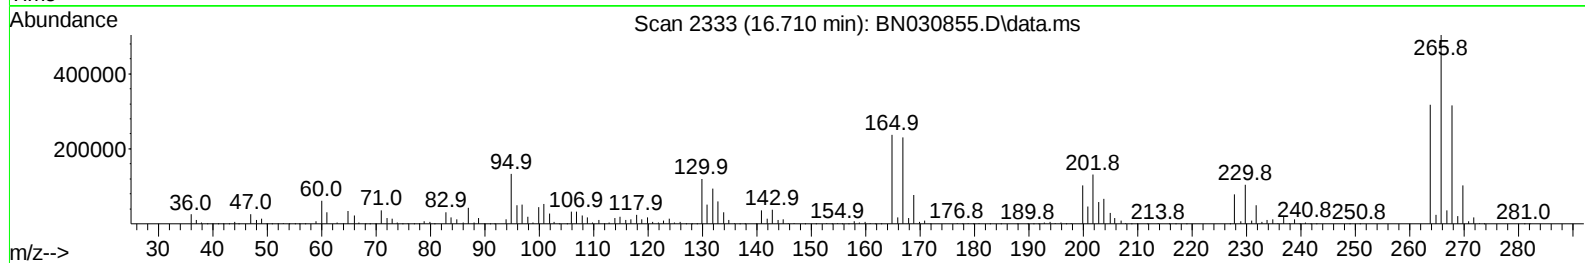


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030855.D
Acq On : 12 Apr 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 03:39:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 03:37:46 2024
Response via : Initial Calibration

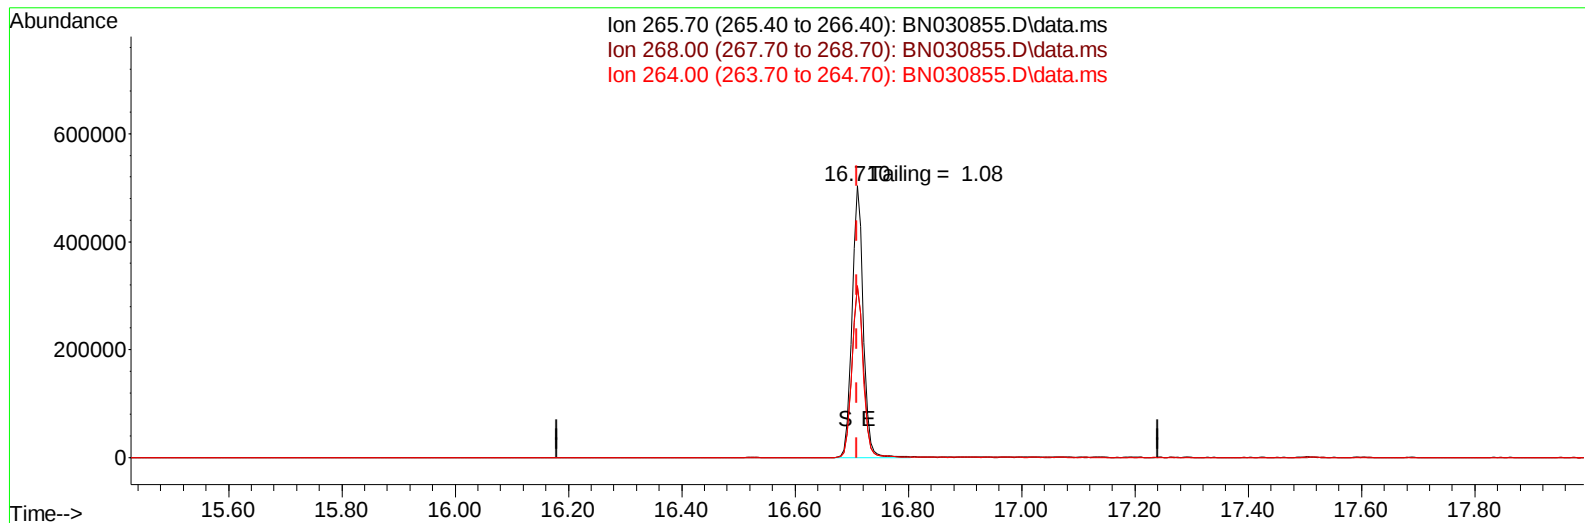




TIC: BN030855.D\data.ms

(70) Pentachlorophenol (C)**16.710min (+ 0.000) 25700.37 ng****response 696839**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030855.D
Acq On : 12 Apr 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 13 03:39:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 03:37:46 2024
Response via : Initial Calibration

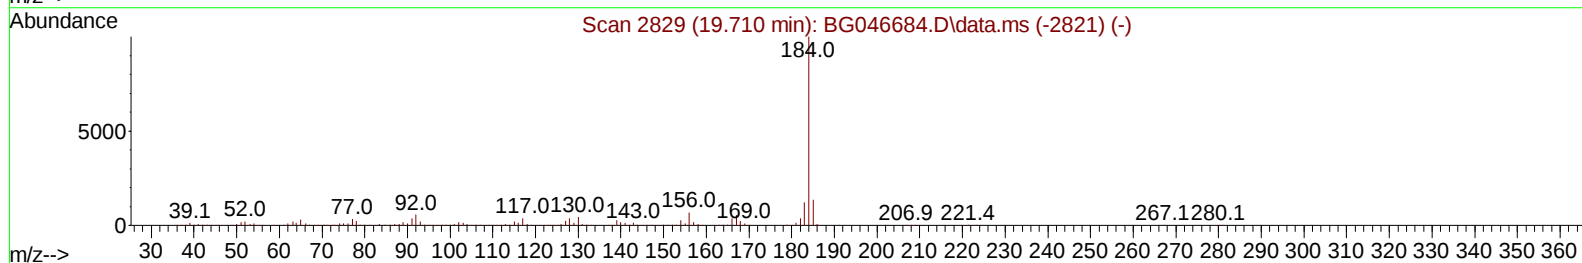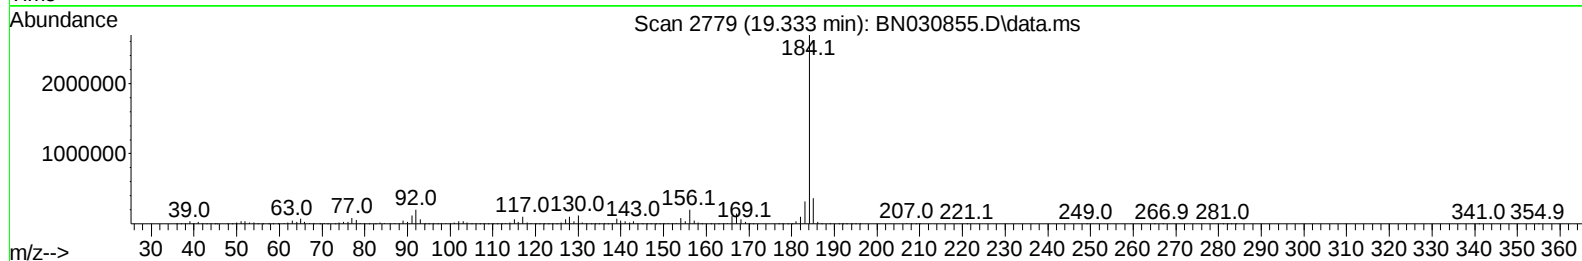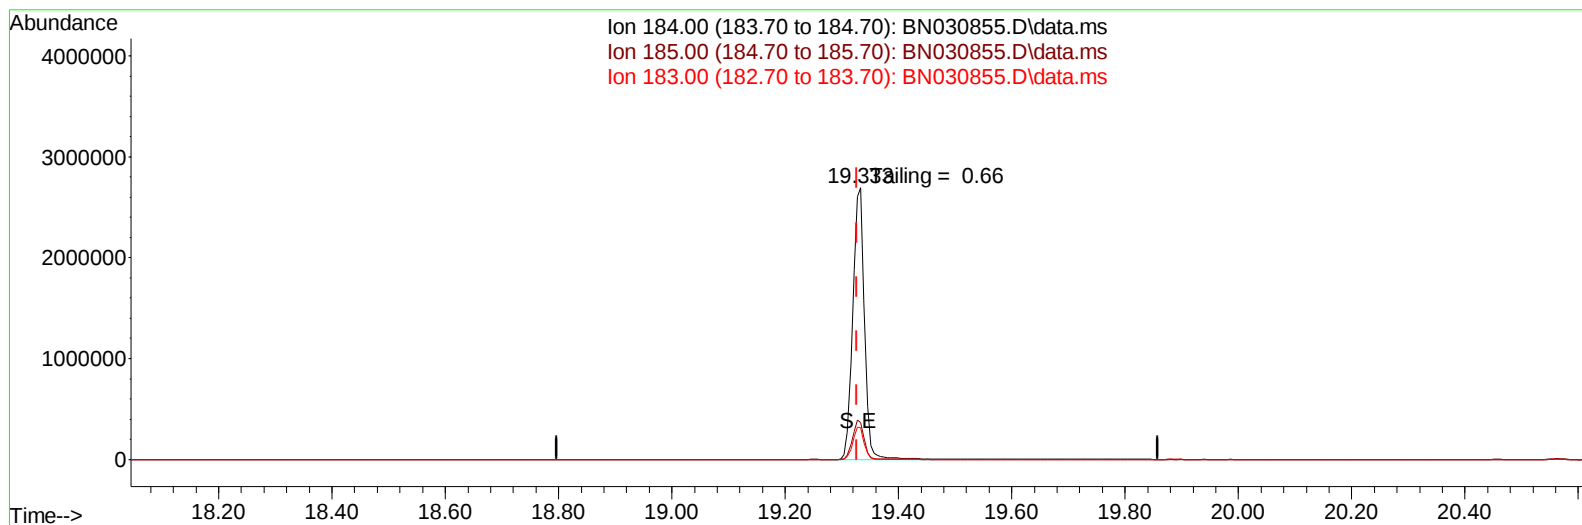

TIC: BN030855.D\data.ms

(77) Benzidine

19.333min (+ 0.006) 0.00 ng

response 3883665

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.74
0.00	0.00	0.00