
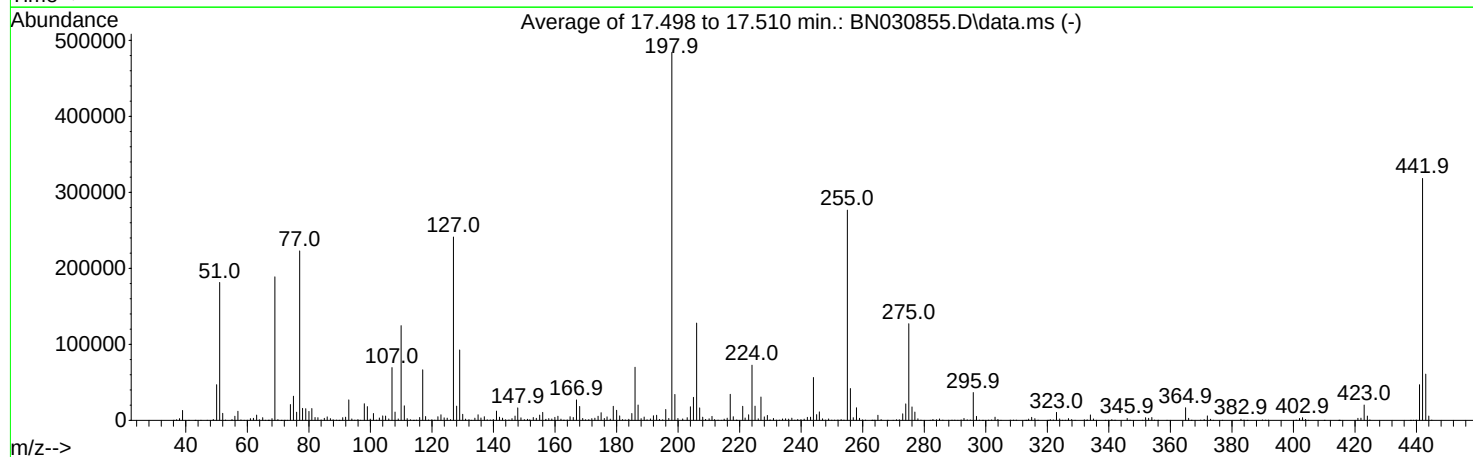


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030855.D
Acq On : 12 Apr 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 12 15:55:57 2024

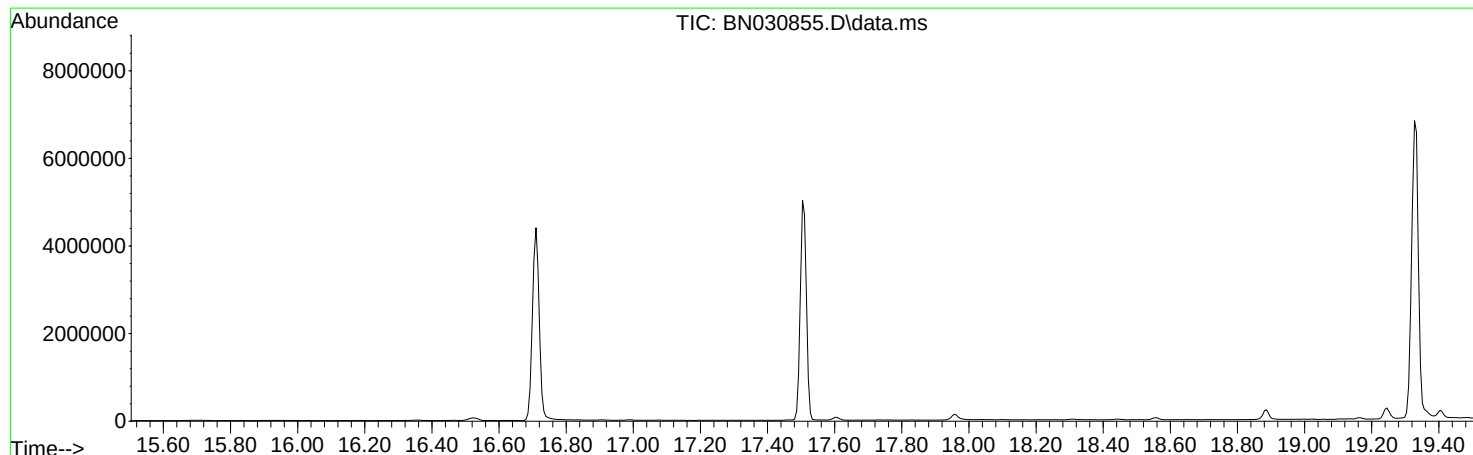




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	181440	PASS
68	69	0.00	2	1.3	2415	PASS
69	198	0.00	100	39.0	188947	PASS
70	69	0.00	2	0.5	962	PASS
127	198	10	80	49.9	241365	PASS
197	198	0.00	2	0.5	2448	PASS
198	198	100	100	100.0	484011	PASS
199	198	5	9	7.0	34117	PASS
275	198	10	60	26.3	127197	PASS
365	198	1	100	3.4	16587	PASS
441	198	0.01	100	9.7	46864	PASS
442	442	50	100	100.0	318336	PASS
443	442	15	24	19.1	60752	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030855.D
Acq On : 12 Apr 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 13 03:39:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 03:37:46 2024
Response via : Initial Calibration

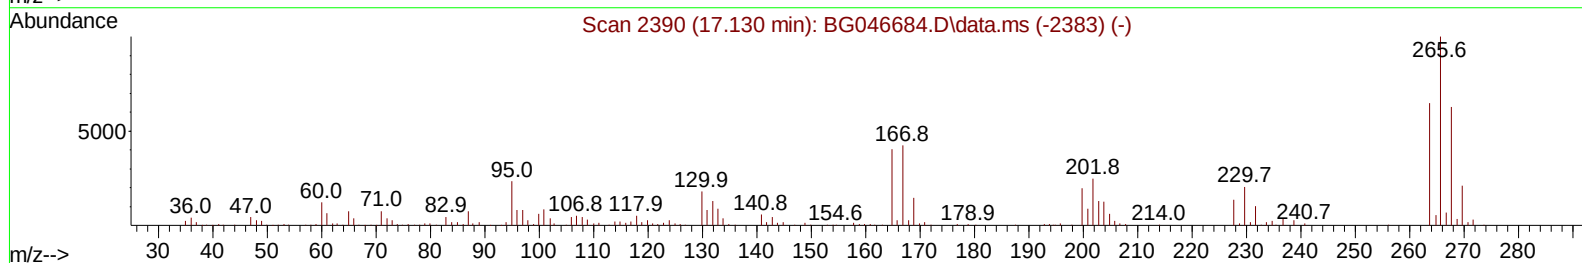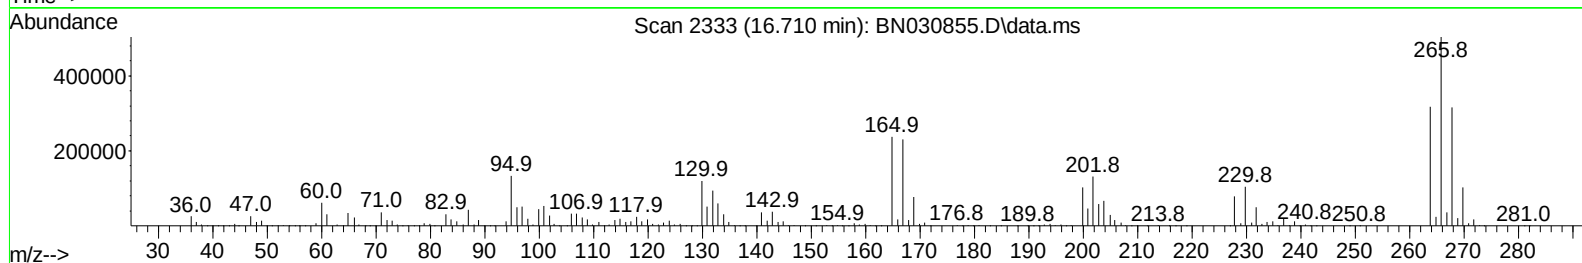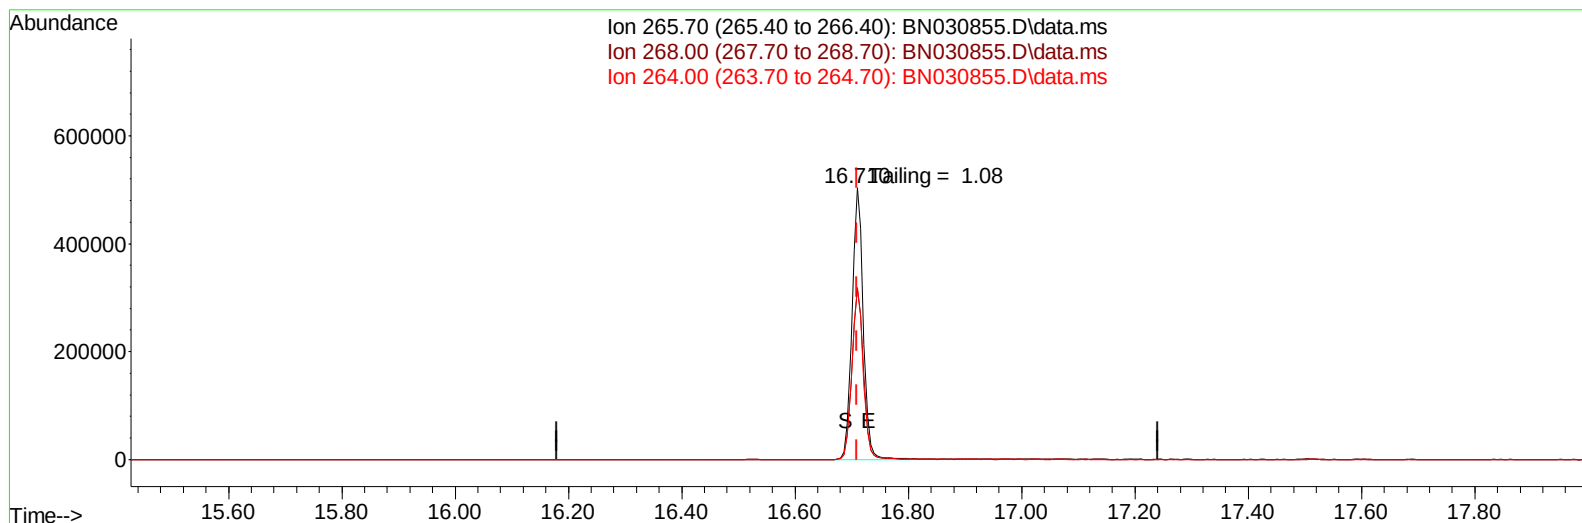

TIC: BN030855.D\data.ms

(70) Pentachlorophenol (C)

16.710min (+ 0.000) 25700.37 ng




response 696839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030855.D
Acq On : 12 Apr 2024 08:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 13 03:39:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 03:37:46 2024
Response via : Initial Calibration

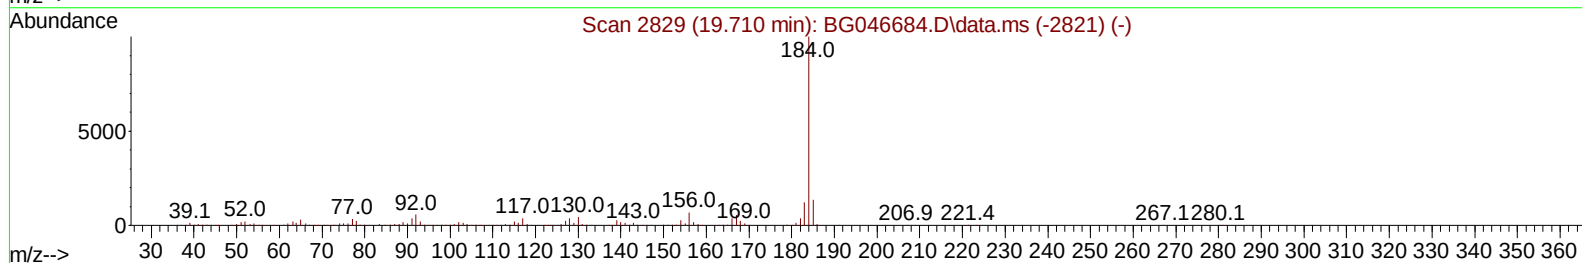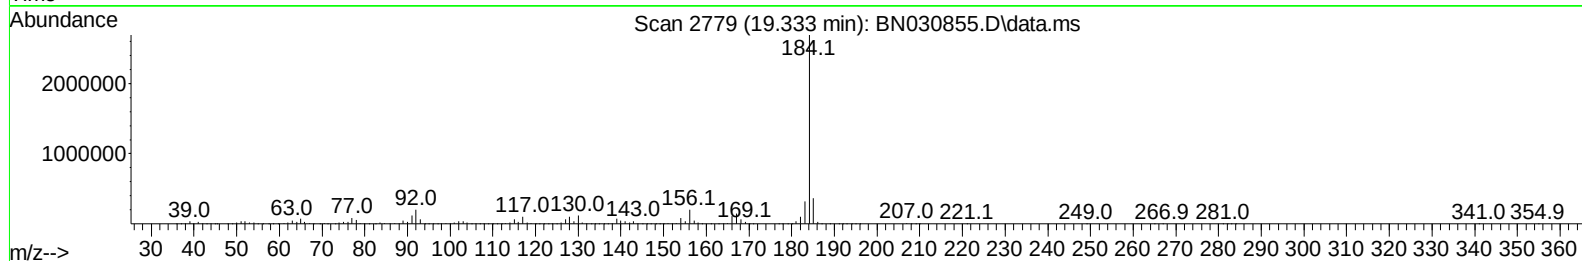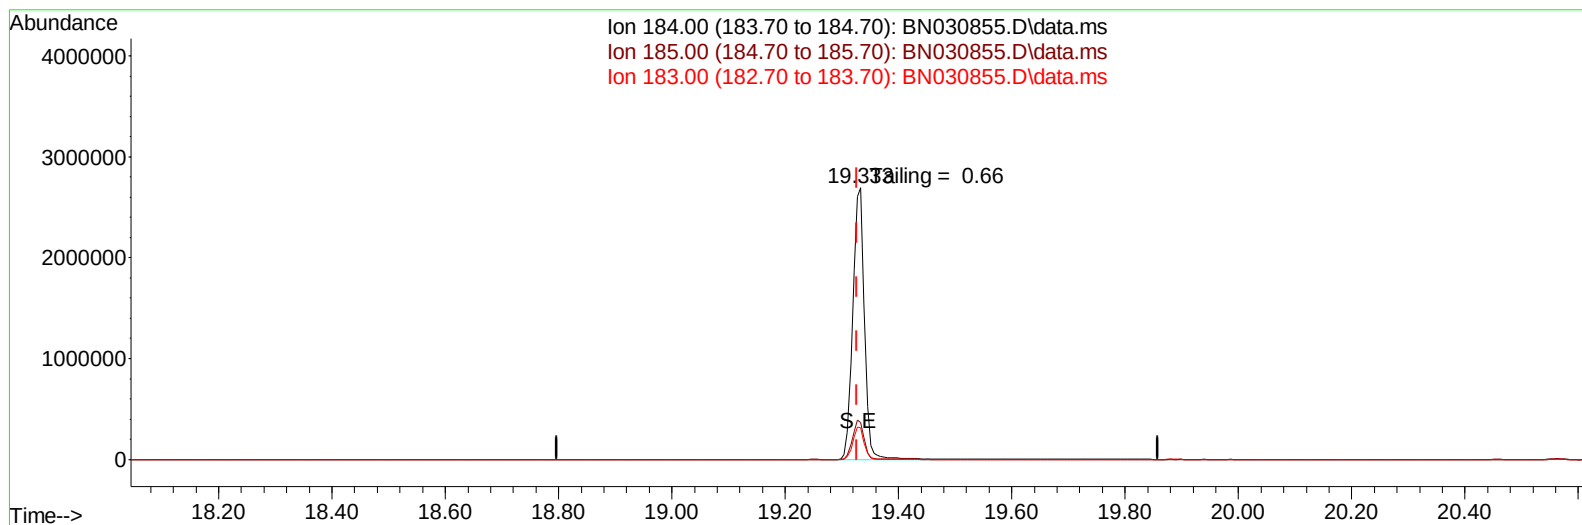

TIC: BN030855.D\data.ms

(77) Benzidine

19.333min (+ 0.006) 0.00 ng

response 3883665

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.60
183.00	13.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2024	BNA_N	<u>BN030855.D</u>
Compound Name	Response	Retention Time
DDT	1946263	20.563
DDD	74294	20.122
DDE	4306	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
78600	2024863	3.88

Instrument :
BNA_N
ClientSampleId :
DFTPP