
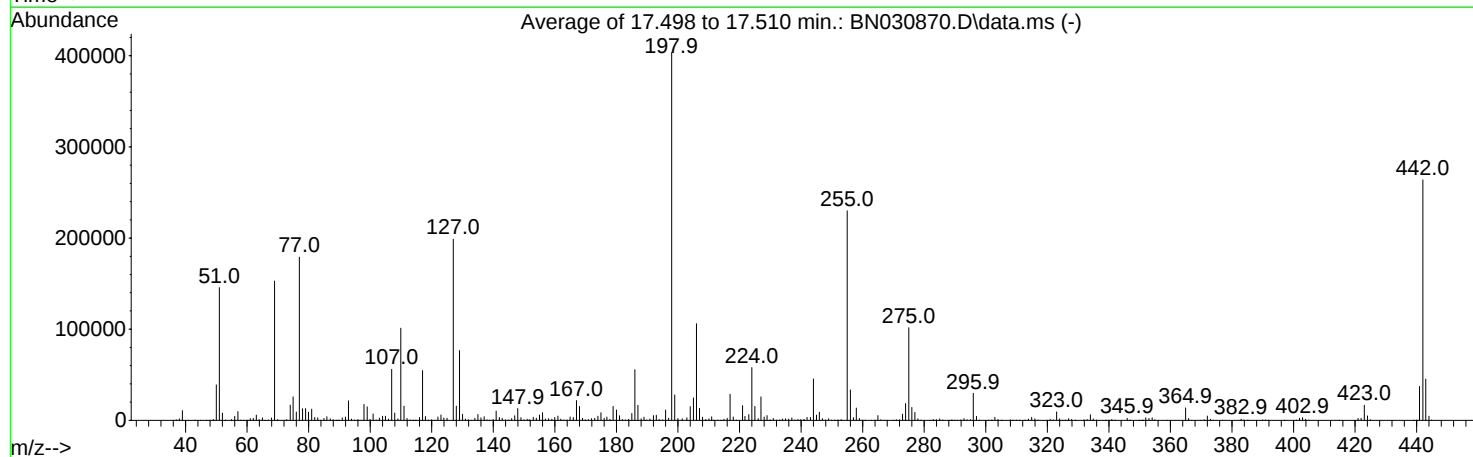


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030870.D
Acq On : 12 Apr 2024 20:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN041224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 12 15:55:57 2024

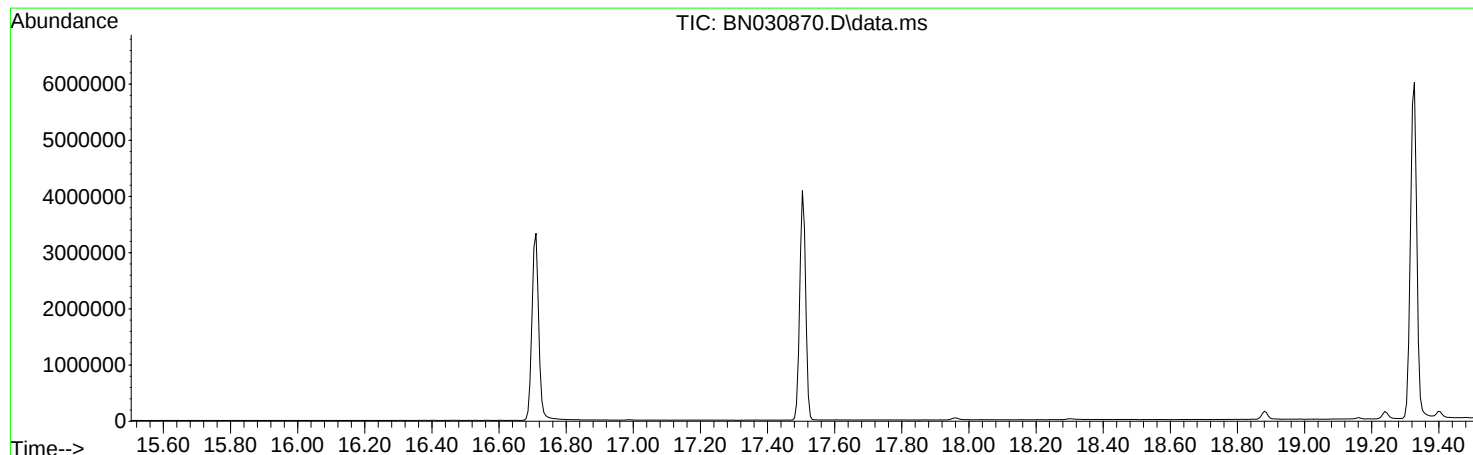




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	145725	PASS
68	69	0.00	2	1.8	2735	PASS
69	198	0.00	100	37.9	152981	PASS
70	69	0.00	2	0.5	818	PASS
127	198	10	80	49.2	198699	PASS
197	198	0.00	2	0.6	2369	PASS
198	198	100	100	100.0	403563	PASS
199	198	5	9	6.9	27859	PASS
275	198	10	60	25.2	101589	PASS
365	198	1	100	3.4	13779	PASS
441	198	0.01	100	9.2	37285	PASS
442	442	50	100	100.0	263851	PASS
443	442	15	24	17.1	45221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030870.D
Acq On : 12 Apr 2024 20:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 13 03:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 03:37:46 2024
Response via : Initial Calibration

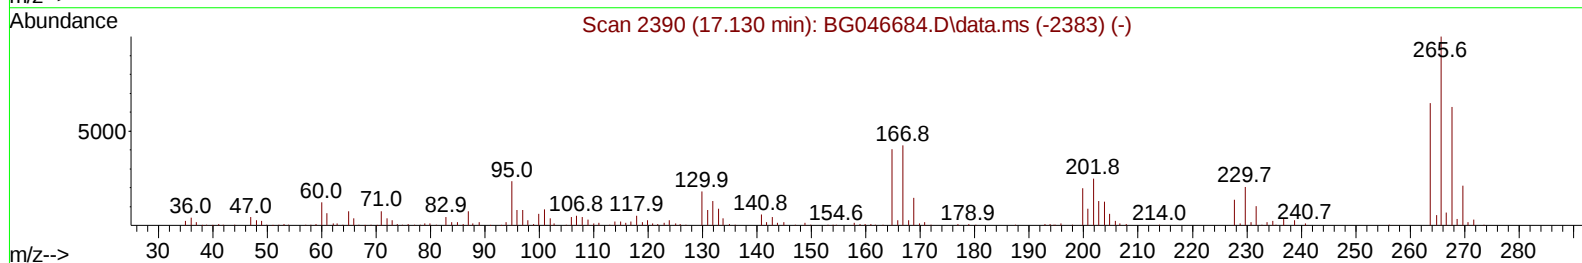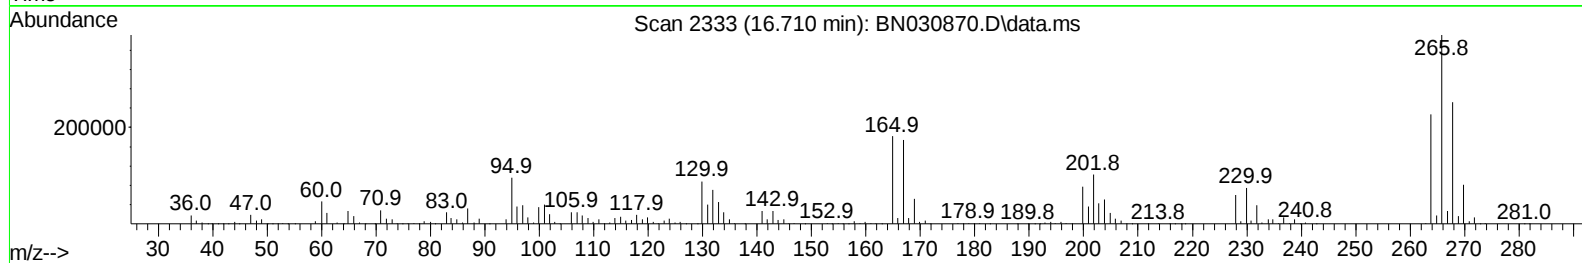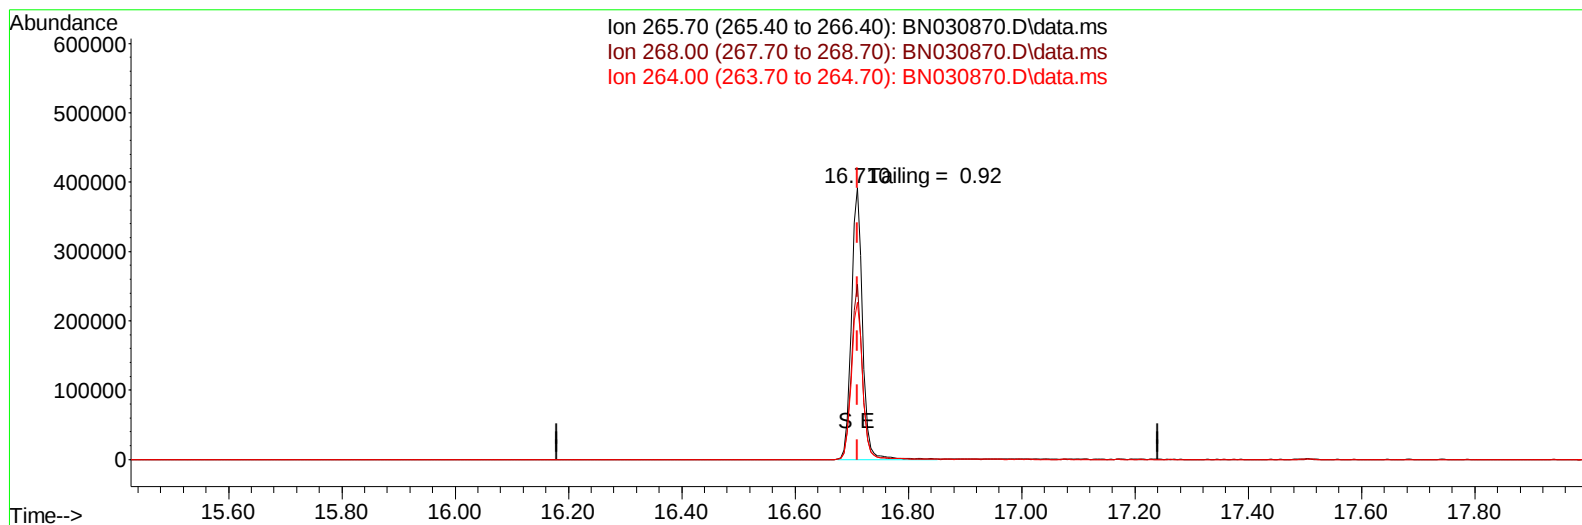

TIC: BN030870.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 25131.91 ng




response 539421

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.55
264.00	61.60	57.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041224\
Data File : BN030870.D
Acq On : 12 Apr 2024 20:17
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 13 03:37:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 13 03:37:46 2024
Response via : Initial Calibration

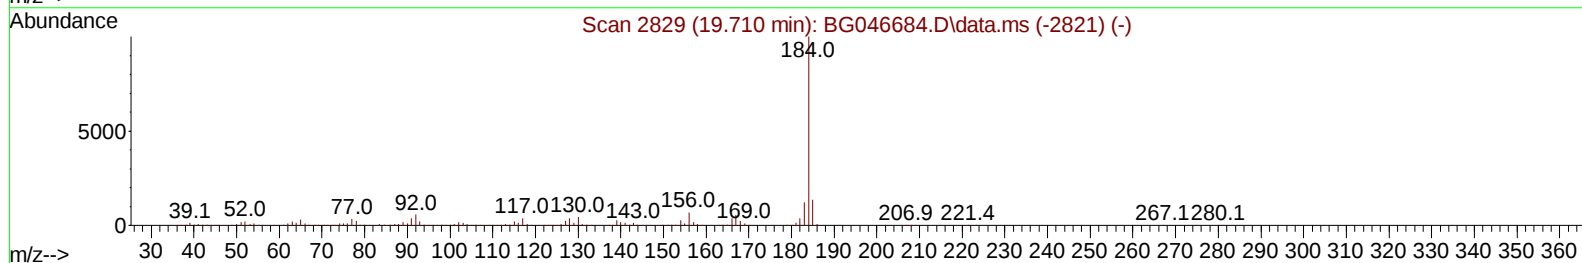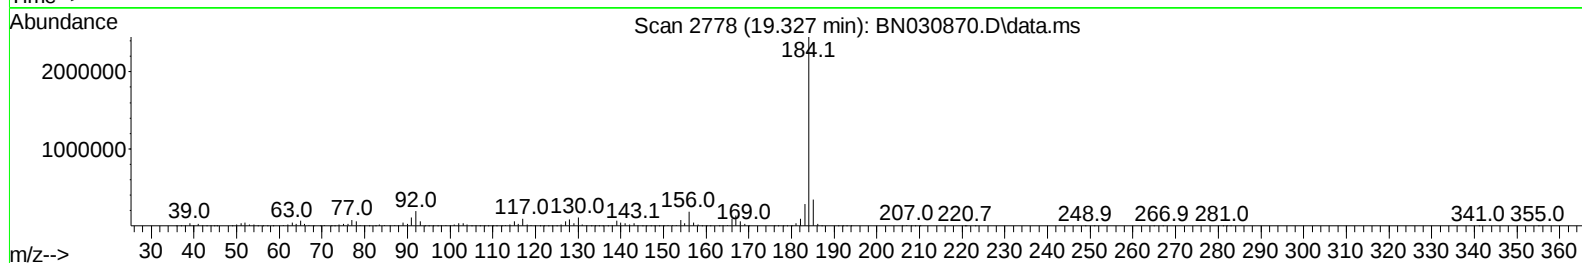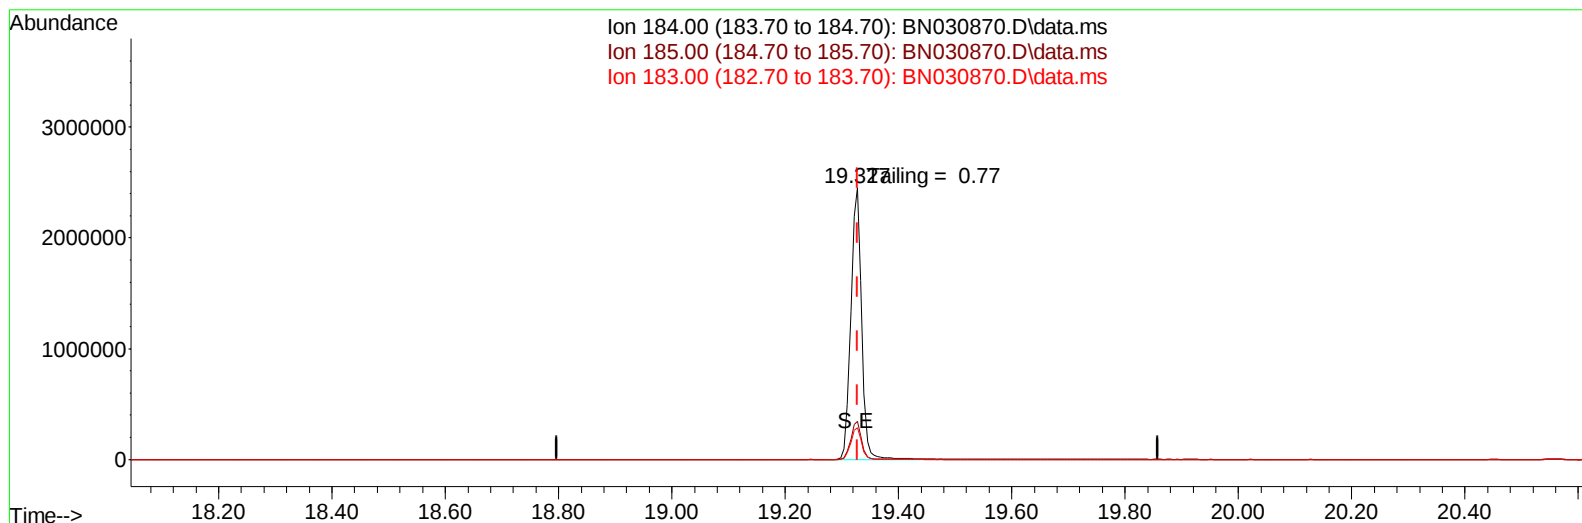

TIC: BN030870.D\data.ms

(77) Benzidine

19.327min (0.000) 0.00 ng

response 3267544

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.95
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/12/2024	BNA_N	<u>BN030870.D</u>
Compound Name	Response	Retention Time
DDT	1636267	20.557
DDD	42428	20.116
DDE	969	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43397	1679664	2.58

Instrument :
BNA_N
ClientSampleId :
DFTPP