


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041320\
 Data File : BN010463.D
 Acq On : 13 Apr 2020 11:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 13 18:04:22 2020

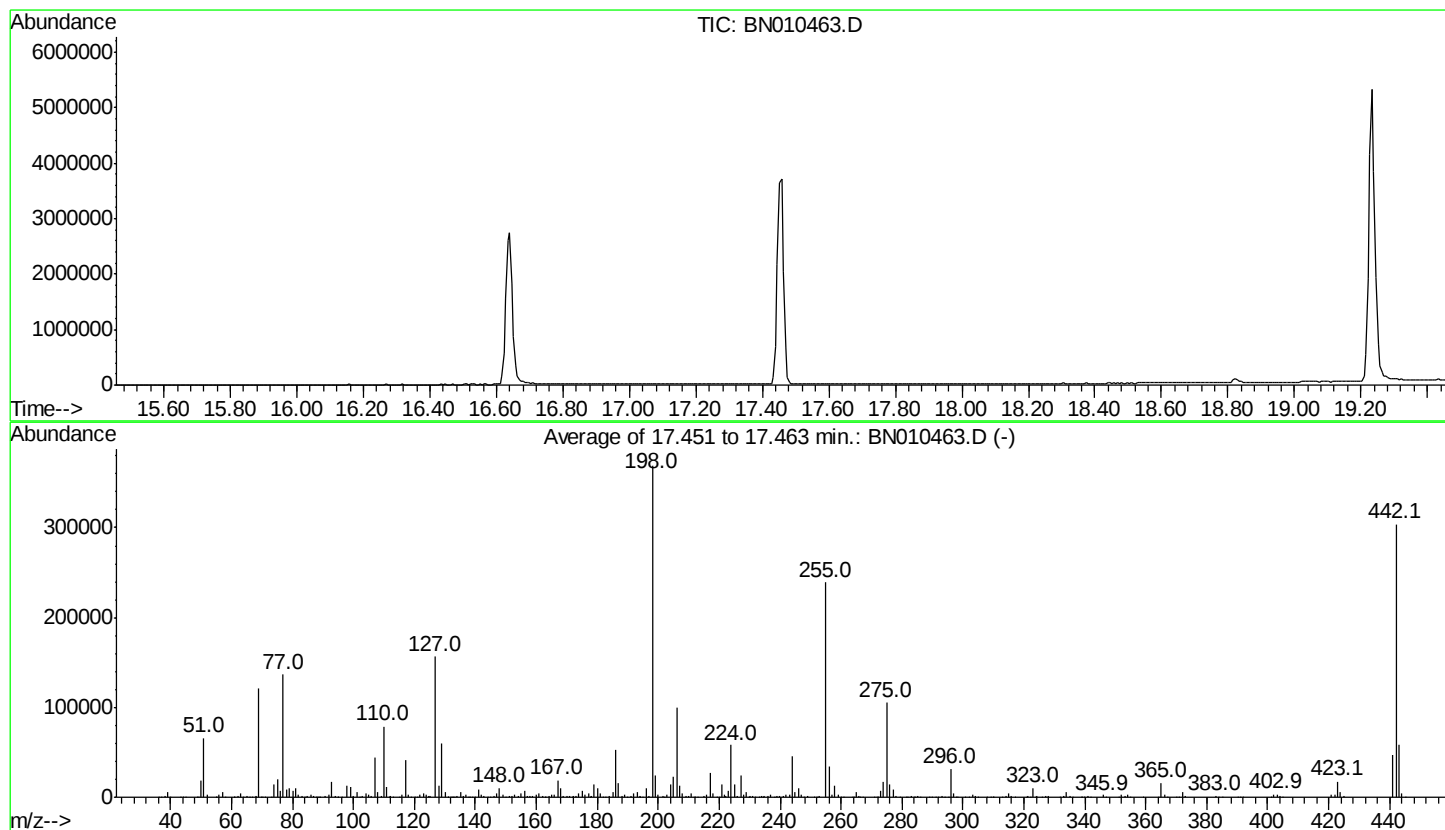

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.9	66077	PASS
68	69	0.00	2	1.8	2155	PASS
69	198	0.00	100	32.9	121314	PASS
70	69	0.00	2	0.5	600	PASS
127	198	10	80	42.4	156536	PASS
197	198	0.00	2	0.2	776	PASS
198	198	100	100	100.0	369109	PASS
199	198	5	9	6.7	24630	PASS
275	198	10	60	28.5	105248	PASS
365	198	1	100	4.4	16065	PASS
441	198	0.01	100	12.8	47154	PASS
442	198	50	100	82.4	304192	PASS
443	442	15	24	19.2	58546	PASS