




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041322\
 Data File : BN019445.D
 Acq On : 13 Apr 2022 17:58
 Operator : CG/JU
 Sample : N2320-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:57:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

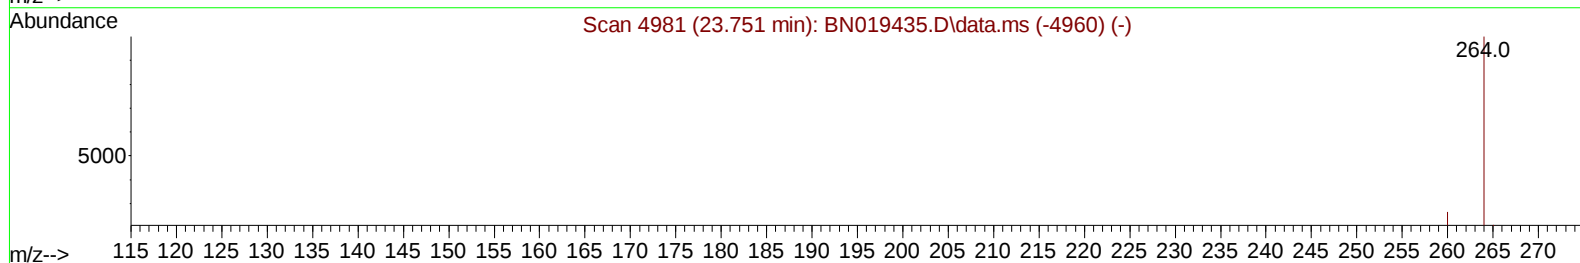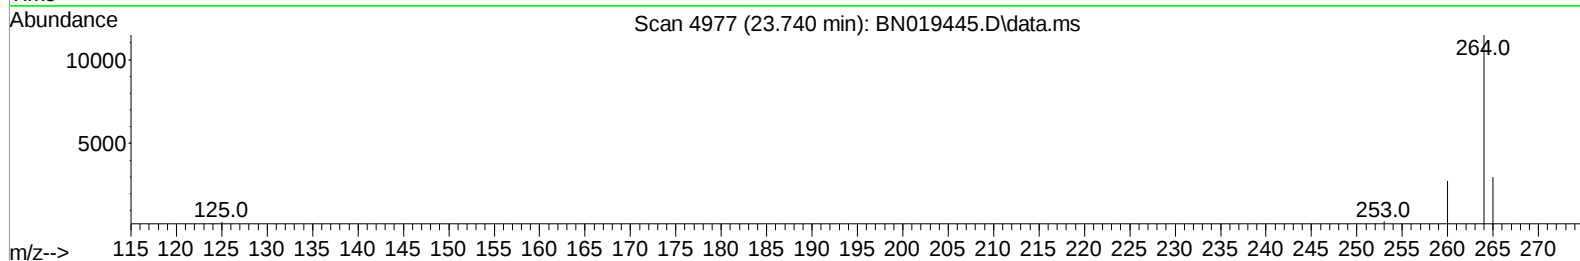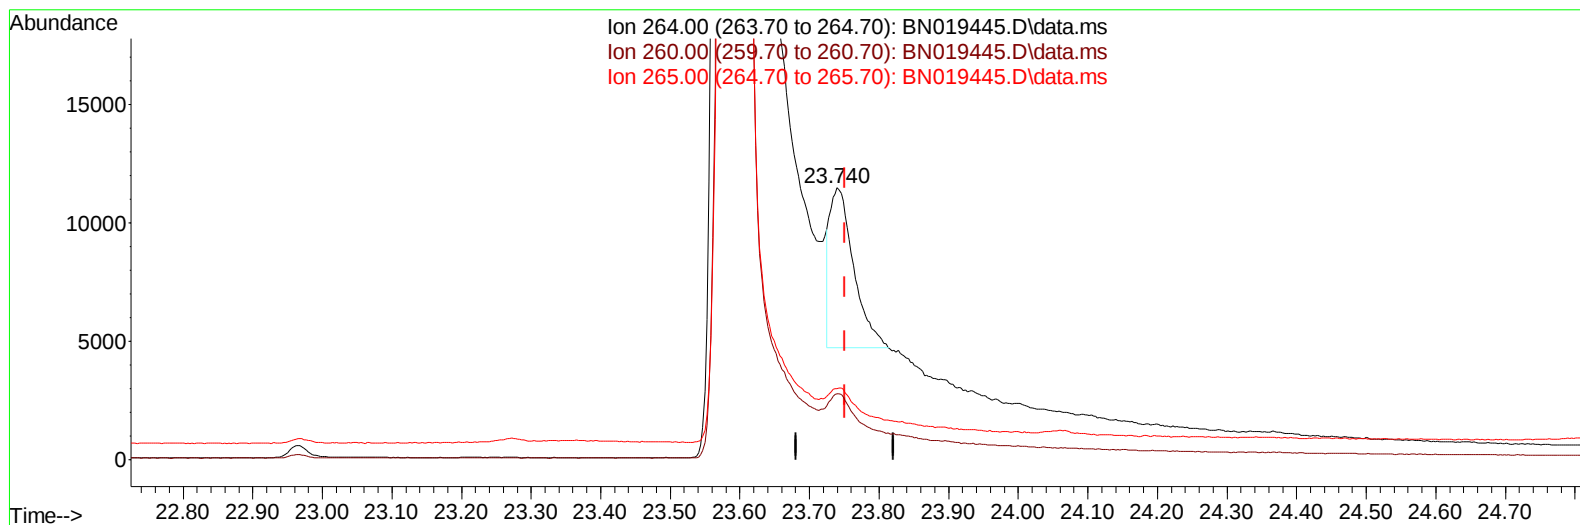

TIC: BN019445.D\data.ms

(23) Perylene-d12 (I)

23.740min (-0.011) 0.40 ng/u1

response 16046

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.11
265.00	45.70	26.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041322\
 Data File : BN019445.D
 Acq On : 13 Apr 2022 17:58
 Operator : CG/JU
 Sample : N2320-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:57:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

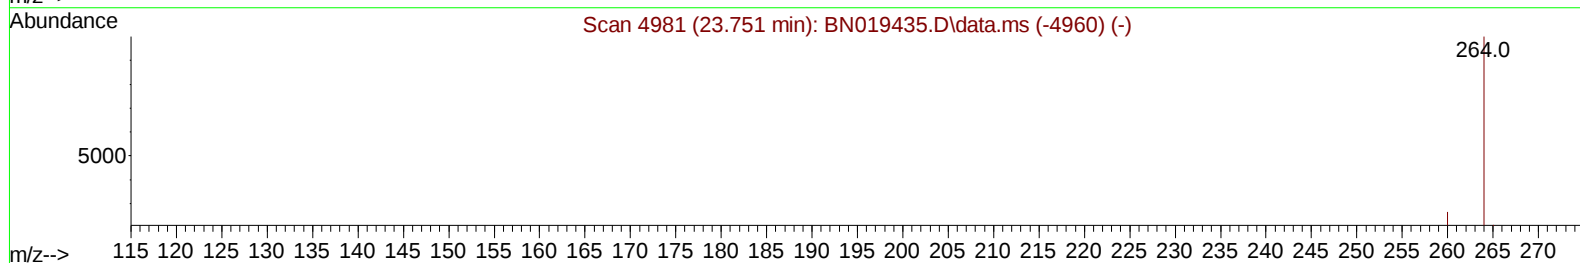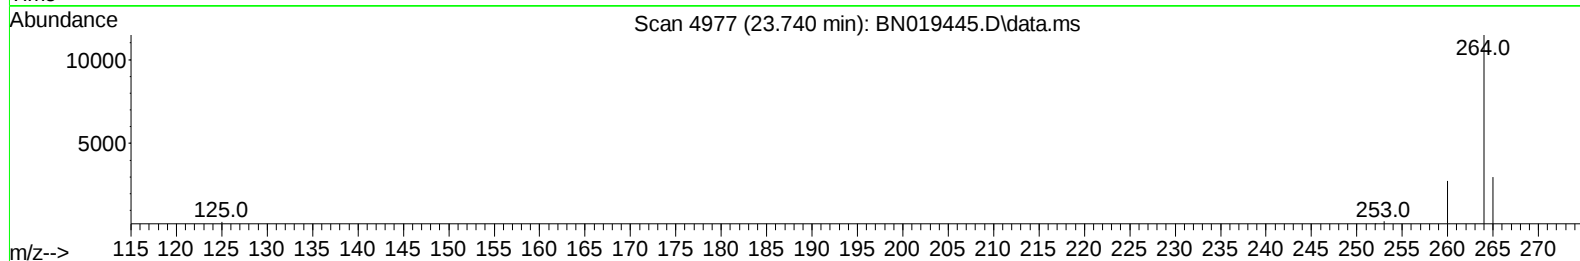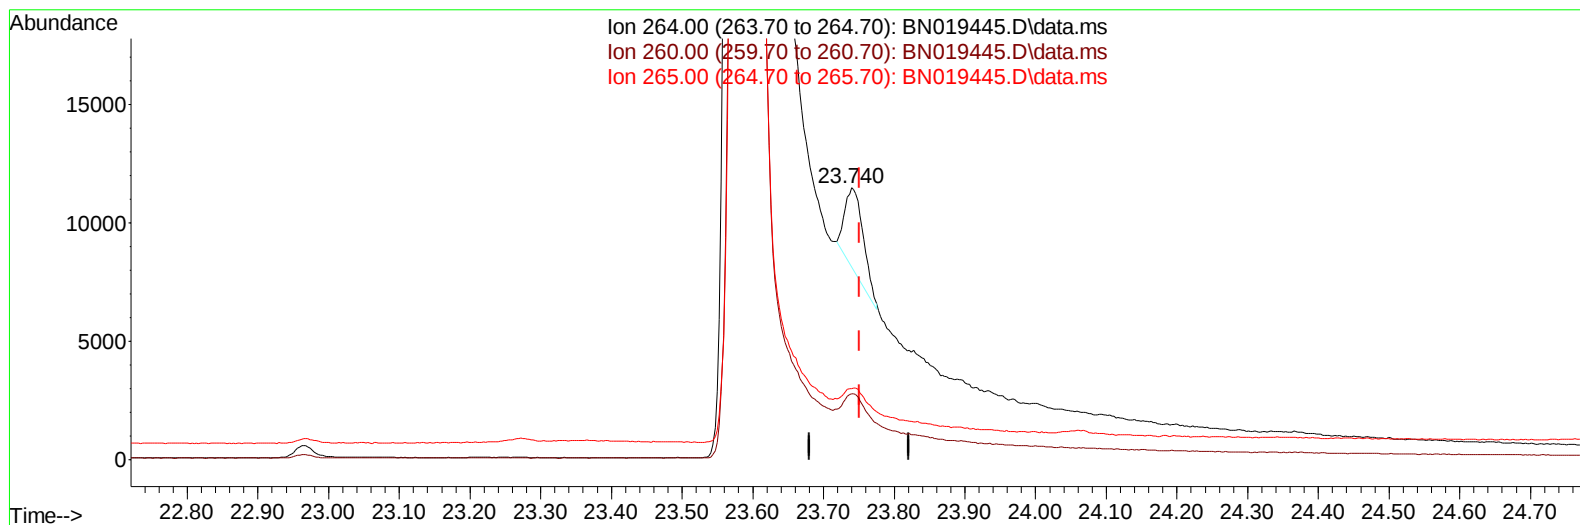

TIC: BN019445.D\data.ms

(23) Perylene-d12 (I)

23.740min (-0.011) 0.40 ng/ul m

response 6019

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	24.11
265.00	45.70	26.05#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041322\
 Data File : BN019445.D
 Acq On : 13 Apr 2022 17:58
 Operator : CG/JU
 Sample : N2320-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB2P7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/14/2022
 Supervised By :Yogesh Patel 04/14/2022

Quant Time: Apr 14 01:57:54 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 13 14:35:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.818	152		4417	0.400	ng/ul	0.00
4) Naphthalene-d8	10.617	136		13721	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.460	164		8950	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.200	188		18653	0.400	ng/ul	0.00
17) Chrysene-d12	21.398	240		12158	0.400	ng/ul	0.00
23) Perylene-d12	23.740	264		6019m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.173	96		26987	4.748	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152		8557	0.441	ng/ul	0.00
18) Fluoranthene-d10	19.234	212		23568	0.523	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041322\
Data File : BN019445.D
Acq On : 13 Apr 2022 17:58
Operator : CG/JU
Sample : N2320-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB2P7

Manual IntegrationsAPPROVED

Quant Time: Apr 14 01:57:54 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN041322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 13 14:35:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/14/2022
Supervised By :Yogesh Patel 04/14/2022

