

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
 Data File : BN024856.D
 Acq On : 13 Apr 2023 11:23
 Operator : CG/JU
 Sample : PB152092BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK092

Quant Time: Apr 14 02:19:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	9343	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	26456	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.589	164	16074	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.339	188	34008	0.400	ng/ul	0.00
17) Chrysene-d12	21.535	240	26596	0.400	ng/ul	0.00
23) Perylene-d12	23.976	264	31338	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	62568	6.133	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	12105	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.364	212	29384	0.445	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.584	166	4783	0.083	ng/ul#	11
20) Pyrene	19.731	202	4572	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.821	252	11186	0.107	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
Data File : BN024856.D
Acq On : 13 Apr 2023 11:23
Operator : CG/JU
Sample : PB152092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Time: Apr 14 02:19:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration




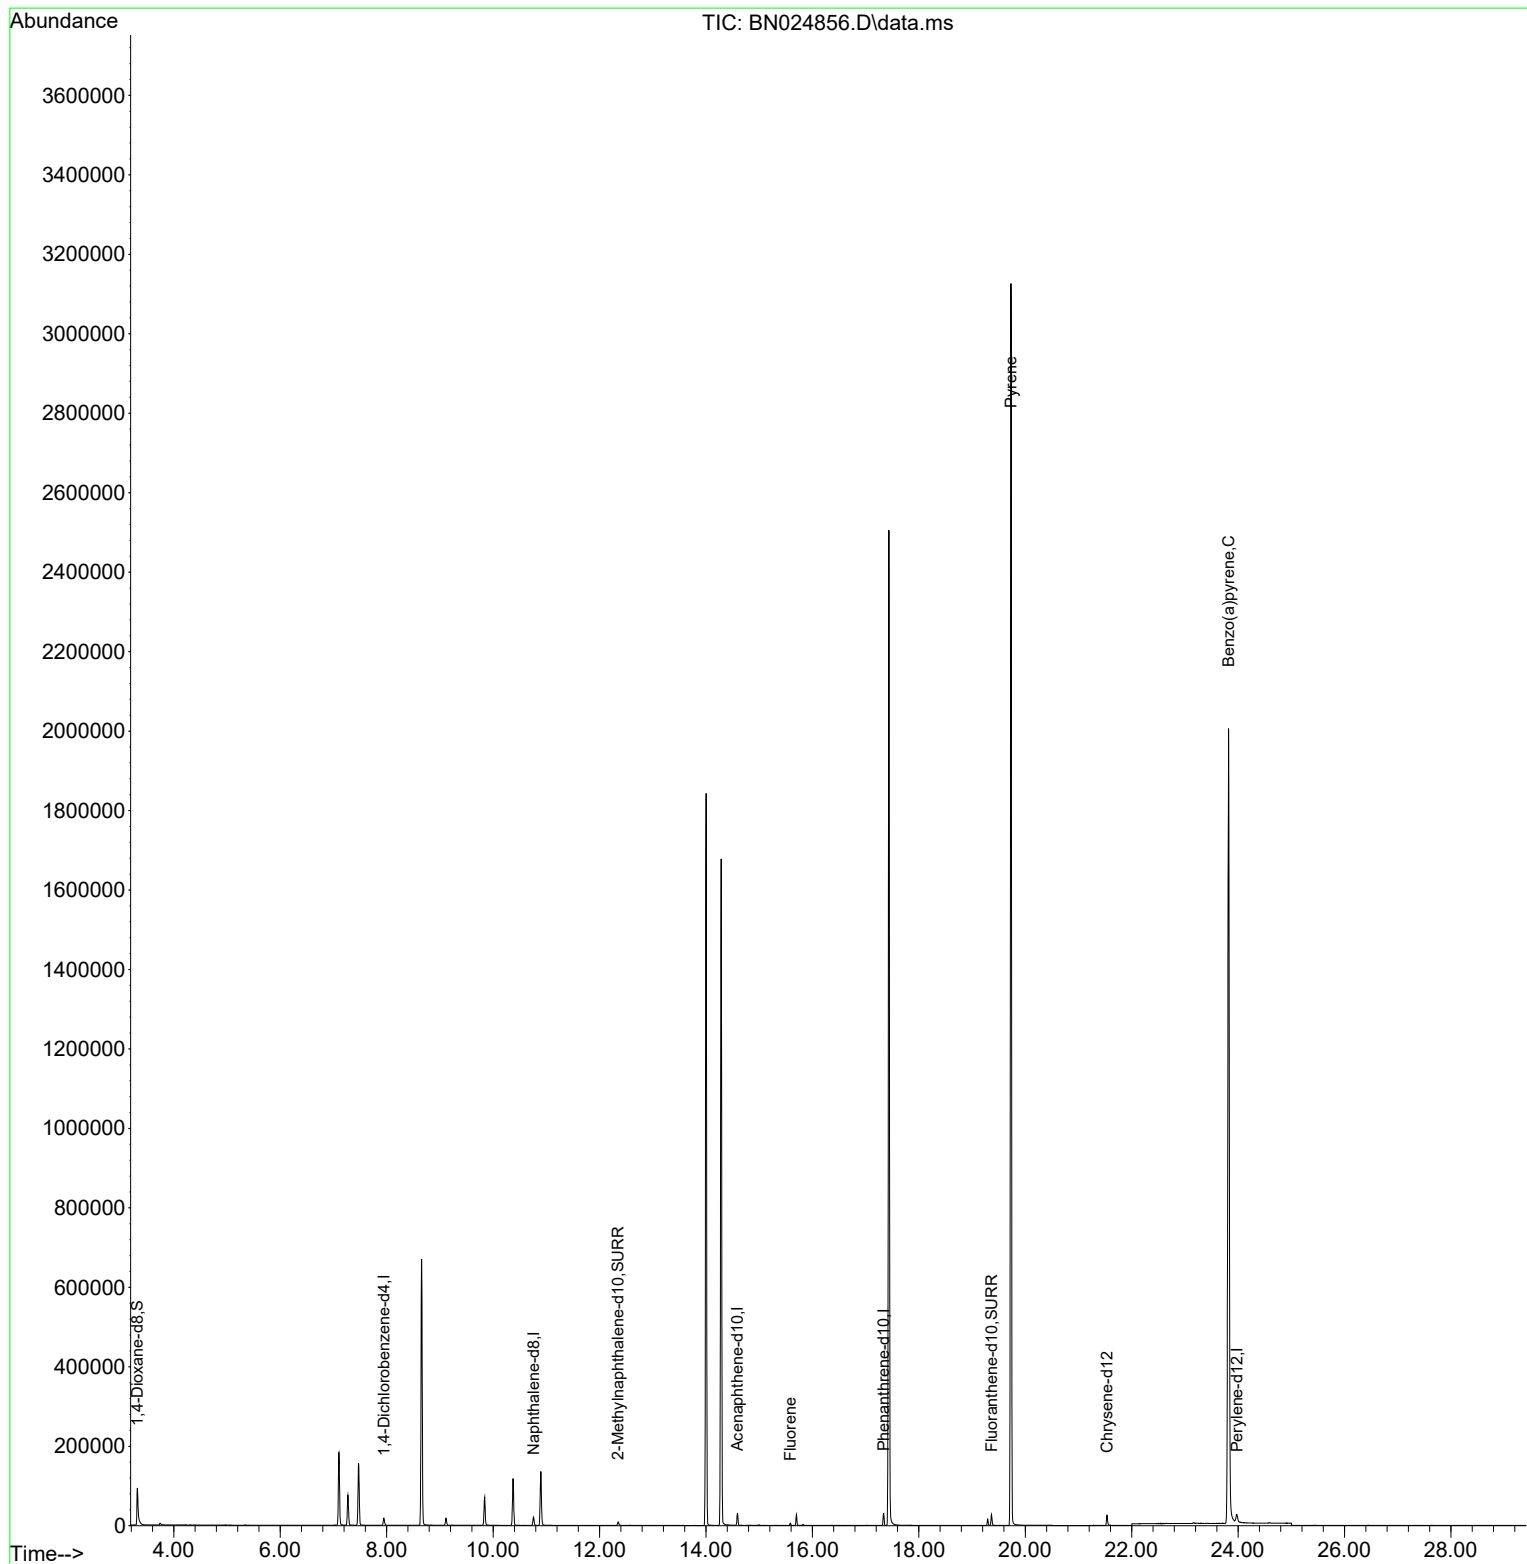


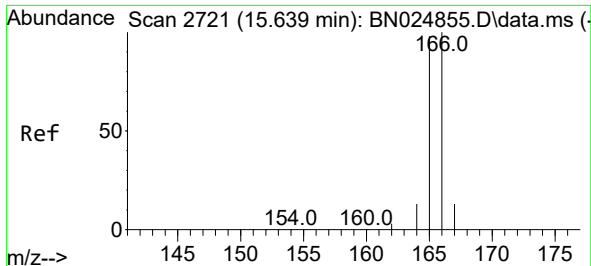

#12
Fluorene
Concen: 0.083 ng/ul
RT: 15.584 min Scan# 21
Delta R.T. -0.054 min
Lab File: BN024856.D
Acq: 13 Apr 2023 11:23




Instrument :
BNA_N
ClientSampleId :
SBLK092


Tgt Ion:166 Resp: 4783
Ion Ratio Lower Upper
166 100
165 6.3 80.1 120.1#
167 34.9 10.7 16.1#

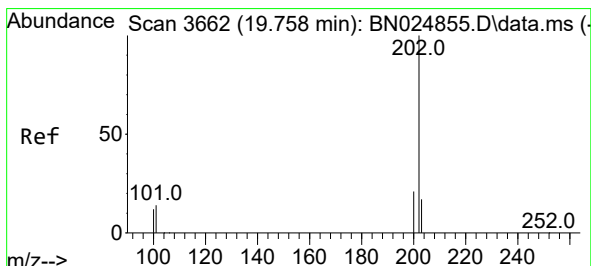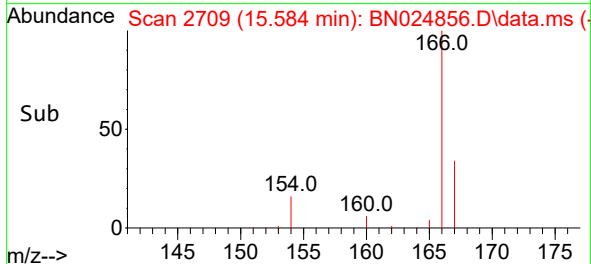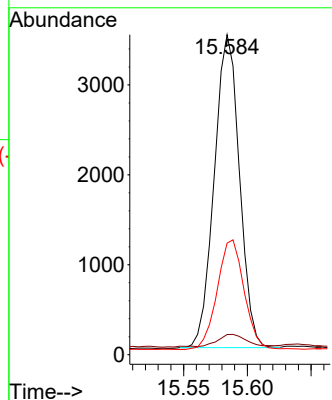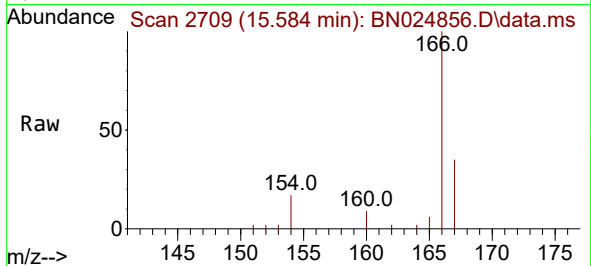

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.731 min Scan# 3656
Delta R.T. -0.031 min
Lab File: BN024856.D
Acq: 13 Apr 2023 11:23


Tgt Ion:202 Resp: 4572
Ion Ratio Lower Upper
202 100
101 184.5 11.8 17.8#
100 1400.5 9.5 14.3#

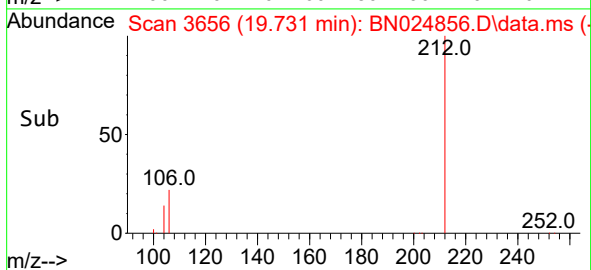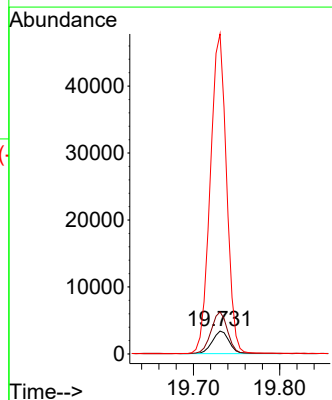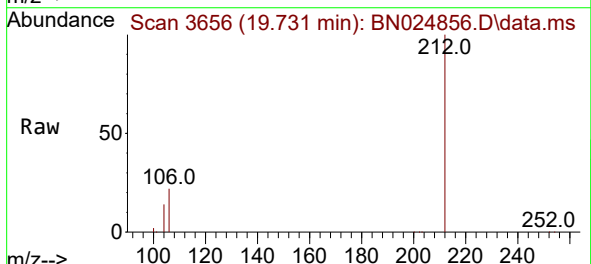

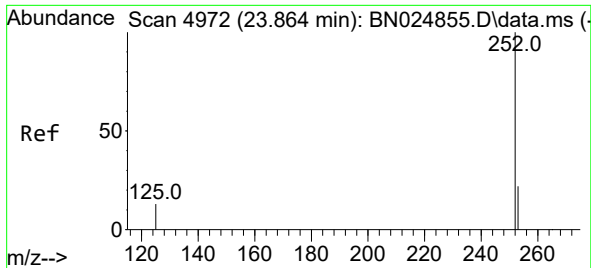

#26
Benzo(a)pyrene
Concen: 0.107 ng/ul
RT: 23.821 min Scan# 4957
Delta R.T. -0.048 min
Lab File: BN024856.D
Acq: 13 Apr 2023 11:23

Instrument :
BNA_N
ClientSampleId :
SBLK092

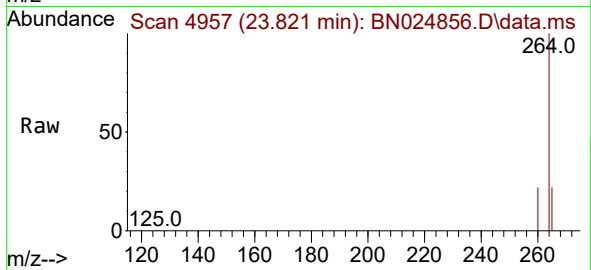

Tgt Ion:252 Resp: 11186
Ion Ratio Lower Upper
252 100
253 40.4 20.7 31.1#
125 36.8 15.9 23.9#

