

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
 Data File : BN024864.D
 Acq On : 13 Apr 2023 17:10
 Operator : CG/JU
 Sample : PB152109BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK109

Quant Time: Apr 14 02:20:54 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	8313	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	24980	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.593	164	14750	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.338	188	31420	0.400	ng/ul	0.00
17) Chrysene-d12	21.532	240	24769	0.400	ng/ul	0.00
23) Perylene-d12	23.987	264	26244	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	58877	6.486	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.348	152	12434	0.388	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	29150	0.474	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.730	202	4362	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.835	252	10502	0.120	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
Data File : BN024864.D
Acq On : 13 Apr 2023 17:10
Operator : CG/JU
Sample : PB152109BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK109

Quant Time: Apr 14 02:20:54 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

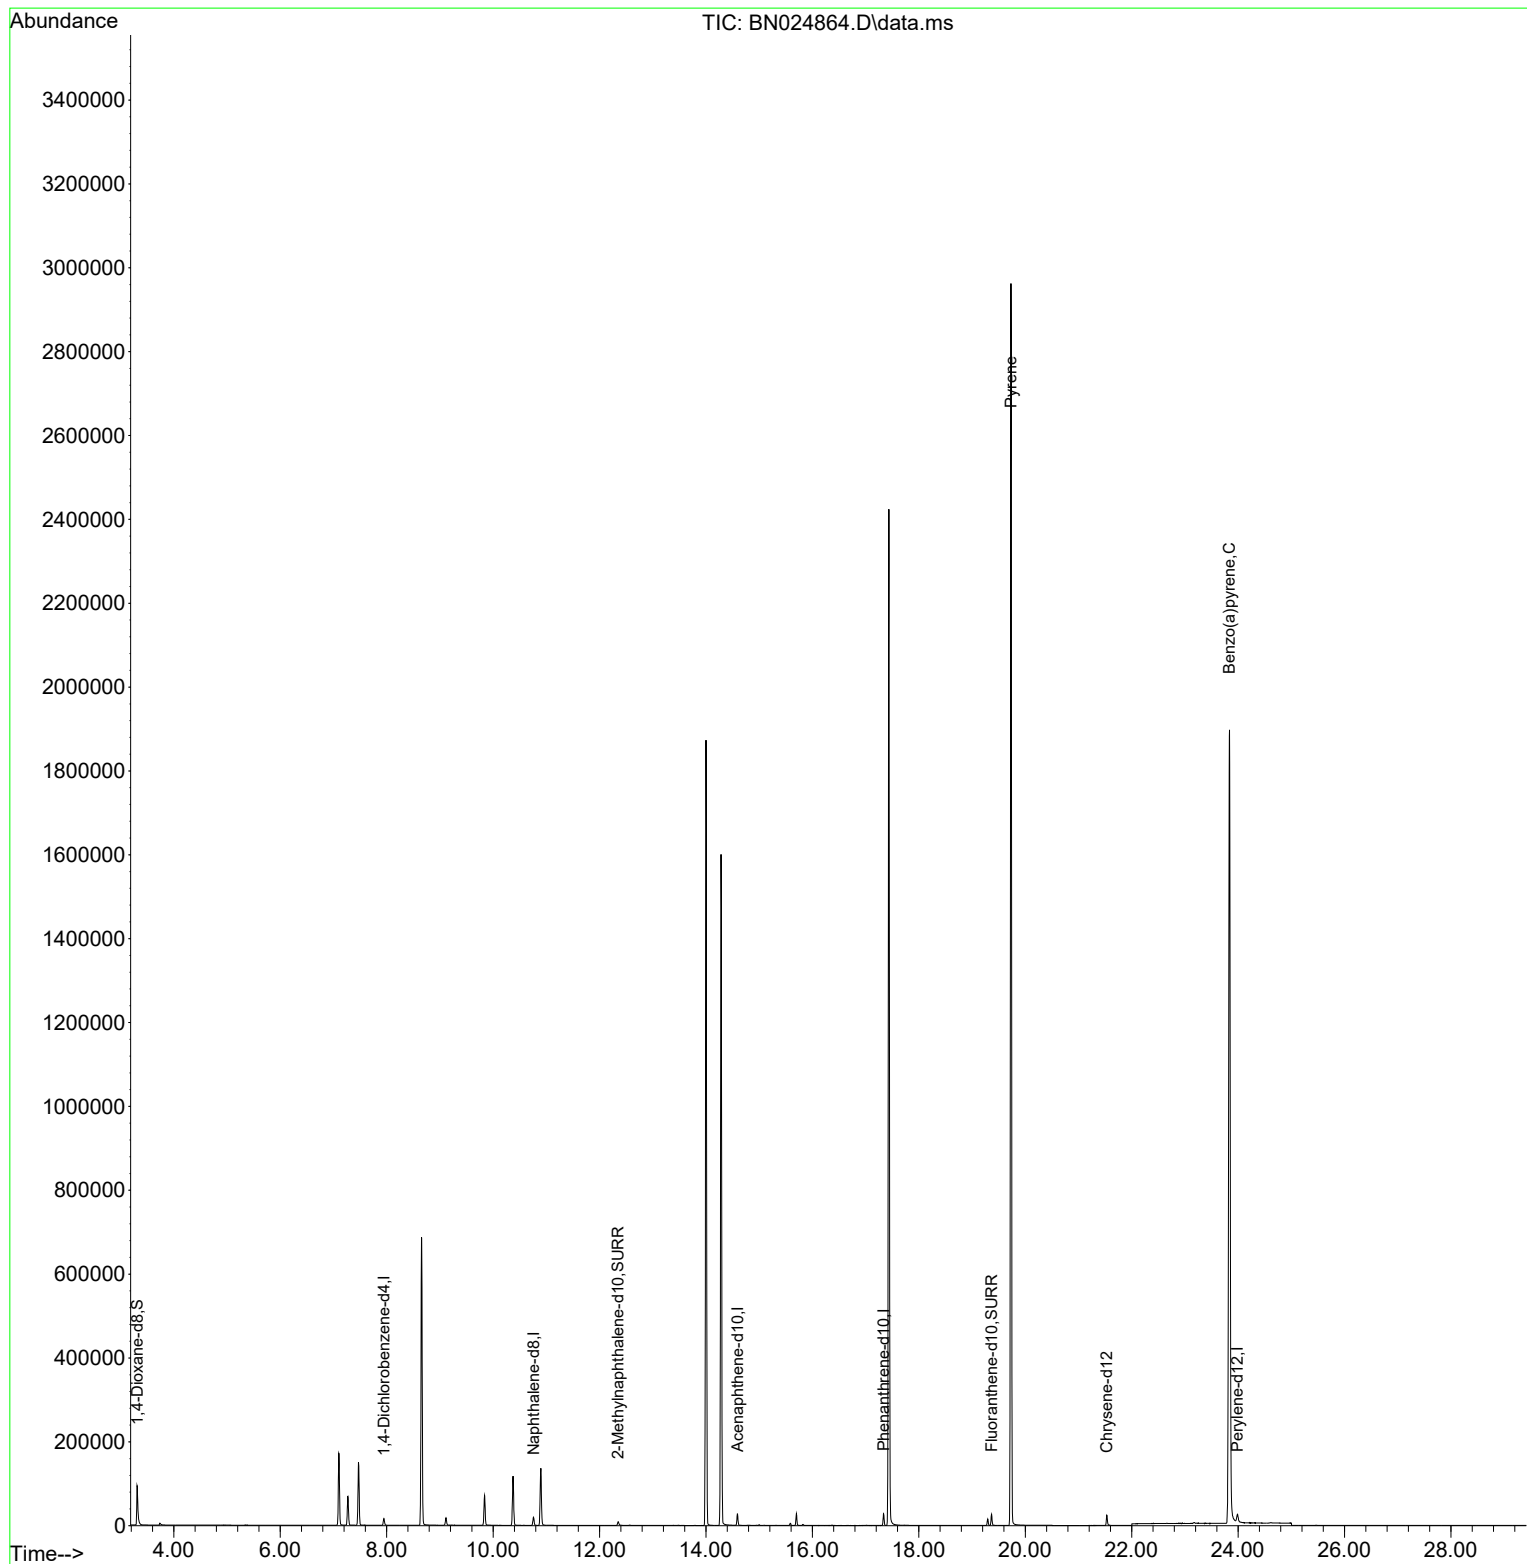

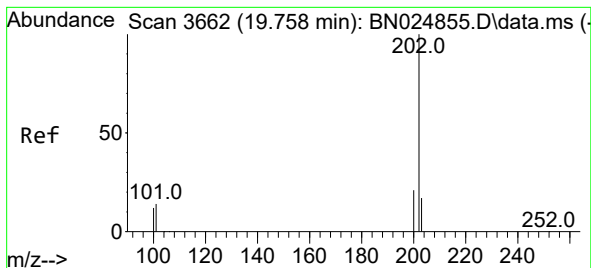

#20

Pyrene

Concen: 0.050 ng/ul

RT: 19.730 min Scan# 3

Delta R.T. -0.032 min

Lab File: BN024864.D

Acq: 13 Apr 2023 17:10

Instrument :

BNA_N

ClientSampleId :

SBLK109





Tgt Ion:202 Resp: 4362

Ion Ratio Lower Upper

202 100

101 182.5 11.8 17.8#

100 1382.0 9.5 14.3#

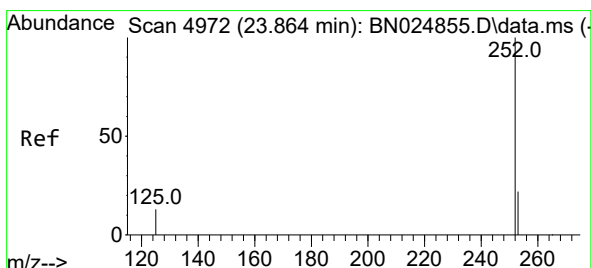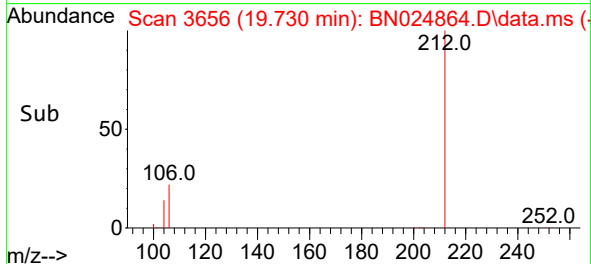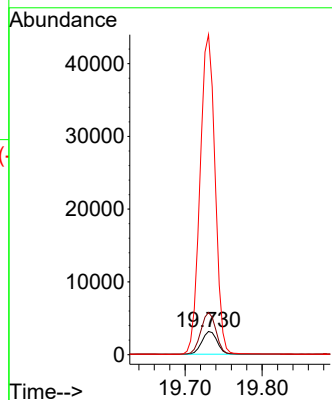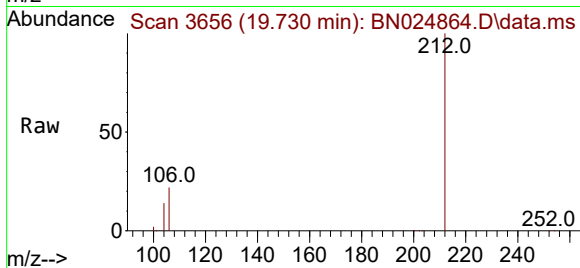

#26

Benzo(a)pyrene

Concen: 0.120 ng/ul

RT: 23.835 min Scan# 4962

Delta R.T. -0.034 min

Lab File: BN024864.D

Acq: 13 Apr 2023 17:10

Tgt Ion:252 Resp: 10502

Ion Ratio Lower Upper

252 100

253 41.4 20.7 31.1#

125 36.0 15.9 23.9#

