

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
 Data File : BN024868.D
 Acq On : 13 Apr 2023 19:41
 Operator : CG/JU
 Sample : 02275-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ7

Quant Time: Apr 14 02:21:22 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7266	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	22196	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.593	164	13070	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.339	188	28358	0.400	ng/ul	0.00
17) Chrysene-d12	21.532	240	23522	0.400	ng/ul	0.00
23) Perylene-d12	23.987	264	25087	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	45840	5.777	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	11991	0.421	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	31500	0.539	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	784	0.090	ng/ul#	66
20) Pyrene	19.731	202	4608	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.835	252	10971	0.131	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
Data File : BN024868.D
Acq On : 13 Apr 2023 19:41
Operator : CG/JU
Sample : 02275-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ7

Quant Time: Apr 14 02:21:22 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration




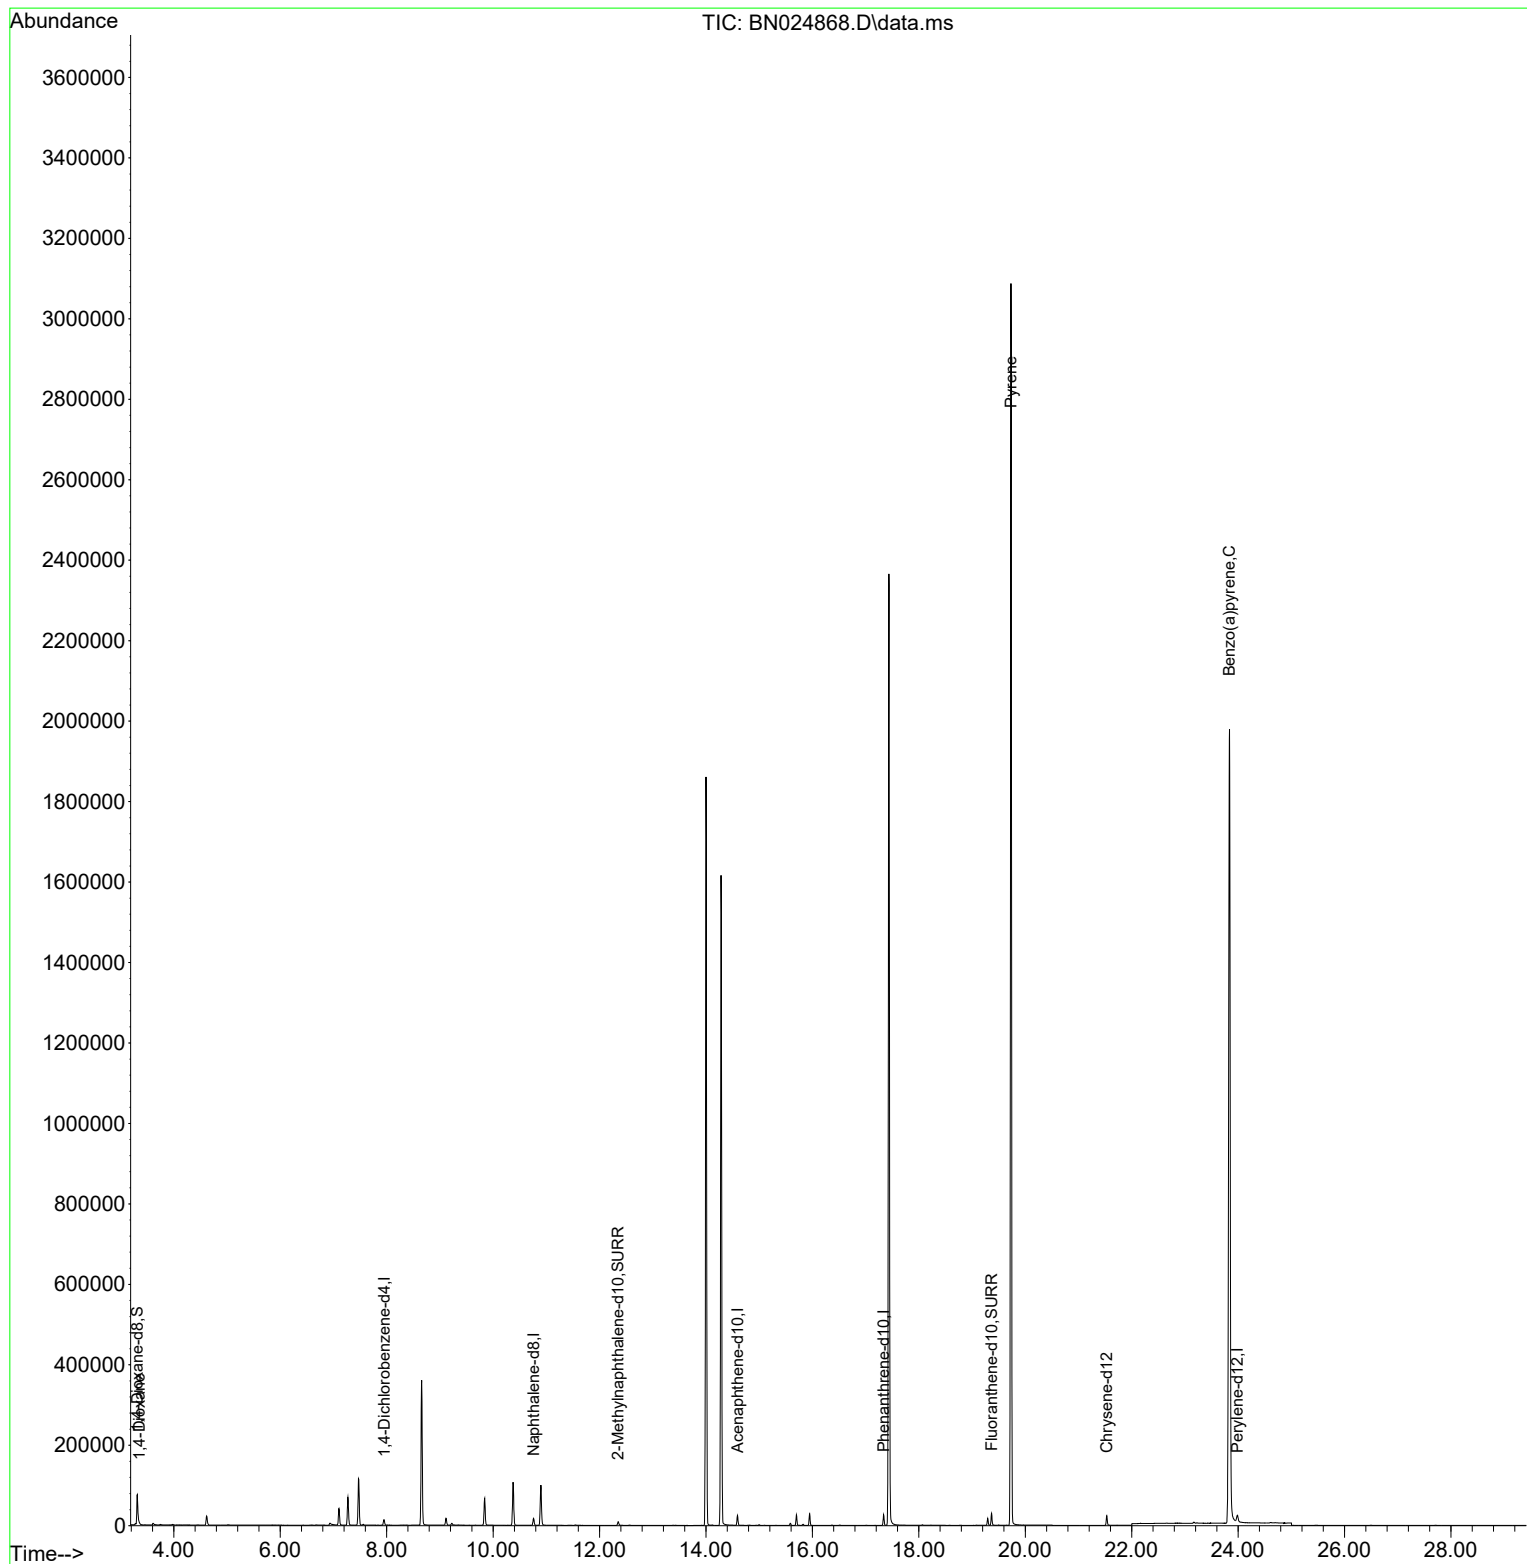


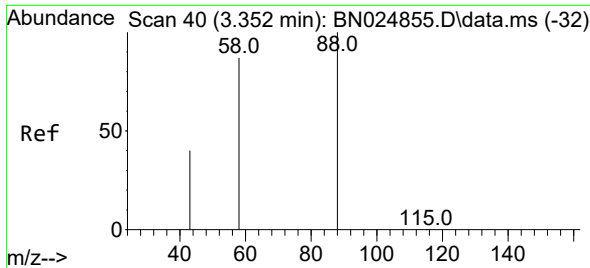

#2
 1,4-Dioxane
 Concen: 0.090 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN024868.D
 Acq: 13 Apr 2023 19:41




Instrument :
 BNA_N
 ClientSampleId :
 BHDZ7


Tgt Ion: 88 Resp: 784
 Ion Ratio Lower Upper
 88 100
 43 85.9 39.1 58.7#
 58 61.8 65.7 98.5#

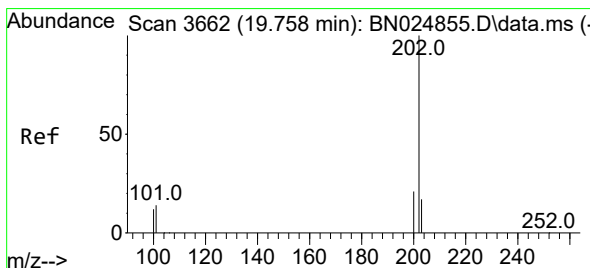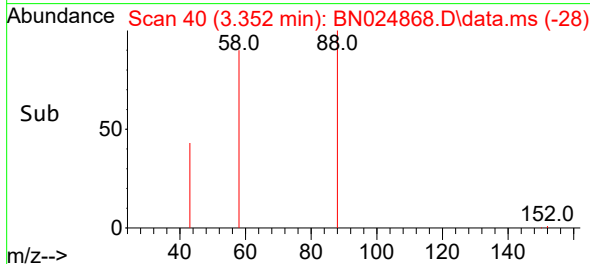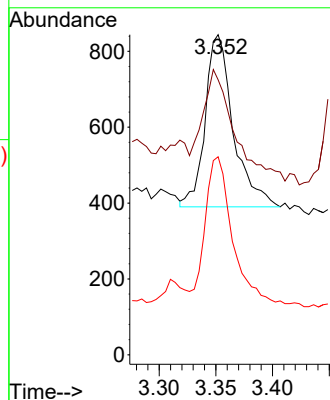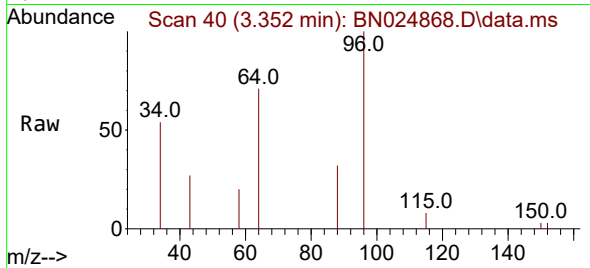

#20
 Pyrene
 Concen: 0.056 ng/ul
 RT: 19.731 min Scan# 3656
 Delta R.T. -0.031 min
 Lab File: BN024868.D
 Acq: 13 Apr 2023 19:41


Tgt Ion: 202 Resp: 4608
 Ion Ratio Lower Upper
 202 100
 101 183.6 11.8 17.8#
 100 1393.4 9.5 14.3#

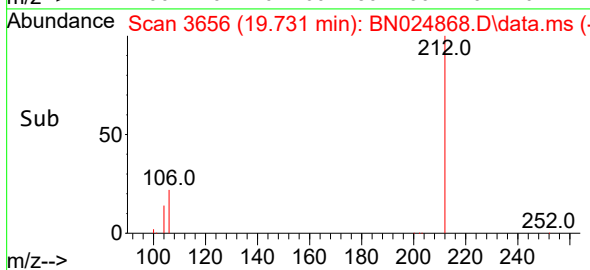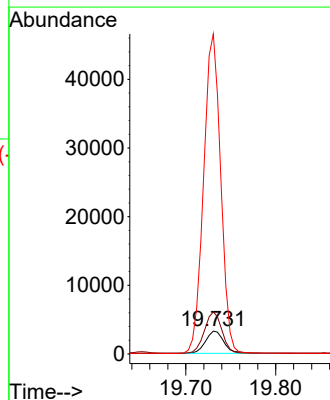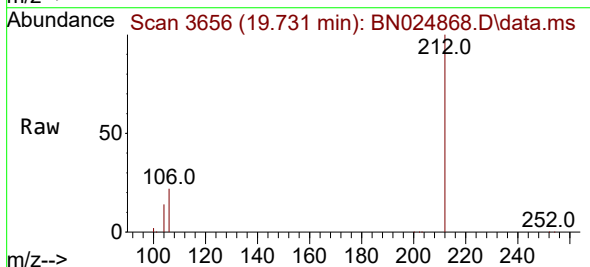

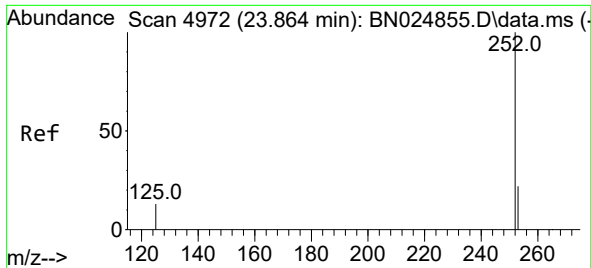

#26
Benzo(a)pyrene
Concen: 0.131 ng/ul
RT: 23.835 min Scan# 4962
Delta R.T. -0.034 min
Lab File: BN024868.D
Acq: 13 Apr 2023 19:41

Instrument :
BNA_N
ClientSampleId :
BHDZ7

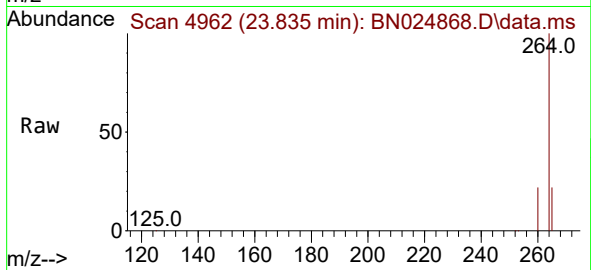

Tgt Ion:252 Resp: 10971
Ion Ratio Lower Upper
252 100
253 43.2 20.7 31.1#
125 37.4 15.9 23.9#

