

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
 Data File : BN024865.D
 Acq On : 13 Apr 2023 17:48
 Operator : CG/JU
 Sample : 02275-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ3

Quant Time: Apr 14 02:21:00 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	8328	0.400	ng/u1	0.00
4) Naphthalene-d8	10.759	136	25390	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.593	164	14681	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.338	188	33315	0.400	ng/u1	0.00
17) Chrysene-d12	21.528	240	28702	0.400	ng/u1	0.00
23) Perylene-d12	23.975	264	29516	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	54100	5.949	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.348	152	10598	0.325	ng/u1	0.00
18) Fluoranthene-d10	19.367	212	30971	0.434	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	14129	1.410	ng/u1	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\  
Data File : BN024865.D  
Acq On    : 13 Apr 2023   17:48  
Operator  : CG/JU  
Sample    : 02275-07  
Misc      :  
ALS Vial  : 11    Sample Multiplier: 1
```


Quant Time: Apr 14 02:21:00 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

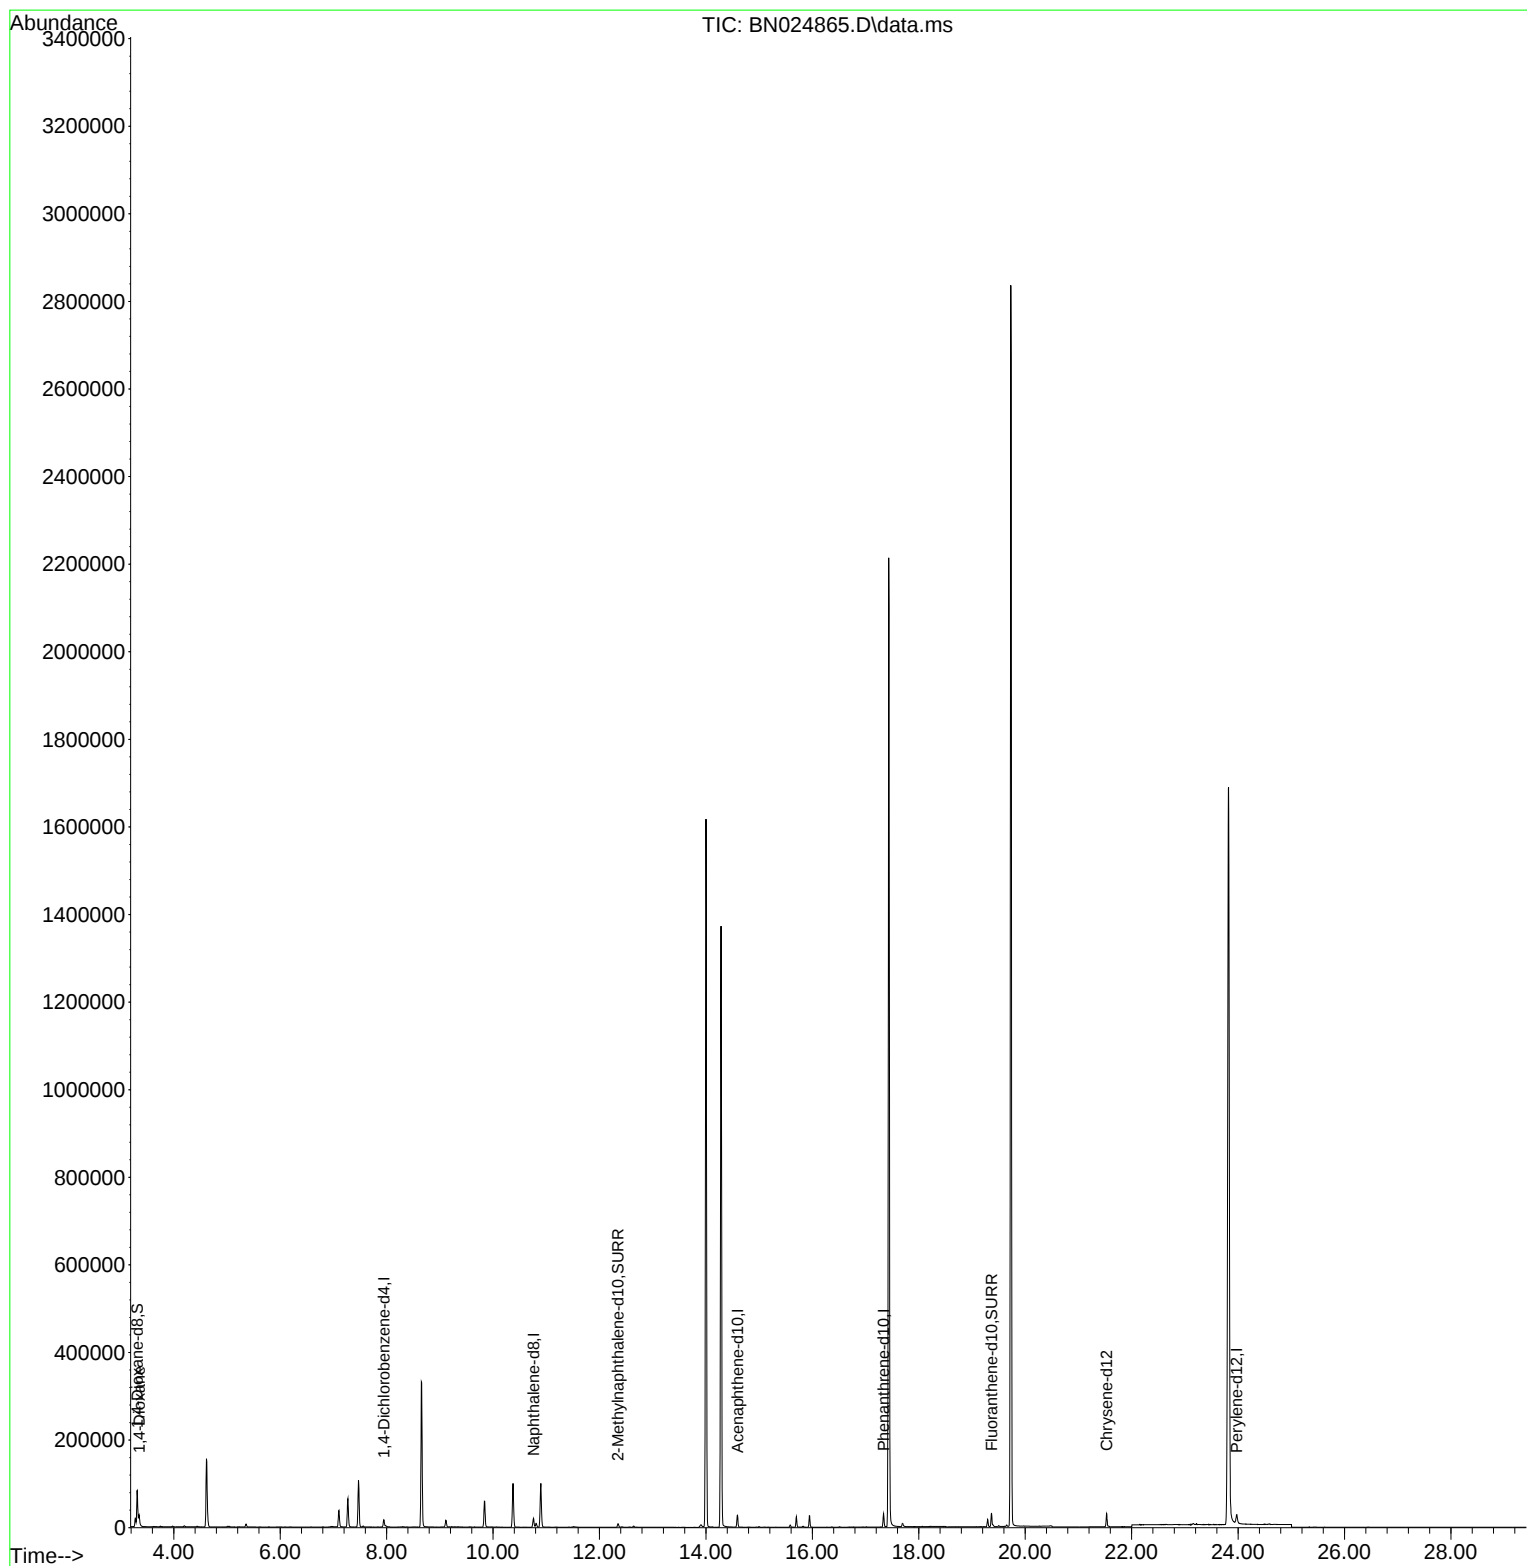

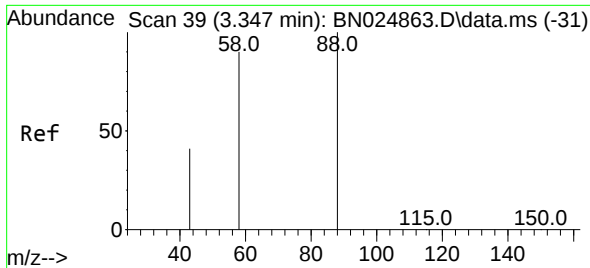

#2
 1,4-Dioxane
 Concen: 1.410 ng/ul
 RT: 3.352 min Scan# 40
 Delta R.T. 0.000 min
 Lab File: BN024865.D
 Acq: 13 Apr 2023 17:48

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ3

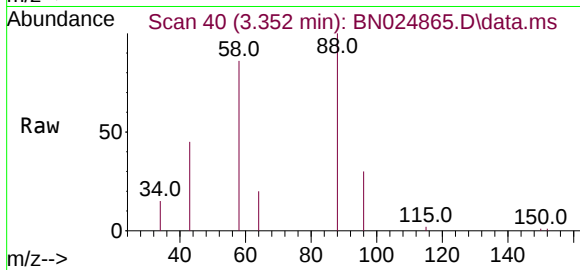

Tgt Ion: 88 Resp: 14129

Ion	Ratio	Lower	Upper
88	100		
43	44.9	39.1	58.7
58	85.9	65.7	98.5

