

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
 Data File : BN024868.D
 Acq On : 13 Apr 2023 19:41
 Operator : CG/JU
 Sample : 02275-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ7

Quant Time: Apr 14 02:21:22 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	7266	0.400	ng/ul	0.00
4) Naphthalene-d8	10.759	136	22196	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.593	164	13070	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.339	188	28358	0.400	ng/ul	0.00
17) Chrysene-d12	21.532	240	23522	0.400	ng/ul	0.00
23) Perylene-d12	23.987	264	25087	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	45840	5.777	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.349	152	11991	0.421	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	31500	0.539	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	784	0.090	ng/ul#	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
Data File : BN024868.D
Acq On : 13 Apr 2023 19:41
Operator : CG/JU
Sample : 02275-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHDZ7

Quant Time: Apr 14 02:21:22 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

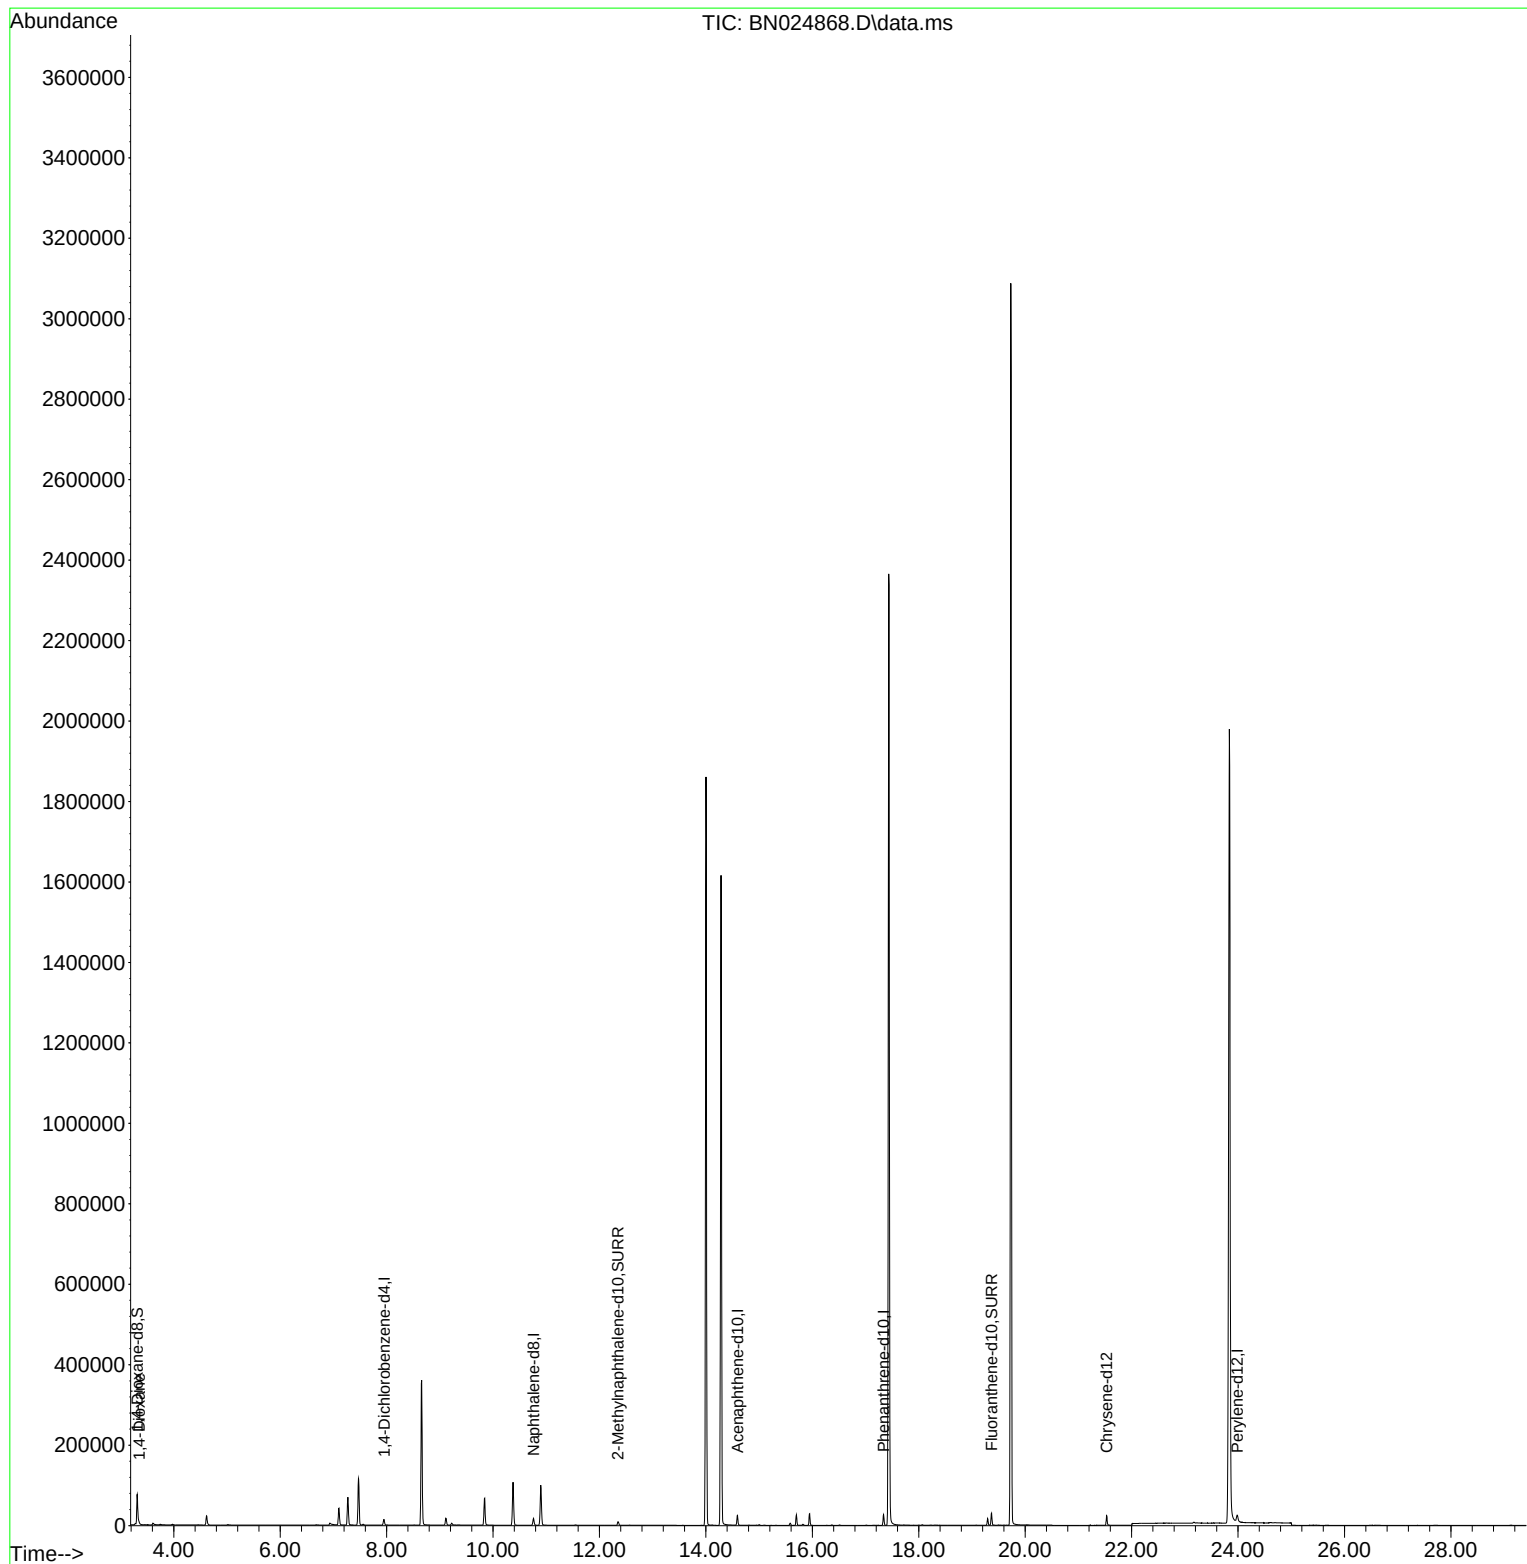

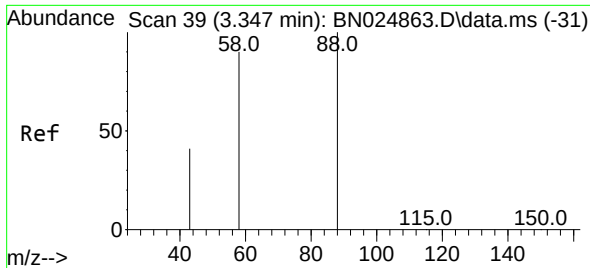

#2

1,4-Dioxane

Concen: 0.090 ng/ul

RT: 3.352 min Scan# 40

Delta R.T. 0.000 min

Lab File: BN024868.D


Acq: 13 Apr 2023 19:41

Instrument :

BNA_N

ClientSampleId :

BHDZ7

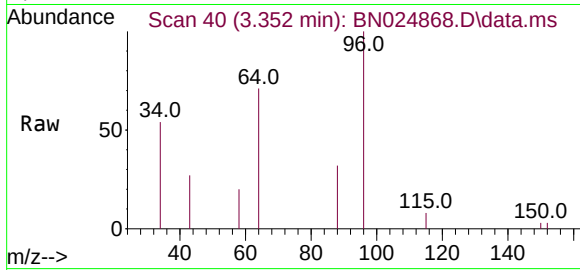

Tgt Ion: 88 Resp: 784

Ion Ratio Lower Upper

88 100

43 85.9 39.1 58.7#

58 61.8 65.7 98.5#

