

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
 Data File : BN024869.D
 Acq On : 13 Apr 2023 20:19
 Operator : CG/JU
 Sample : 02275-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ8

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 04/14/2023
 Supervised By : Jagrut Upadhyay 04/14/2023

Quant Time: Apr 14 02:21:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 13 02:44:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	7574	0.400	ng/u1	0.00
4) Naphthalene-d8	10.763	136	23131	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.592	164	13791	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.337	188	30544	0.400	ng/u1	0.00
17) Chrysene-d12	21.531	240	25052	0.400	ng/u1	0.00
23) Perylene-d12	23.977	264	26965	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.309	96	69148m	8.360	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.347	152	13088	0.441	ng/u1	0.00
18) Fluoranthene-d10	19.367	212	34981	0.562	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.347	88	30173	3.311	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041323\
Data File : BN024869.D
Acq On : 13 Apr 2023 20:19
Operator : CG/JU
Sample : 02275-13
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BHDZ8

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 04/14/2023
Supervised By : Jagrut Upadhyay 04/14/2023


Quant Time: Apr 14 02:21:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN040723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 13 02:44:00 2023
Response via : Initial Calibration

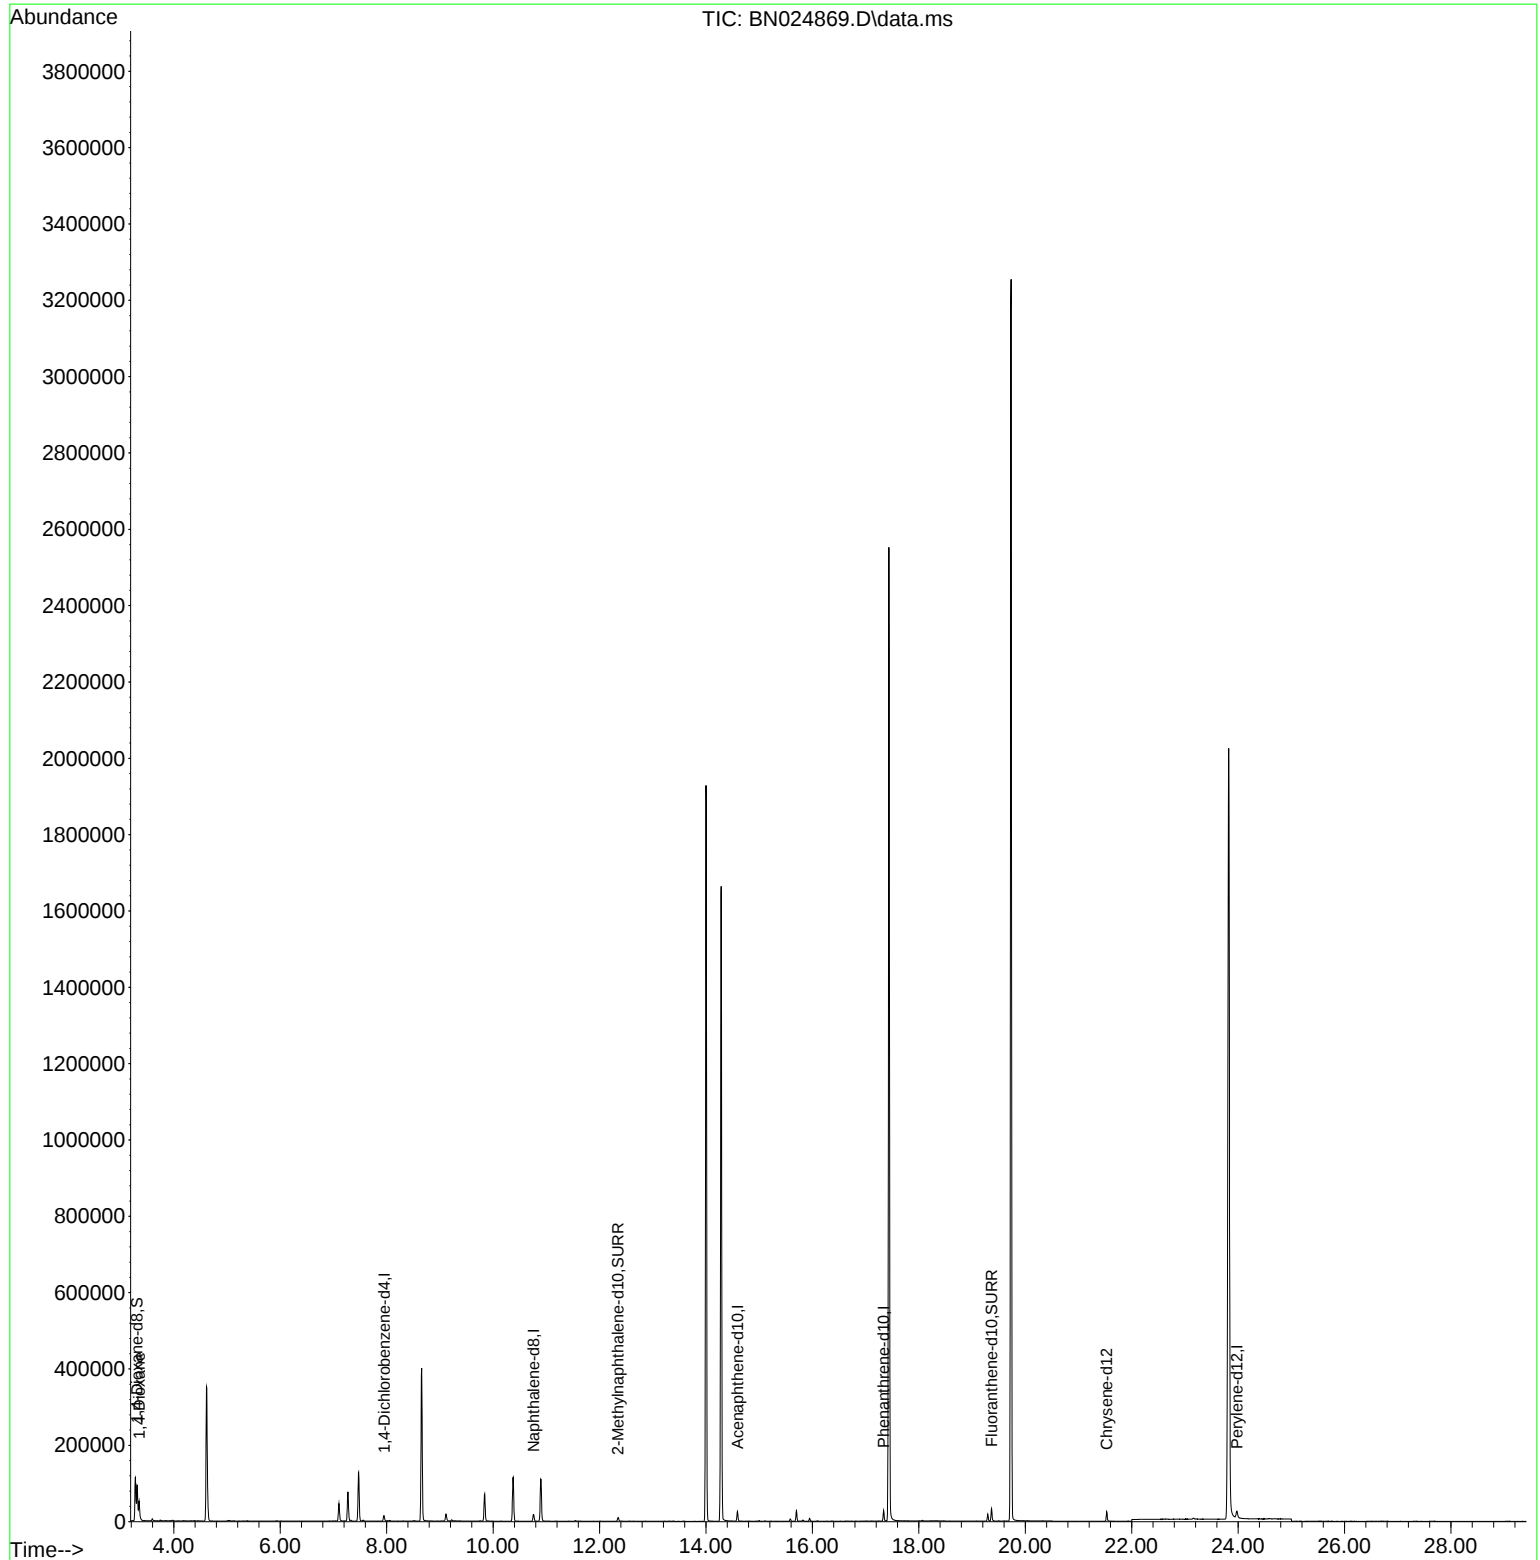

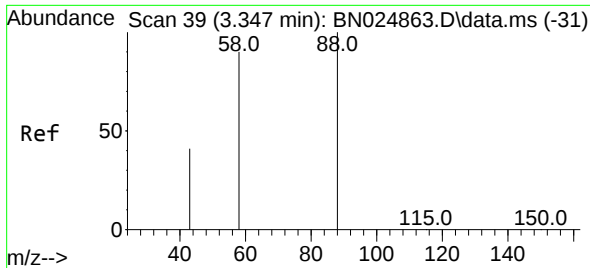

#2
 1,4-Dioxane
 Concen: 3.311 ng/ul
 RT: 3.347 min Scan# 39
 Delta R.T. -0.004 min
 Lab File: BN024869.D
 Acq: 13 Apr 2023 20:19

Instrument :
 BNA_N
 ClientSampleId :
 BHDZ8

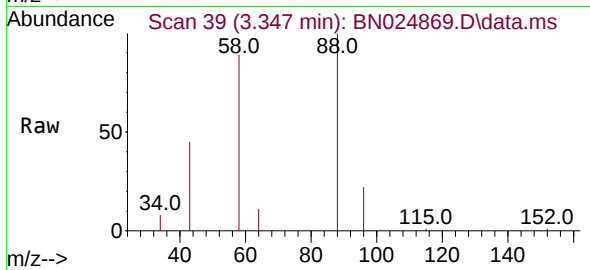

Tgt Ion: 88	Resp: 30173
Ion Ratio	Lower Upper
88	100
43	45.3 39.1 58.7
58	89.1 65.7 98.5

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 04/14/2023
 Supervised By :Jagrut Upadhyay 04/14/2023

