

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
 Data File : BN030878.D
 Acq On : 13 Apr 2024 13:29
 Operator : MA/JU
 Sample : PB160170BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK170

Quant Time: Apr 14 22:16:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 14 22:12:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	146590	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	661090	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.310	164	439667	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.057	188	983296	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	1091626	20.000	ng/ul	0.00
88) Perylene-d12	24.221	264	1208696	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	23259	7.439	ng/uL	0.00
4) Pyridine-d5	3.581	84	342851	36.573	ng/ul	0.00
7) Phenol-d5	6.834	99	431823	36.415	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.005	67	262898	35.894	ng/ul	0.00
11) 2-Chlorophenol-d4	7.199	132	343062	38.136	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	347220	34.937	ng/ul	0.00
21) Nitrobenzene-d5	8.822	128	173242	37.777	ng/ul	0.00
24) 2-Nitrophenol-d4	9.540	143	173201	41.285	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.069	165	333304	36.290	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131	560287	37.055	ng/ul	0.00
46) Dimethylphthalate-d6	13.728	166	1141414	38.884	ng/ul	0.00
49) Acenaphthylene-d8	13.998	160	1268048	37.571	ng/ul	0.00
54) 4-Nitrophenol-d4	14.516	143	204806	36.475	ng/ul	0.00
60) Fluorene-d10	15.304	176	991760	38.608	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.428	200	125867	29.000	ng/ul	0.00
73) Anthracene-d10	17.157	188	1646792	38.870	ng/ul	0.00
81) Pyrene-d10	19.463	212	2075268	35.360	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.021	264	2235107	40.132	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.369	70	8312	1.052 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN041324\
Data File : BN030878.D
Acq On : 13 Apr 2024 13:29
Operator : MA/JU
Sample : PB160170BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK170


Quant Time: Apr 14 22:16:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 14 22:12:55 2024
Response via : Initial Calibration

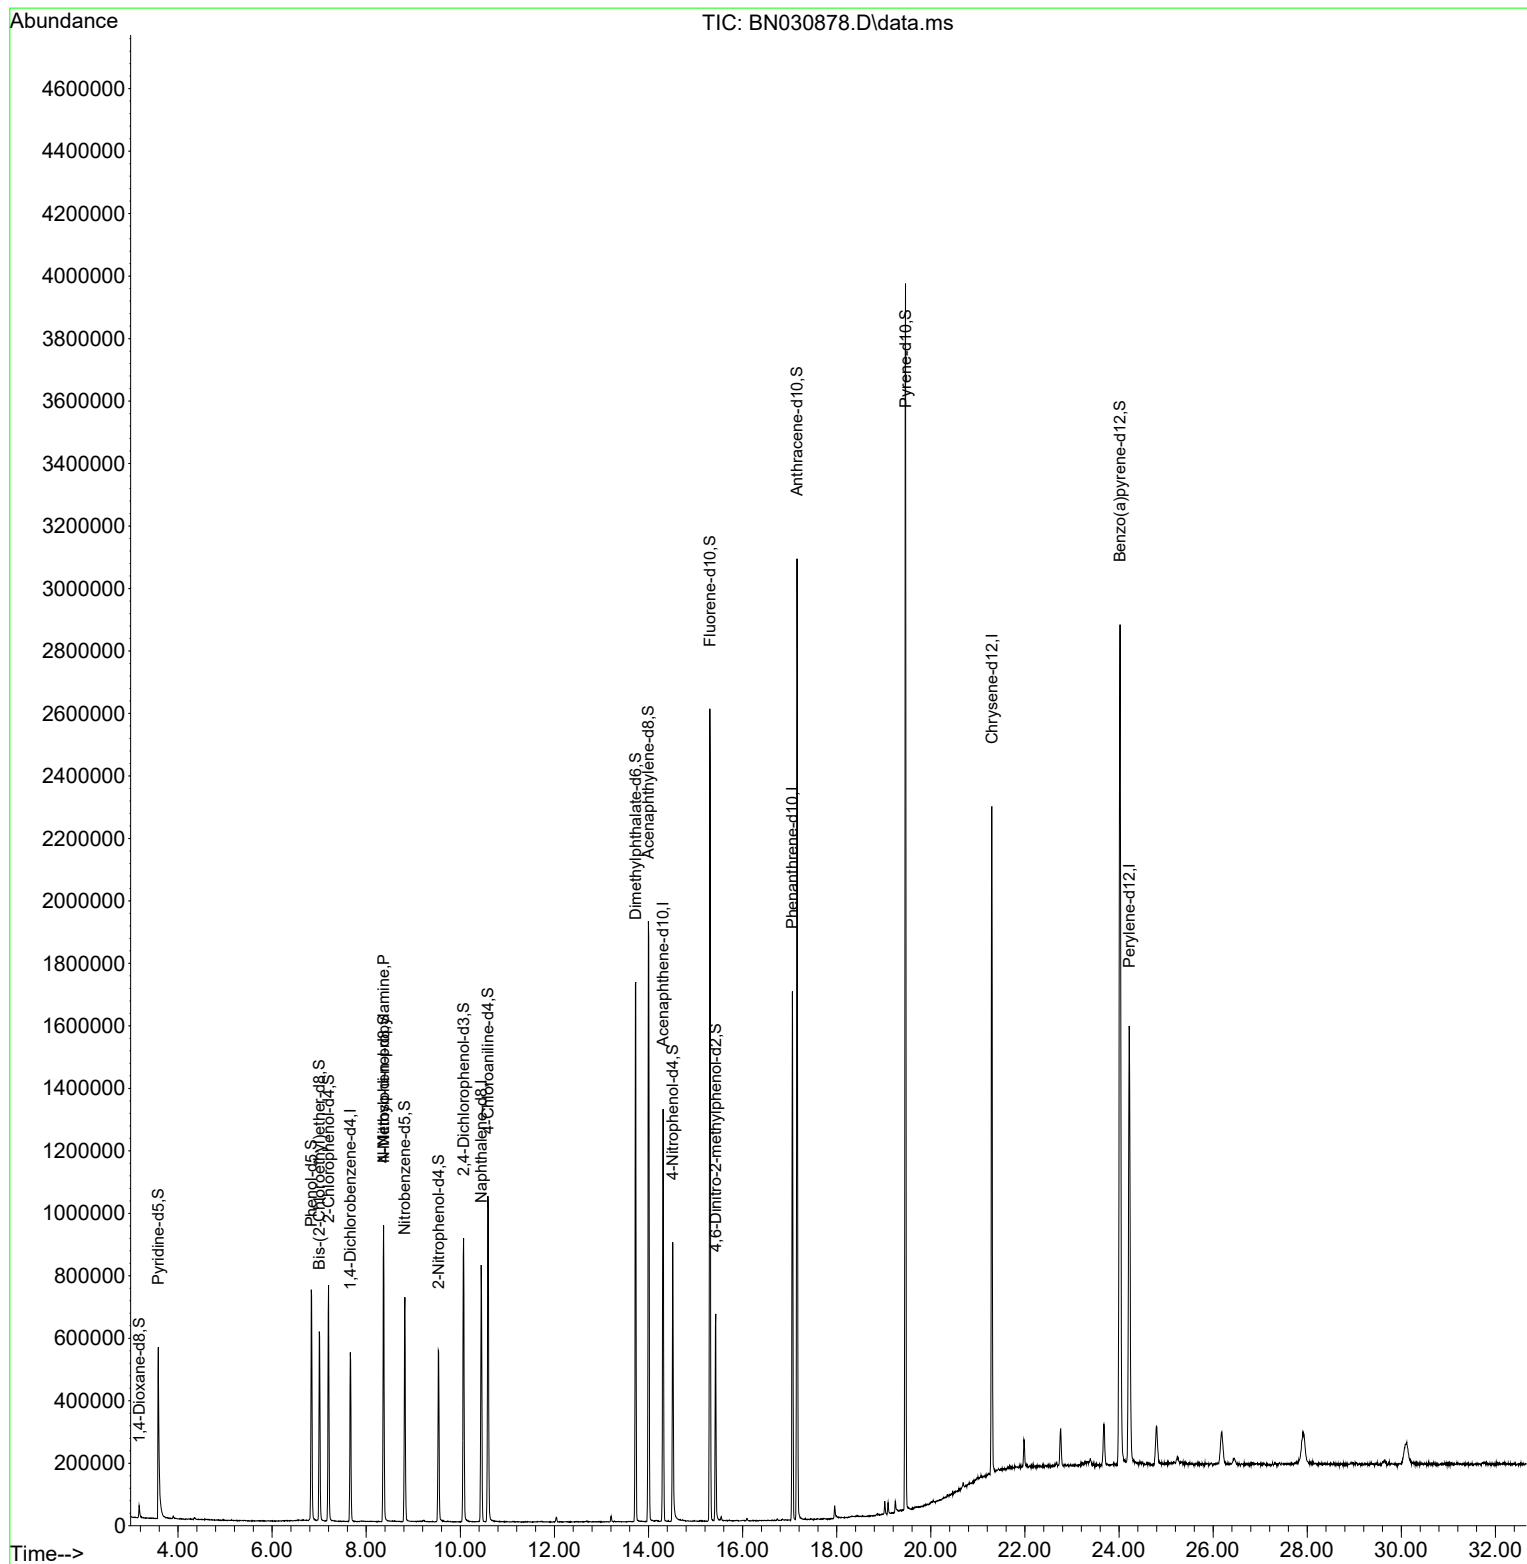

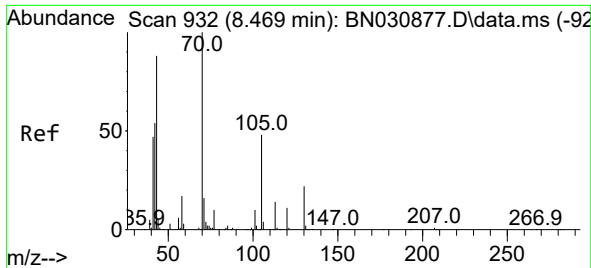

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.052 ng/ul
 RT: 8.369 min Scan# 91
 Delta R.T. -0.100 min
 Lab File: BN030878.D
 Acq: 13 Apr 2024 13:29

Instrument :
 BNA_N
 ClientSampleId :
 SBLK170

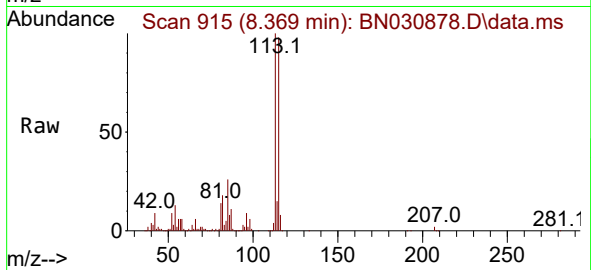

Tgt Ion: 70 Resp: 8312

Ion	Ratio	Lower	Upper
70	100		
42	402.1	47.4	71.0#
101	0.0	7.9	11.9#
130	0.0	19.0	28.4#

